


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032816\
 Data File : BF085794.D
 Acq On : 28 Mar 2016 11:39
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 28 15:27:05 2016

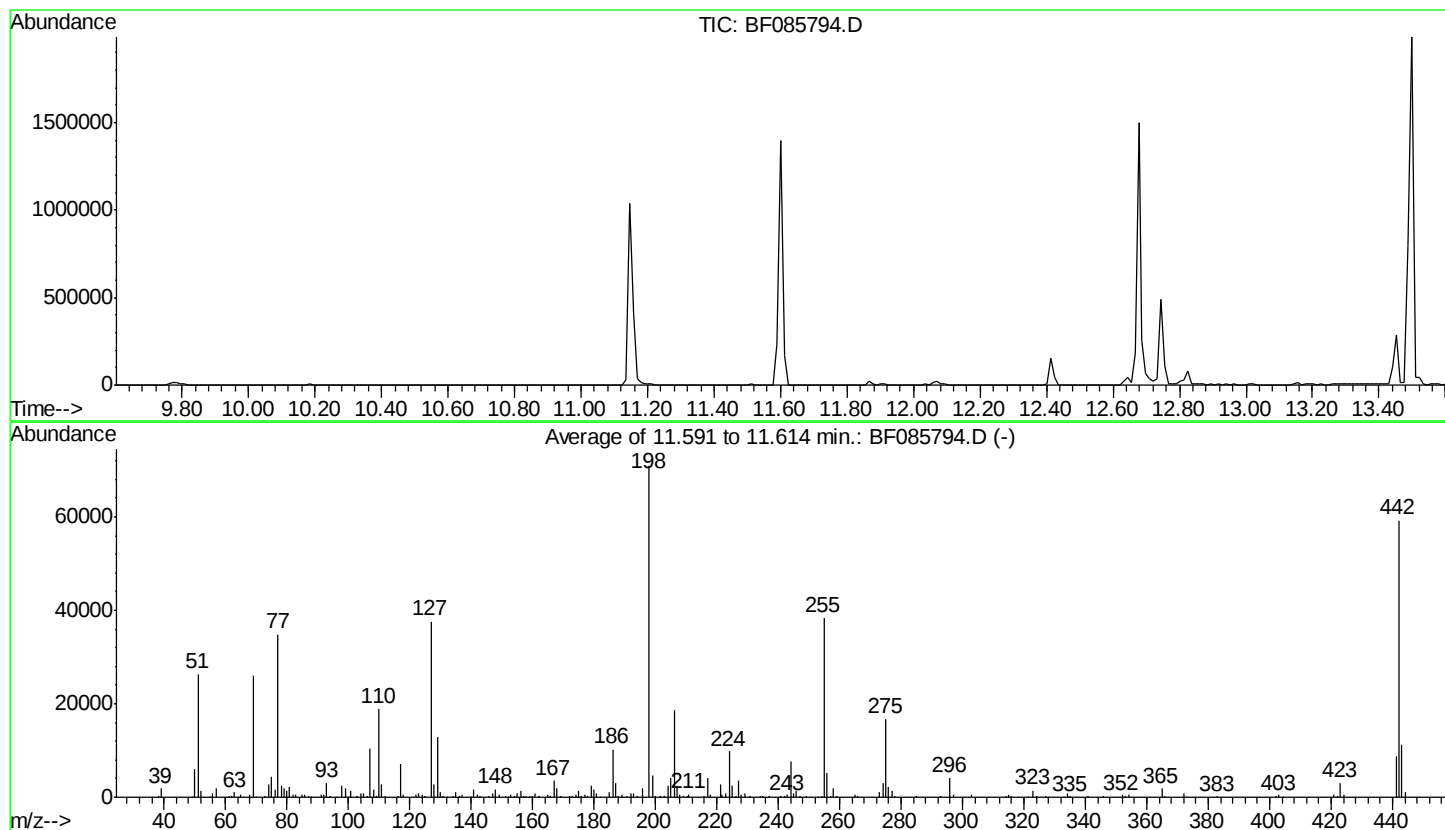

AutoFind: Scans 814, 815, 816; Background Corrected with Scan 811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	26329	PASS
68	69	0.00	2	1.7	443	PASS
69	198	0.00	100	36.6	25990	PASS
70	69	0.00	2	0.5	119	PASS
127	198	10	80	53.1	37650	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70934	PASS
199	198	5	9	6.6	4690	PASS
275	198	10	60	23.7	16836	PASS
365	198	1	100	2.7	1901	PASS
441	442	0.01	24	14.9	8791	PASS
442	198	50	100	83.4	59192	PASS
443	442	15	24	19.2	11372	PASS