


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032816\
 Data File : BF085827.D
 Acq On : 29 Mar 2016 3:21
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 28 15:27:05 2016

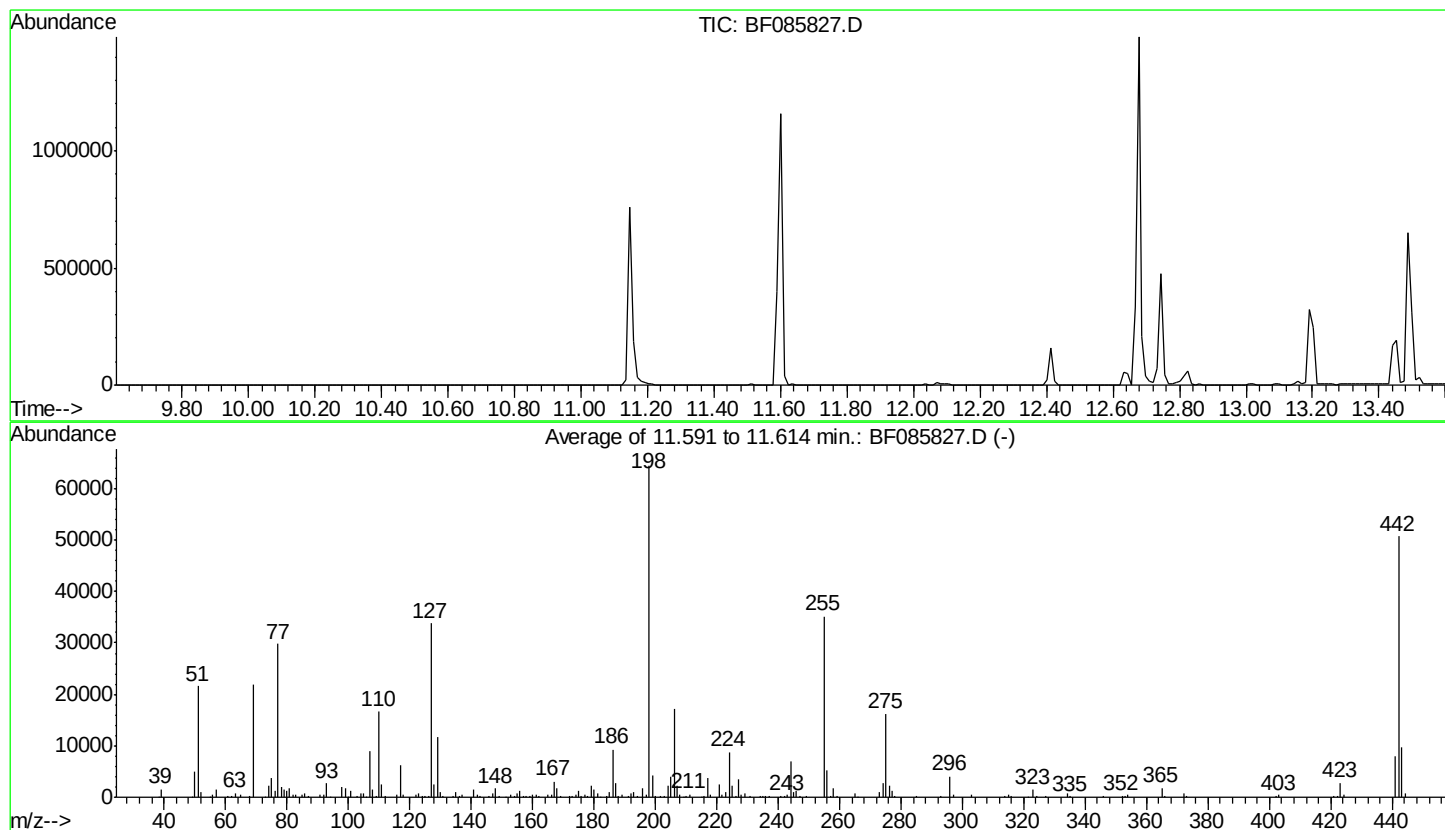

AutoFind: Scans 814, 815, 816; Background Corrected with Scan 811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	21603	PASS
68	69	0.00	2	1.7	366	PASS
69	198	0.00	100	33.8	21797	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.4	33760	PASS
197	198	0.00	2	0.8	485	PASS
198	198	100	100	100.0	64466	PASS
199	198	5	9	6.6	4269	PASS
275	198	10	60	25.2	16225	PASS
365	198	1	100	2.8	1789	PASS
441	442	0.01	24	15.6	7901	PASS
442	198	50	100	78.6	50658	PASS
443	442	15	24	19.1	9654	PASS