
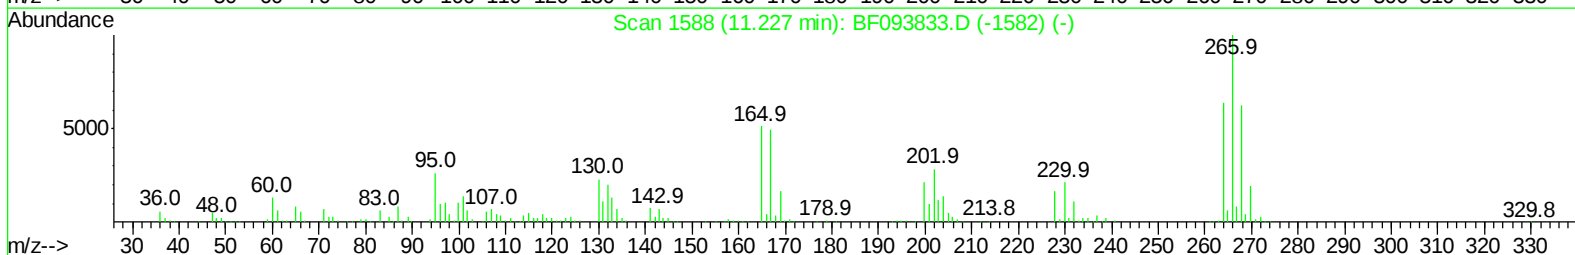
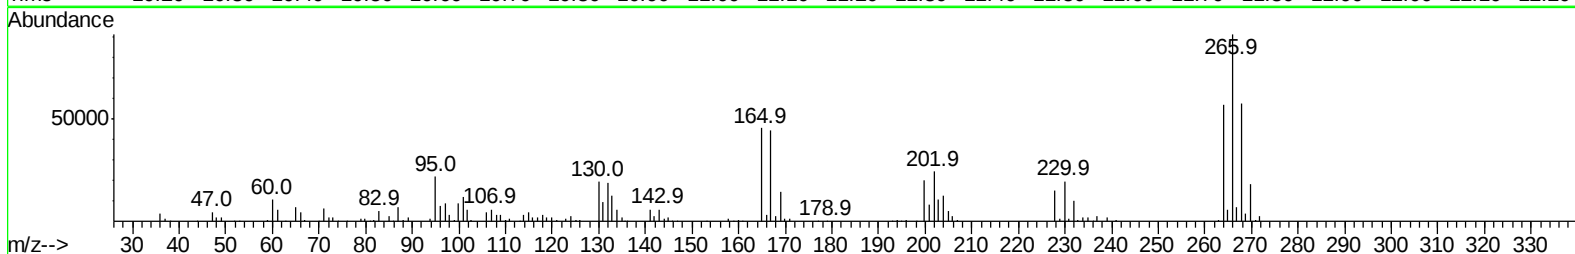


Data Path : Z:\HPCHEM1\BNA F\DATA\BF032817\
Data File : BF093991.D
Acq On : 28 Mar 2017 14:31
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 16:55:27 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 27 16:10:49 2017
Response via : Initial Calibration

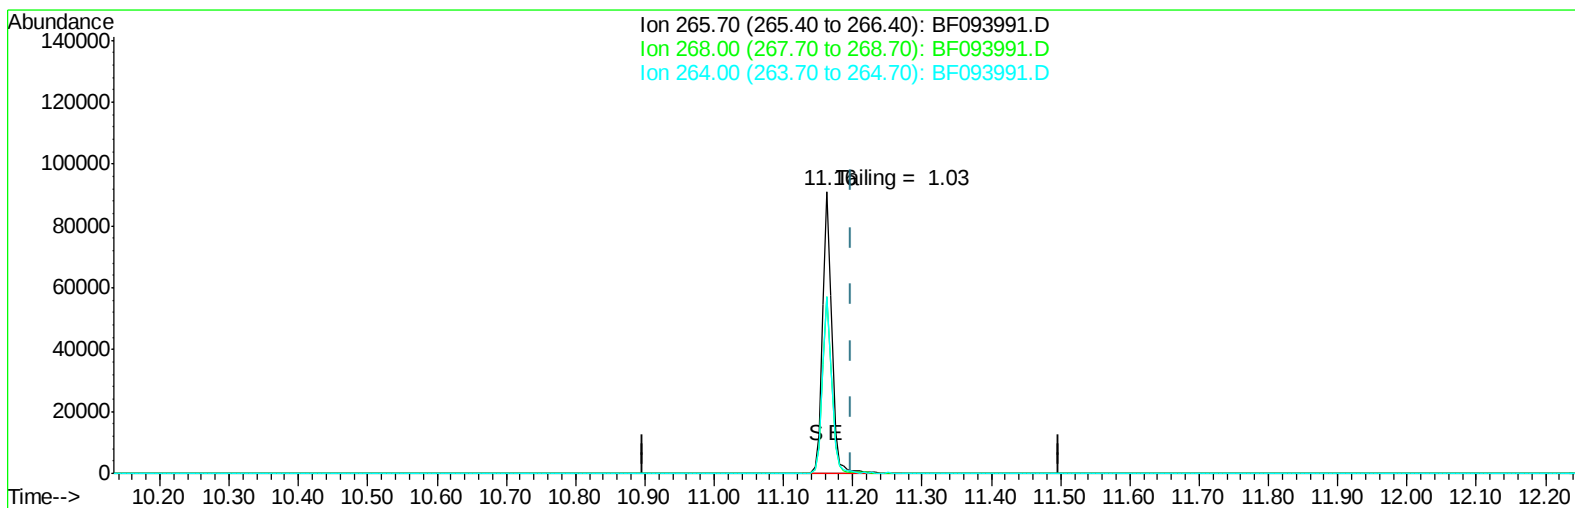

TIC: BF093991.D

(69) Pentachlorophenol (C)




11.163min (-0.035) 0.00ng

response 85621

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.93
264.00	64.60	62.62
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032817\
Data File : BF093991.D
Acq On : 28 Mar 2017 14:31
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 16:55:27 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 27 16:10:49 2017
Response via : Initial Calibration

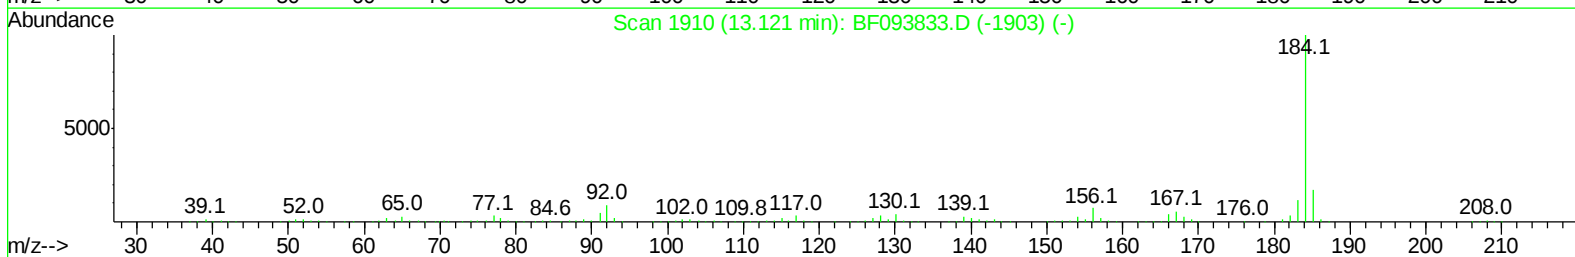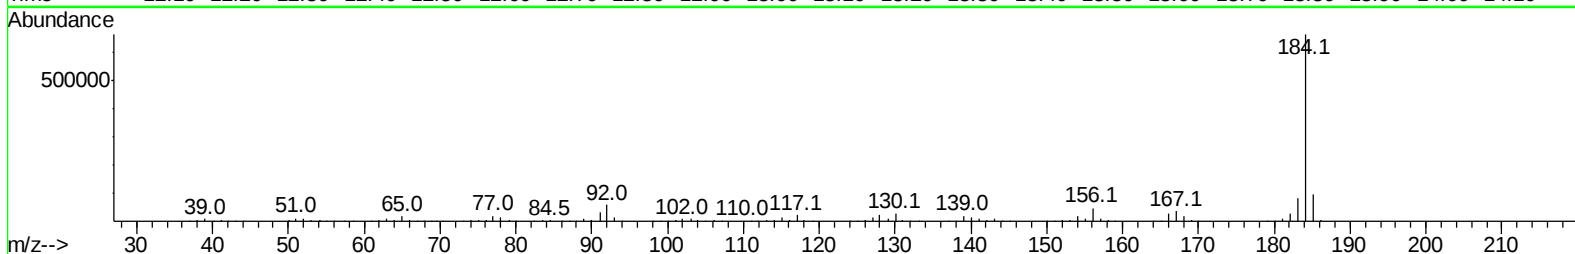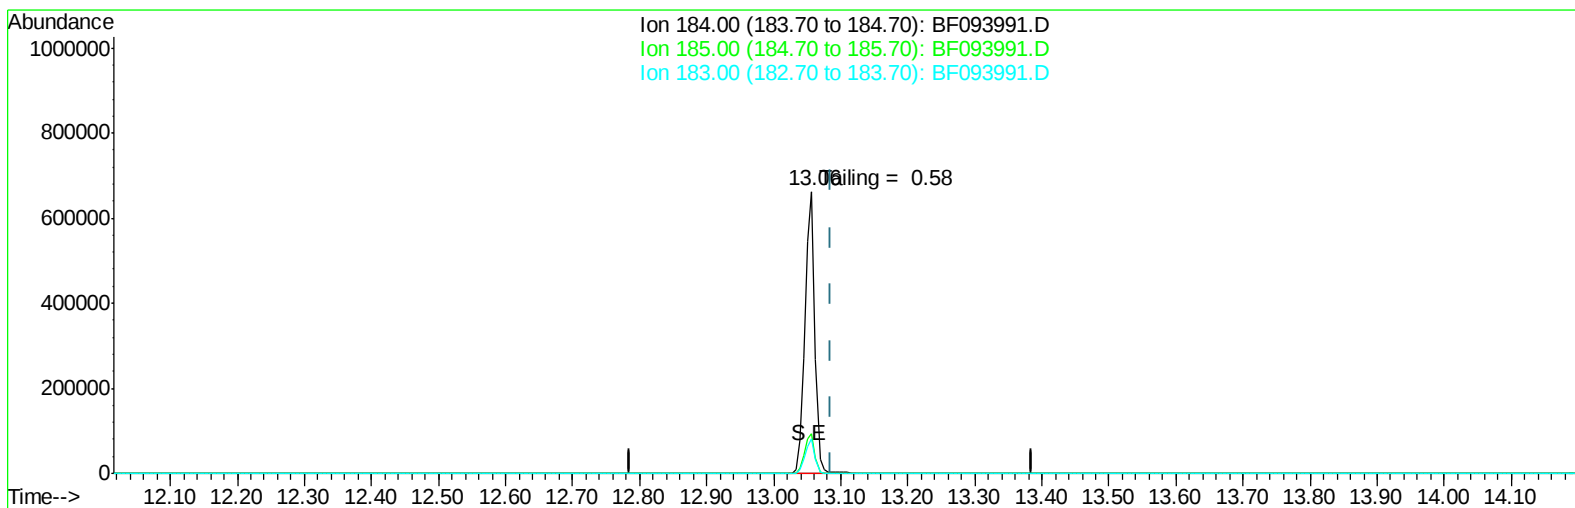

TIC: BF093991.D

(76) Benzidine

13.057min (-0.029) 0.00ng

response 671359

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.14#
183.00	12.20	12.28
0.00	0.00	0.00