


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032817\
 Data File : BF093991.D
 Acq On : 28 Mar 2017 14:31
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 27 16:10:49 2017

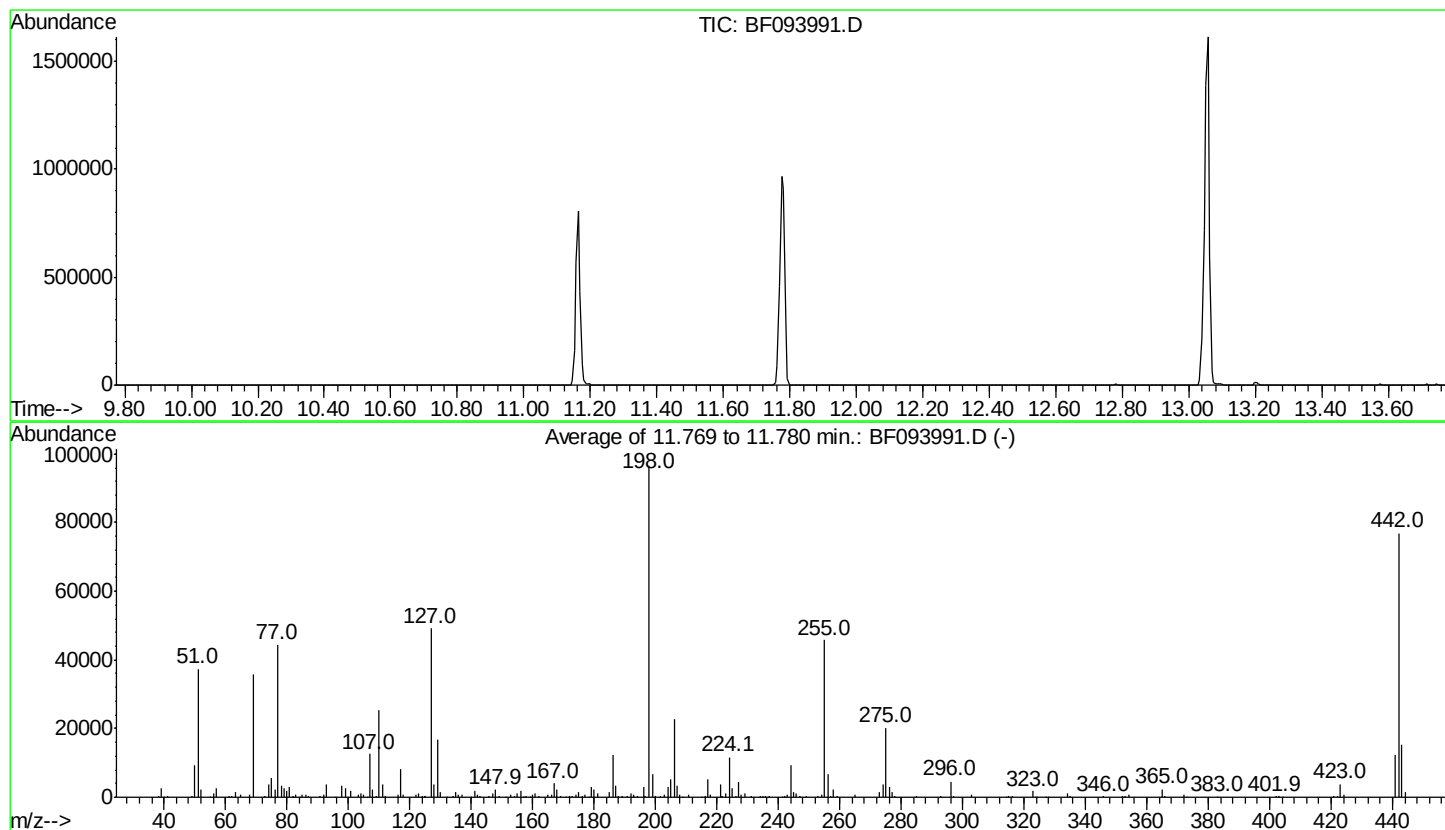

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1675

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	37405	PASS
68	69	0.00	2	2.0	699	PASS
69	198	0.00	100	36.9	35618	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.9	49202	PASS
197	198	0.00	2	0.2	240	PASS
198	198	100	100	100.0	96573	PASS
199	198	5	9	6.8	6595	PASS
275	198	10	60	21.0	20308	PASS
365	198	1	100	2.4	2292	PASS
441	442	0.01	24	15.9	12246	PASS
442	198	50	100	79.7	76973	PASS
443	442	15	24	19.9	15324	PASS