
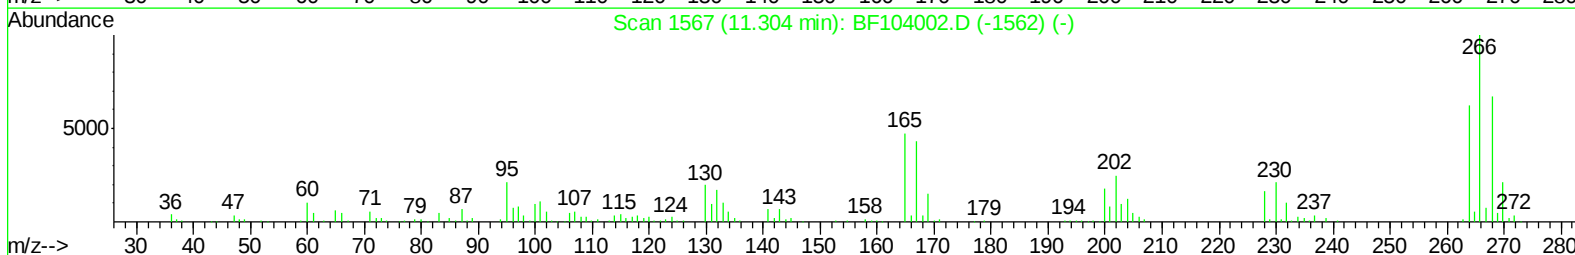
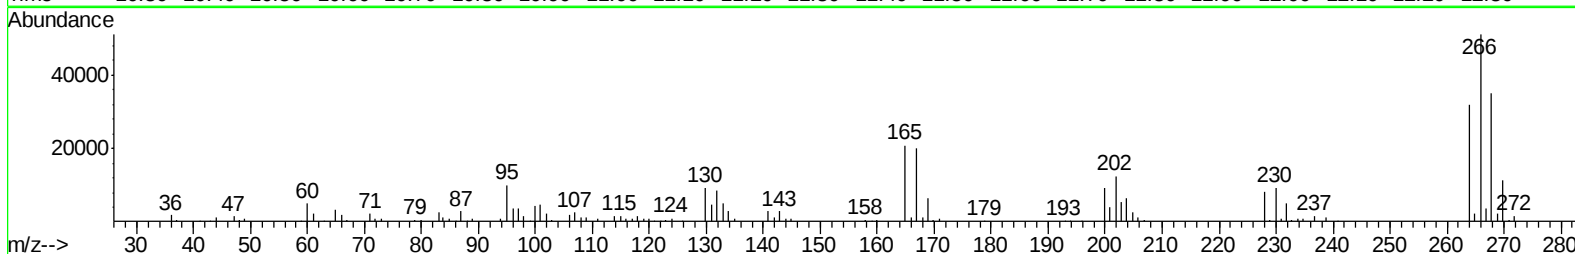


Data Path : Z:\HPCHEM1\BNA F\Data\BF032818\
Data File : BF103998.D
Acq On : 28 Mar 2018 9:43
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 15:07:34 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 13:41:47 2018
Response via : Initial Calibration

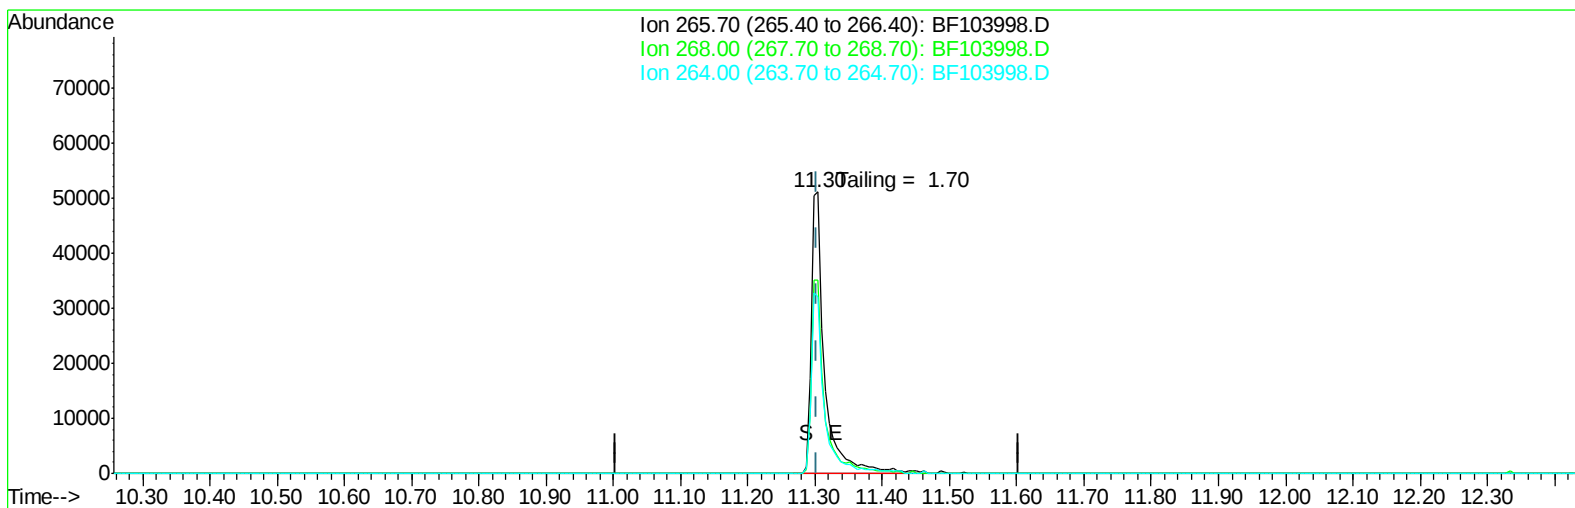

TIC: BF103998.D

(69) Pentachlorophenol (C)




11.304min (-0.000) 79807.04ng

response 71881

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.82
264.00	61.90	62.78
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF032818\
Data File : BF103998.D
Acq On : 28 Mar 2018 9:43
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 15:07:34 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 13:41:47 2018
Response via : Initial Calibration

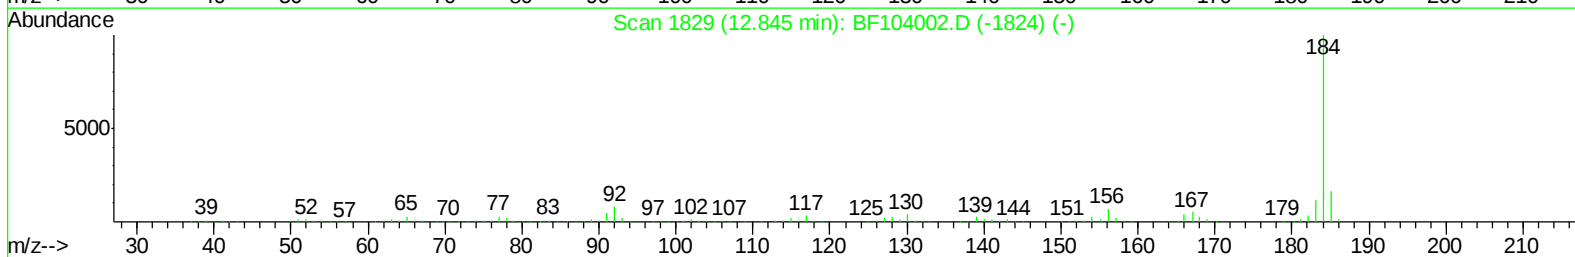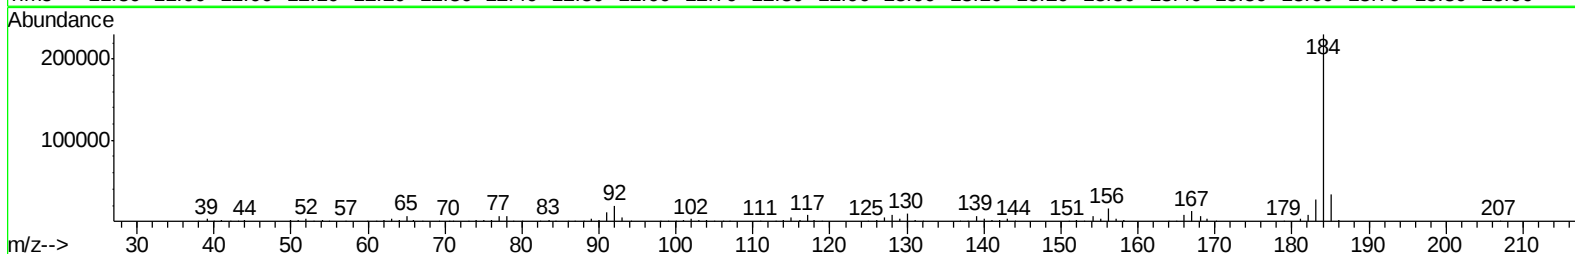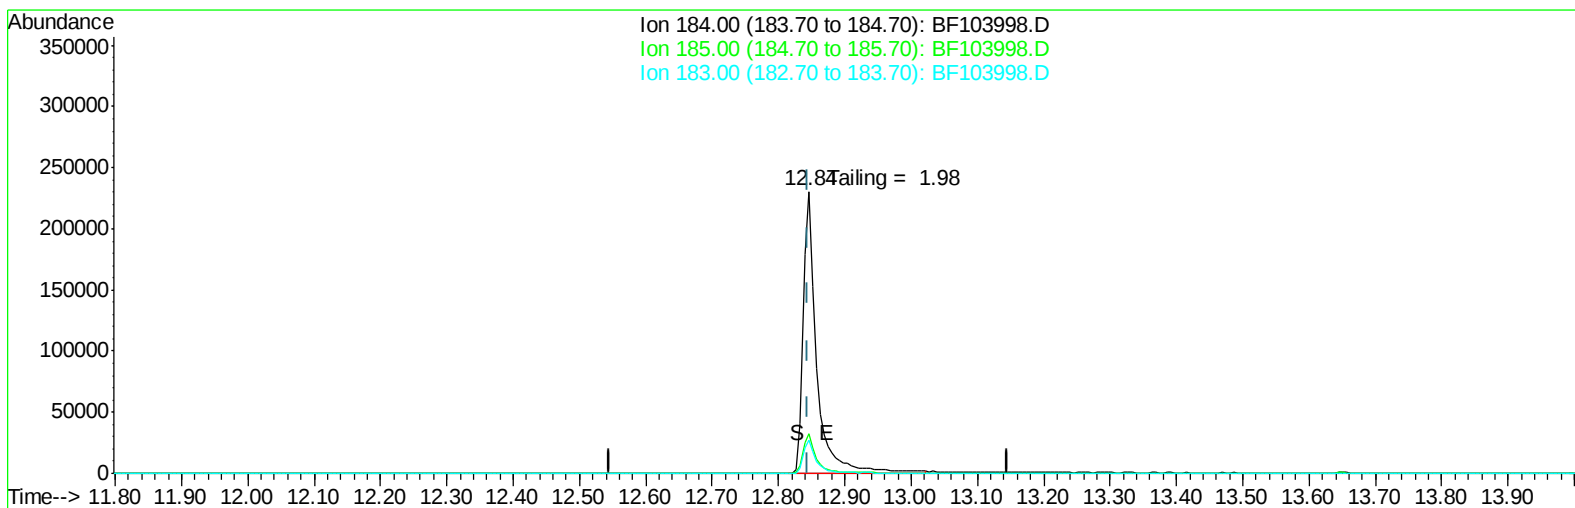

TIC: BF103998.D

(76) Benzidine

12.845min (-0.000) 0.00ng

response 320117

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.33
183.00	11.60	11.90
0.00	0.00	0.00