
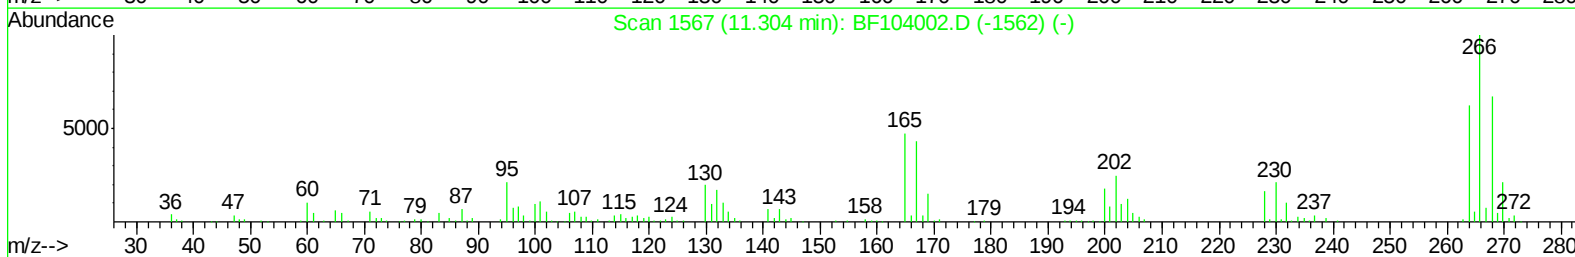
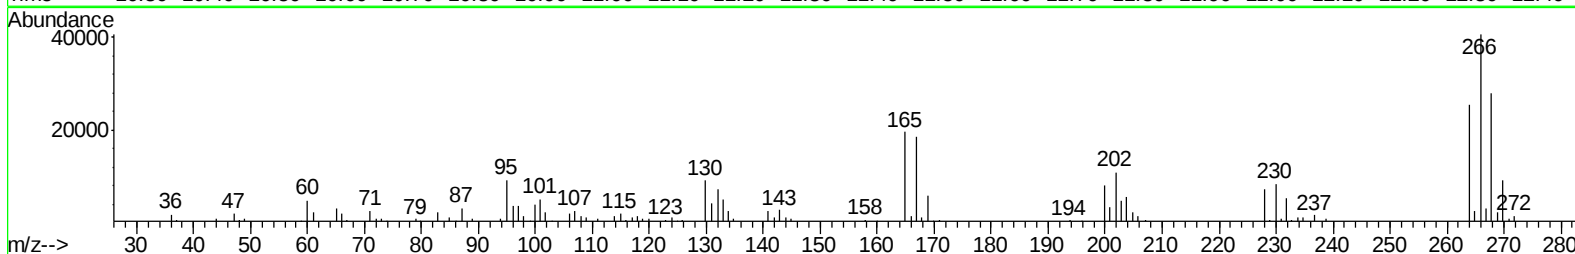


Data Path : Z:\HPCHEM1\BNA F\Data\BF032818\
Data File : BF104007.D
Acq On : 28 Mar 2018 13:59
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 15:09:12 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 13:41:47 2018
Response via : Initial Calibration

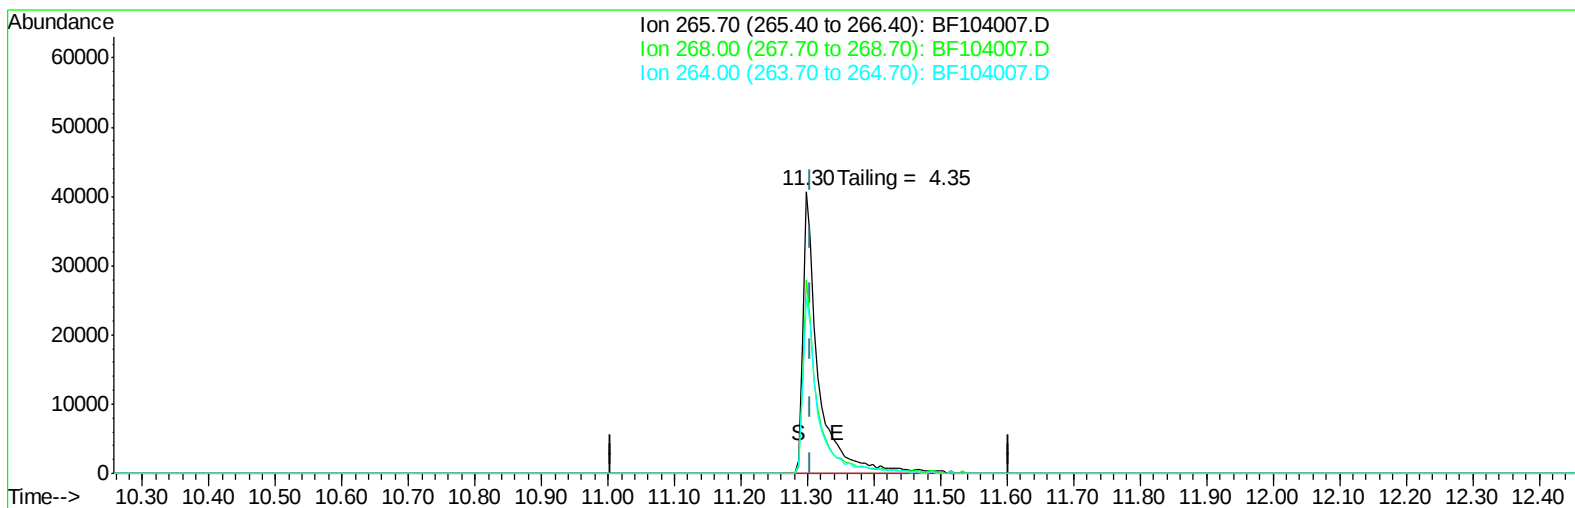

TIC: BF104007.D

(69) Pentachlorophenol (C)




11.298min (-0.006) 0.00ng

response 65628

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.42
264.00	61.90	62.35
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF032818\
Data File : BF104007.D
Acq On : 28 Mar 2018 13:59
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 15:09:12 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 13:41:47 2018
Response via : Initial Calibration

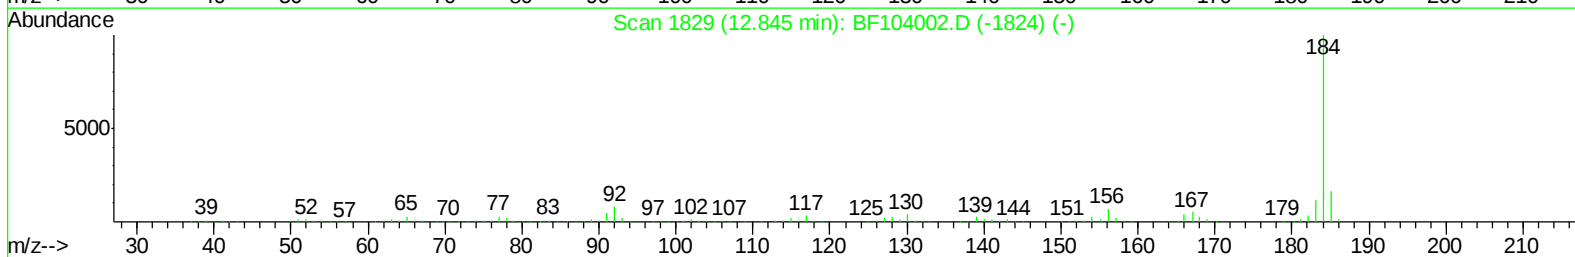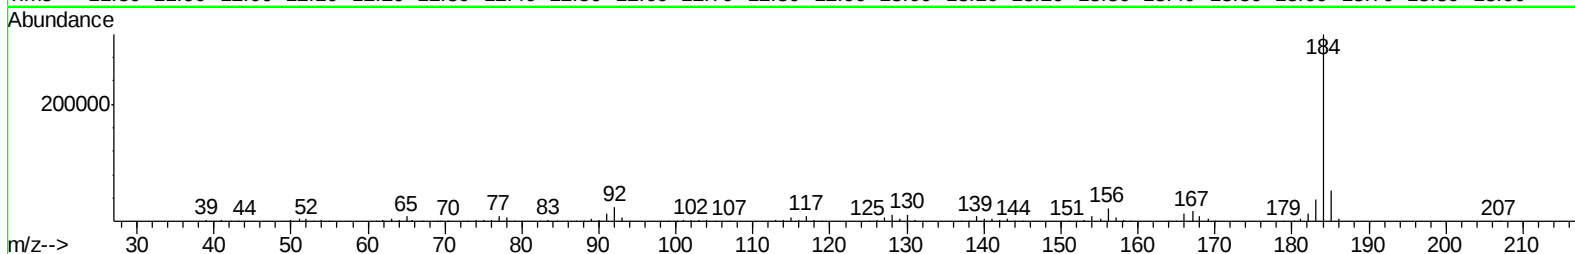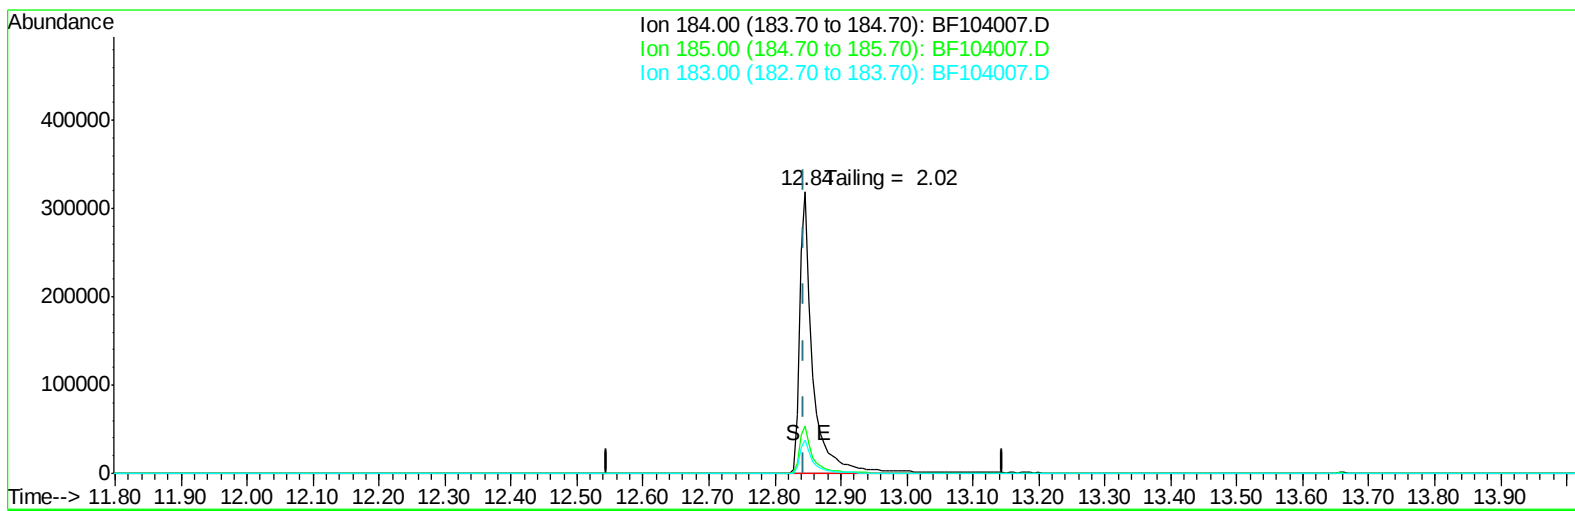

TIC: BF104007.D

(76) Benzidine

12.845min (-0.000) 0.00ng

response 442032

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.72
183.00	11.60	11.82
0.00	0.00	0.00