
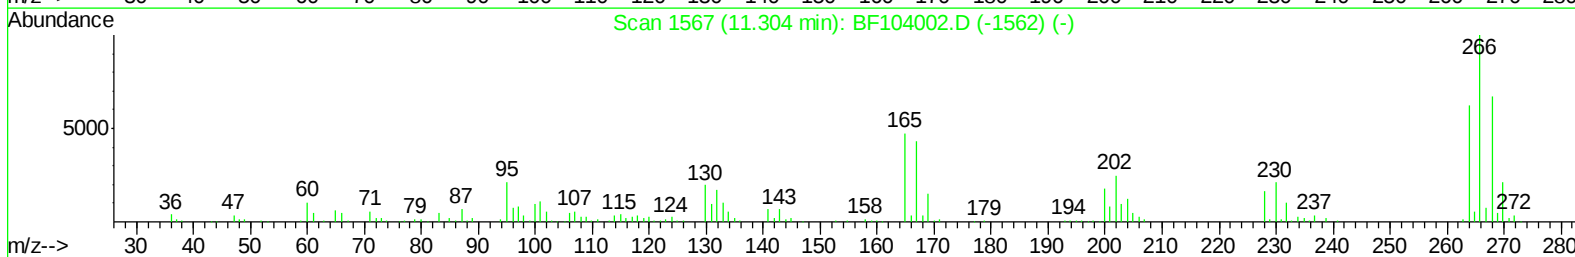
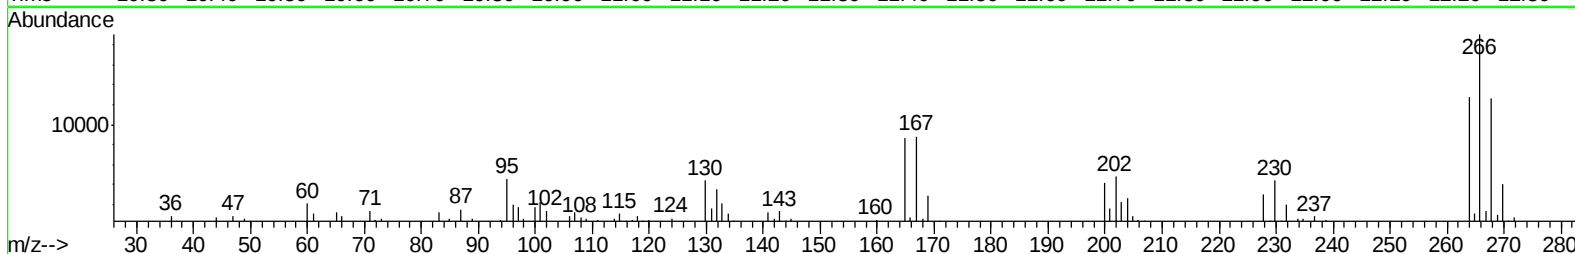


Data Path : Z:\HPCHEM1\BNA F\Data\BF032818\
 Data File : BF104034.D
 Acq On : 29 Mar 2018 2:51
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 15:11:39 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 28 13:41:47 2018
 Response via : Initial Calibration

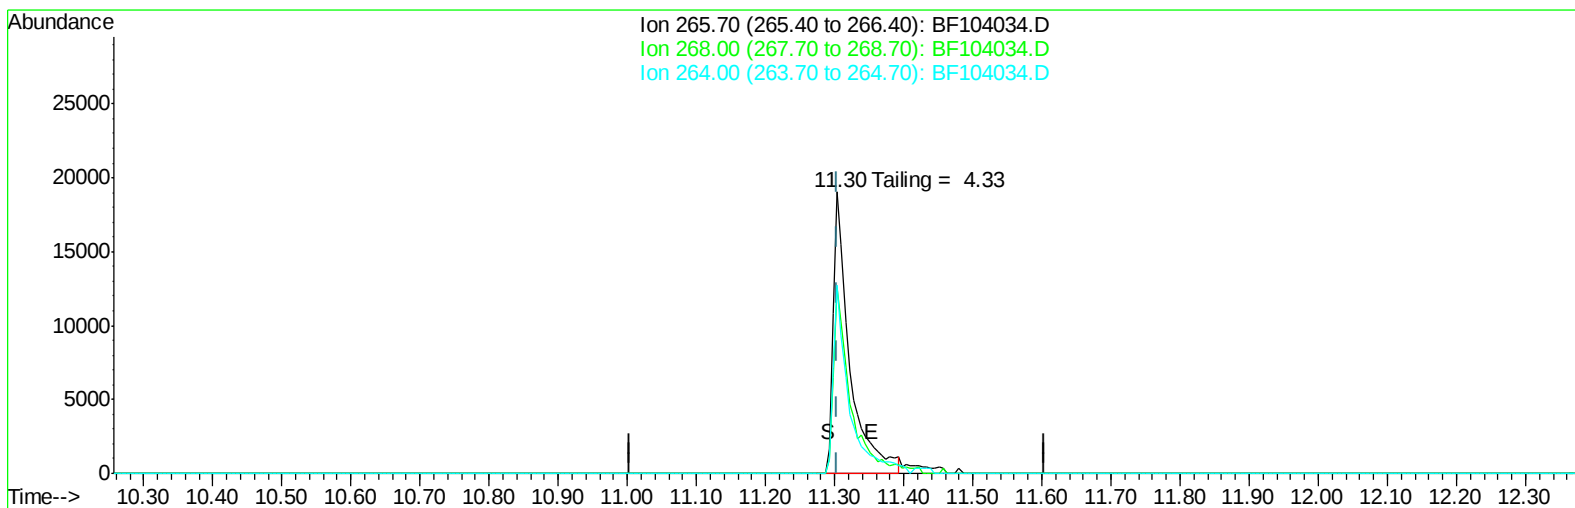

TIC: BF104034.D

(69) Pentachlorophenol (C)




11.304min (-0.000) 29112.14ng

response 30361

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.11
264.00	61.90	66.79
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF032818\
Data File : BF104034.D
Acq On : 29 Mar 2018 2:51
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 15:11:39 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 13:41:47 2018
Response via : Initial Calibration

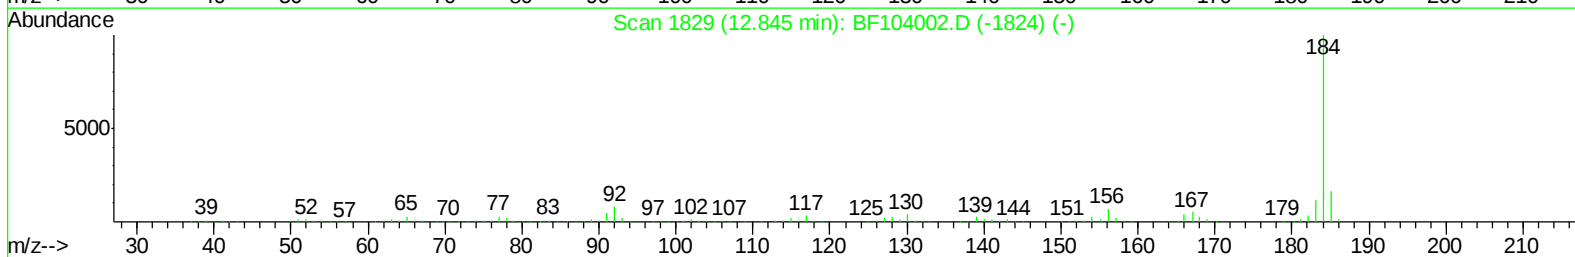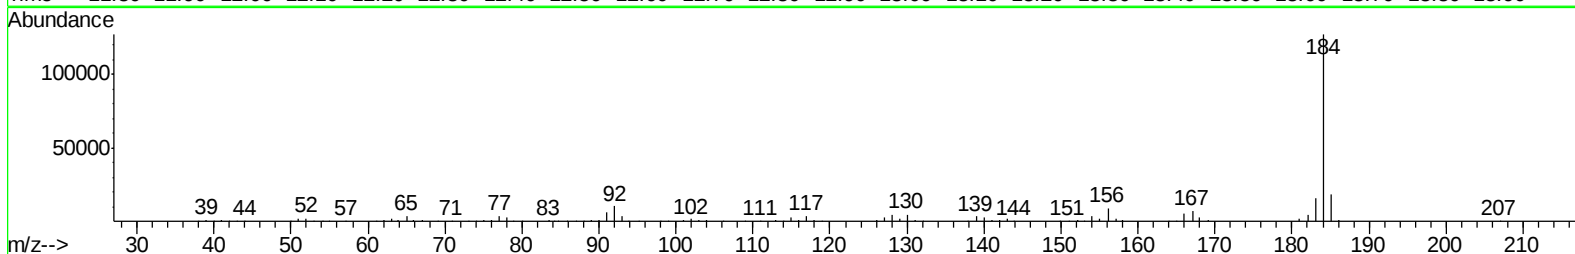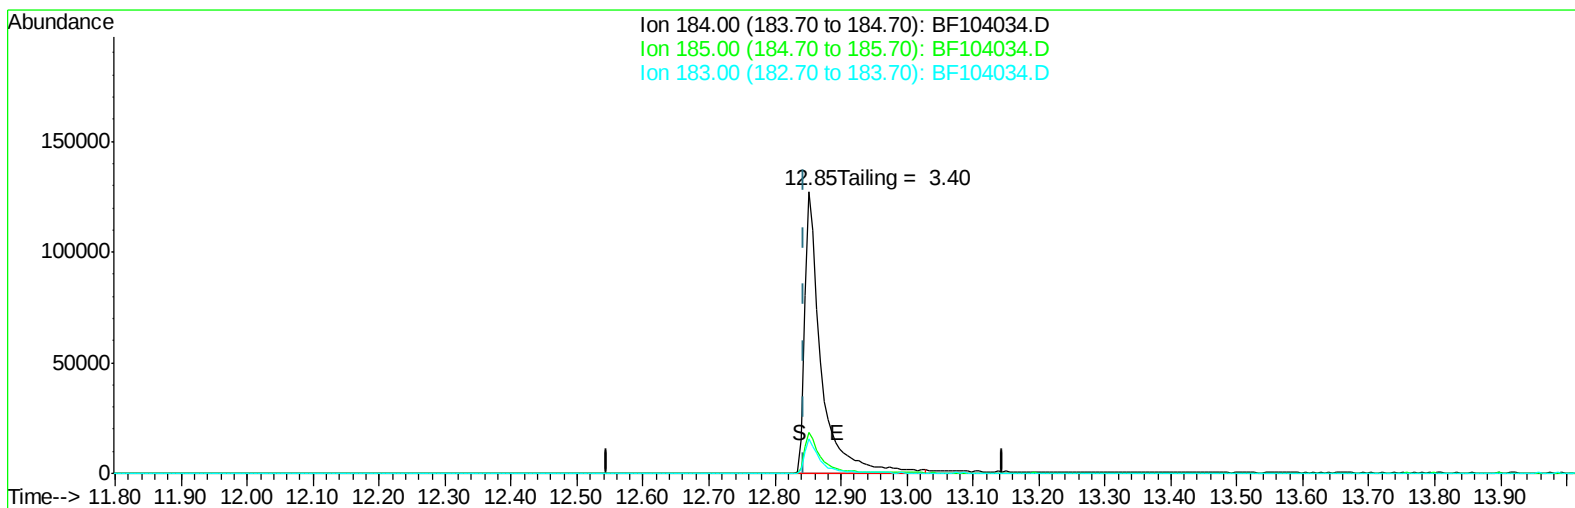

TIC: BF104034.D

(76) Benzidine

12.851min (+0.006) 71294.97ng

response 223491

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.76
183.00	11.60	12.46
0.00	0.00	0.00