


Data Path : U:\HPCHEM1\BNA F\Data\BF032818\
 Data File : BF104034.D
 Acq On : 29 Mar 2018 2:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 30 17:20:53 2018

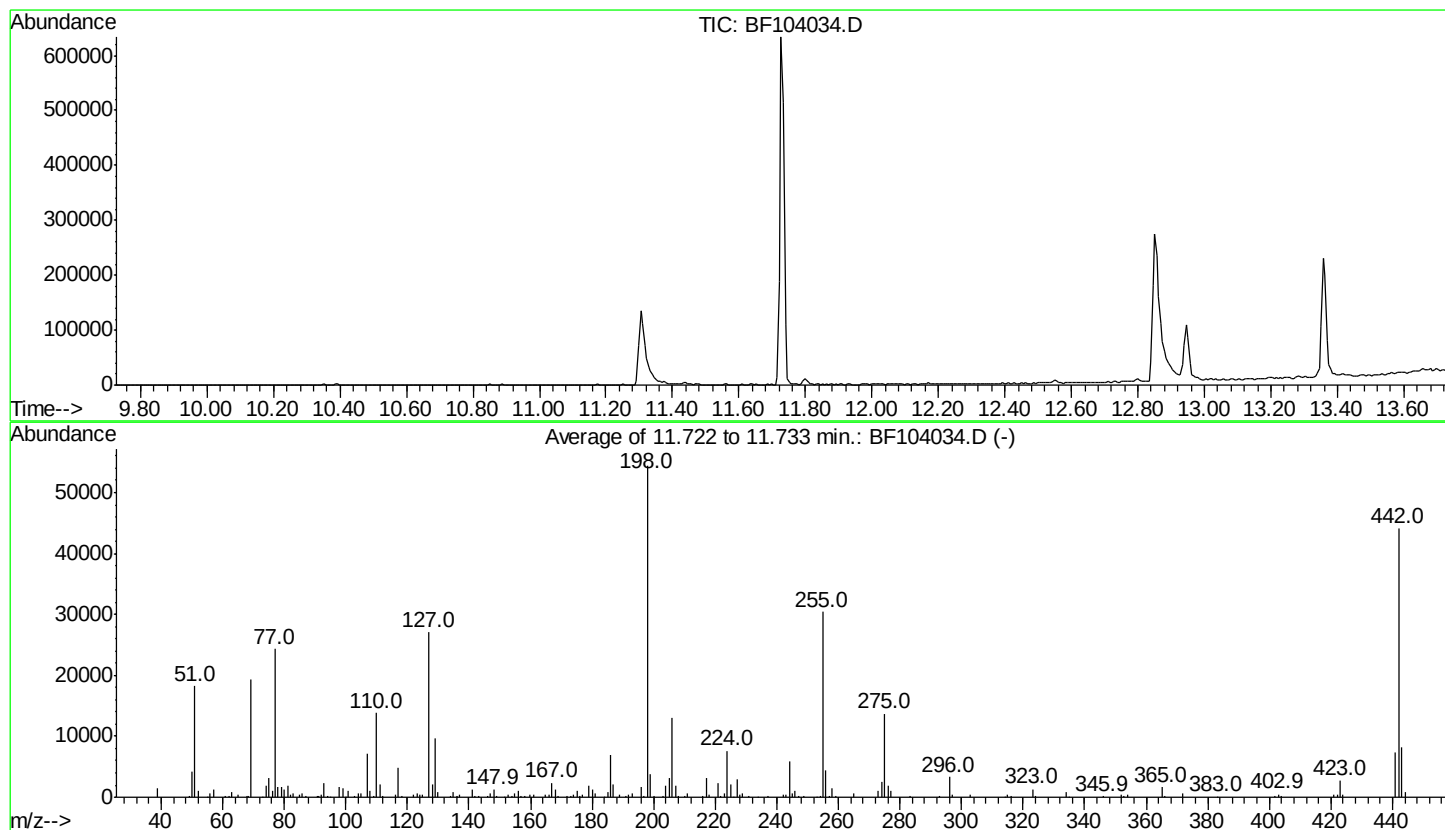

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1634

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	18248	PASS
68	69	0.00	2	1.1	215	PASS
69	198	0.00	100	35.4	19261	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	27057	PASS
197	198	0.00	2	0.4	236	PASS
198	198	100	100	100.0	54418	PASS
199	198	5	9	6.9	3739	PASS
275	198	10	60	25.2	13720	PASS
365	198	1	100	3.0	1634	PASS
441	443	0.01	100	88.9	7328	PASS
442	198	50	100	80.9	44019	PASS
443	442	15	24	18.7	8239	PASS