
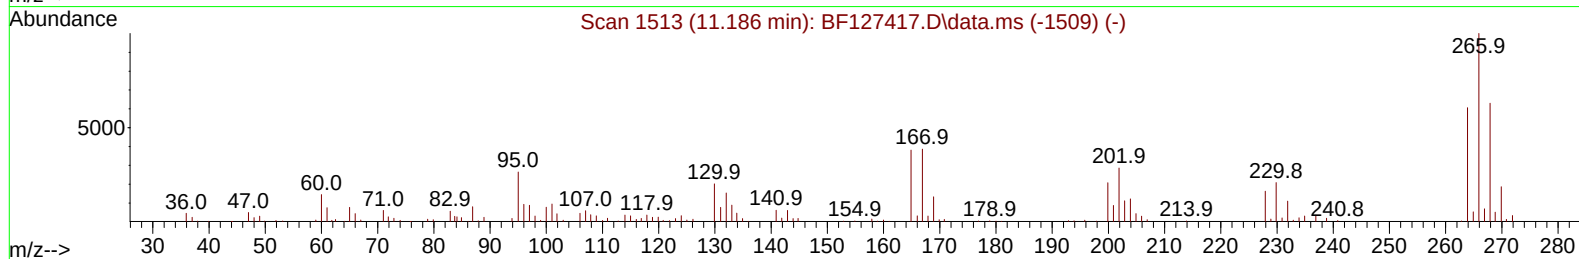
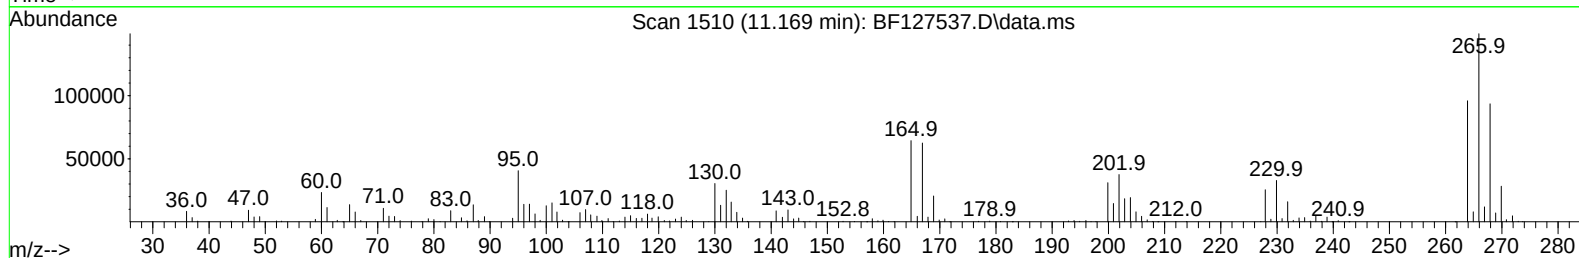


Quant Time: Mar 29 08:33:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 29 07:13:31 2022
Response via : Initial Calibration

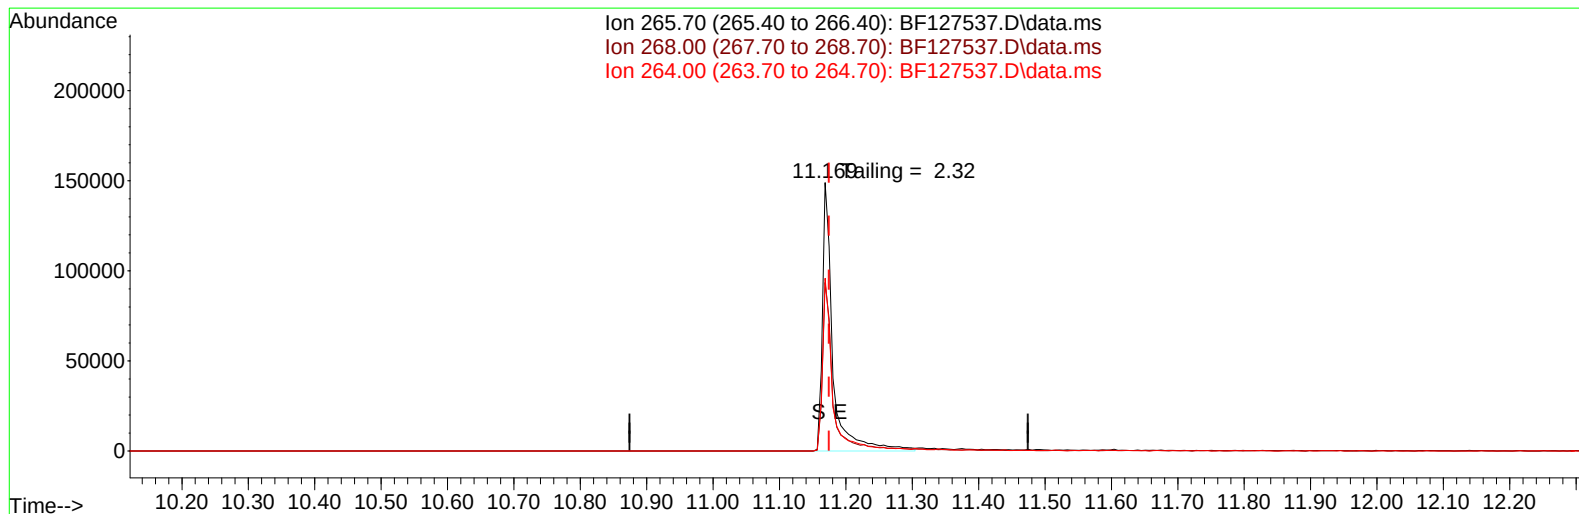

TIC: BF127537.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.006) 41418.78 ng

response	163996
----------	--------

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.78
264.00	60.60	64.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
Data File : BF127537.D
Acq On : 28 Mar 2022 12:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 08:33:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 29 07:13:31 2022
Response via : Initial Calibration

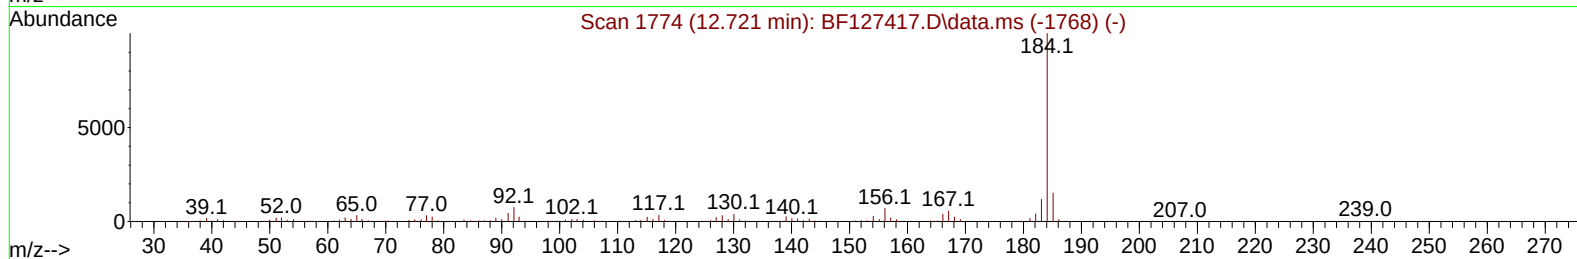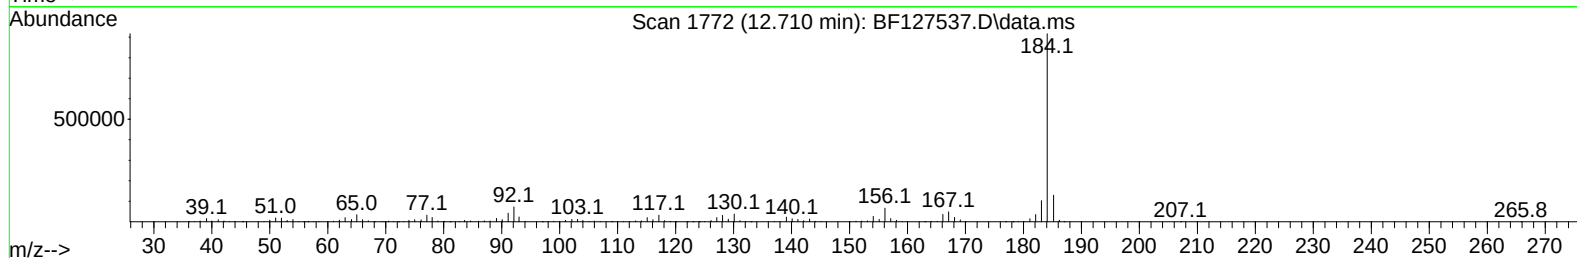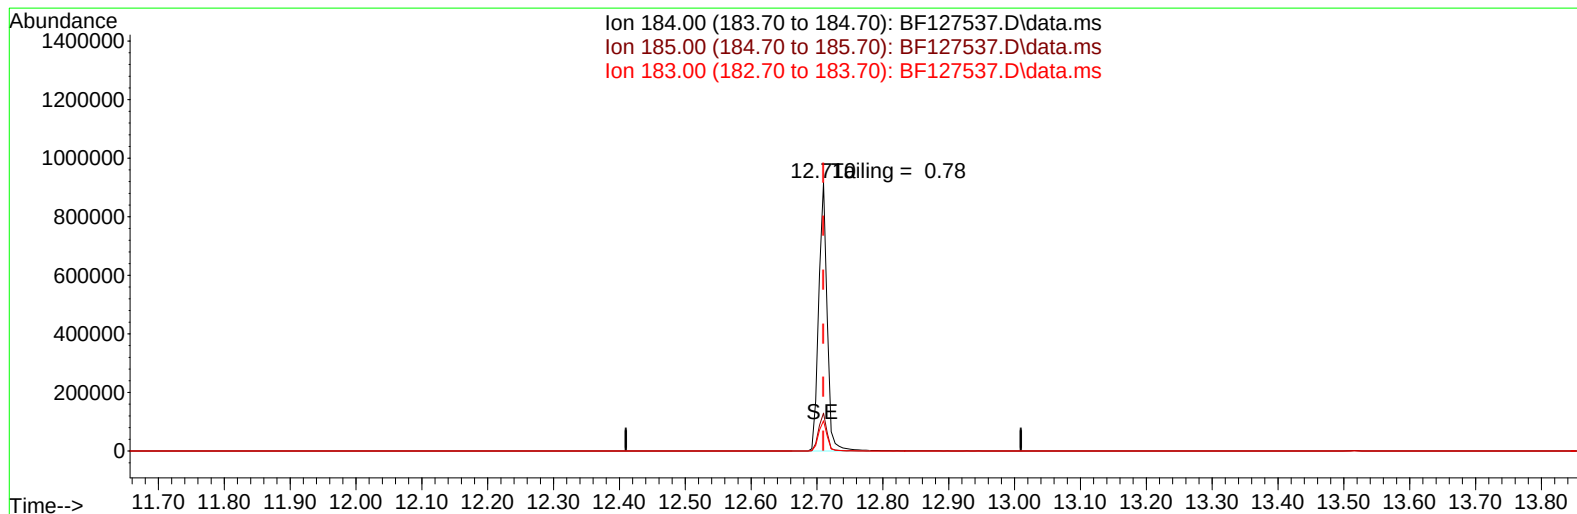

TIC: BF127537.D\data.ms

(77) Benzidine

12.710min (+ 0.000) 66870.32 ng

response 814765

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.12
183.00	11.70	11.30
0.00	0.00	0.00