

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
 Data File : BF127545.D
 Acq On : 28 Mar 2022 16:40
 Operator : CG\JU
 Sample : PB143554TB
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143554TB

Quant Time: Mar 29 07:16:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 29 07:13:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.834	152	107017	20.000	ng	0.00
21) Naphthalene-d8	8.116	136	400821	20.000	ng	0.00
39) Acenaphthene-d10	9.869	164	236316	20.000	ng	0.00
64) Phenanthrene-d10	11.363	188	419987	20.000	ng	0.00
76) Chrysene-d12	14.010	240	288987	20.000	ng	0.00
86) Perylene-d12	15.492	264	212396	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.469	112	844464	125.957	ng	0.01
7) Phenol-d6	6.475	99	1155472	126.083	ng	0.00
23) Nitrobenzene-d5	7.404	82	788370	84.076	ng	0.00
42) 2,4,6-Tribromophenol	10.669	330	303532	120.575	ng	0.00
45) 2-Fluorobiphenyl	9.192	172	1335282	82.509	ng	0.00
79) Terphenyl-d14	12.951	244	1501775	85.071	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
Data File : BF127545.D
Acq On : 28 Mar 2022 16:40
Operator : CG\JU
Sample : PB143554TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143554TB

Quant Time: Mar 29 07:16:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 29 07:13:31 2022
Response via : Initial Calibration




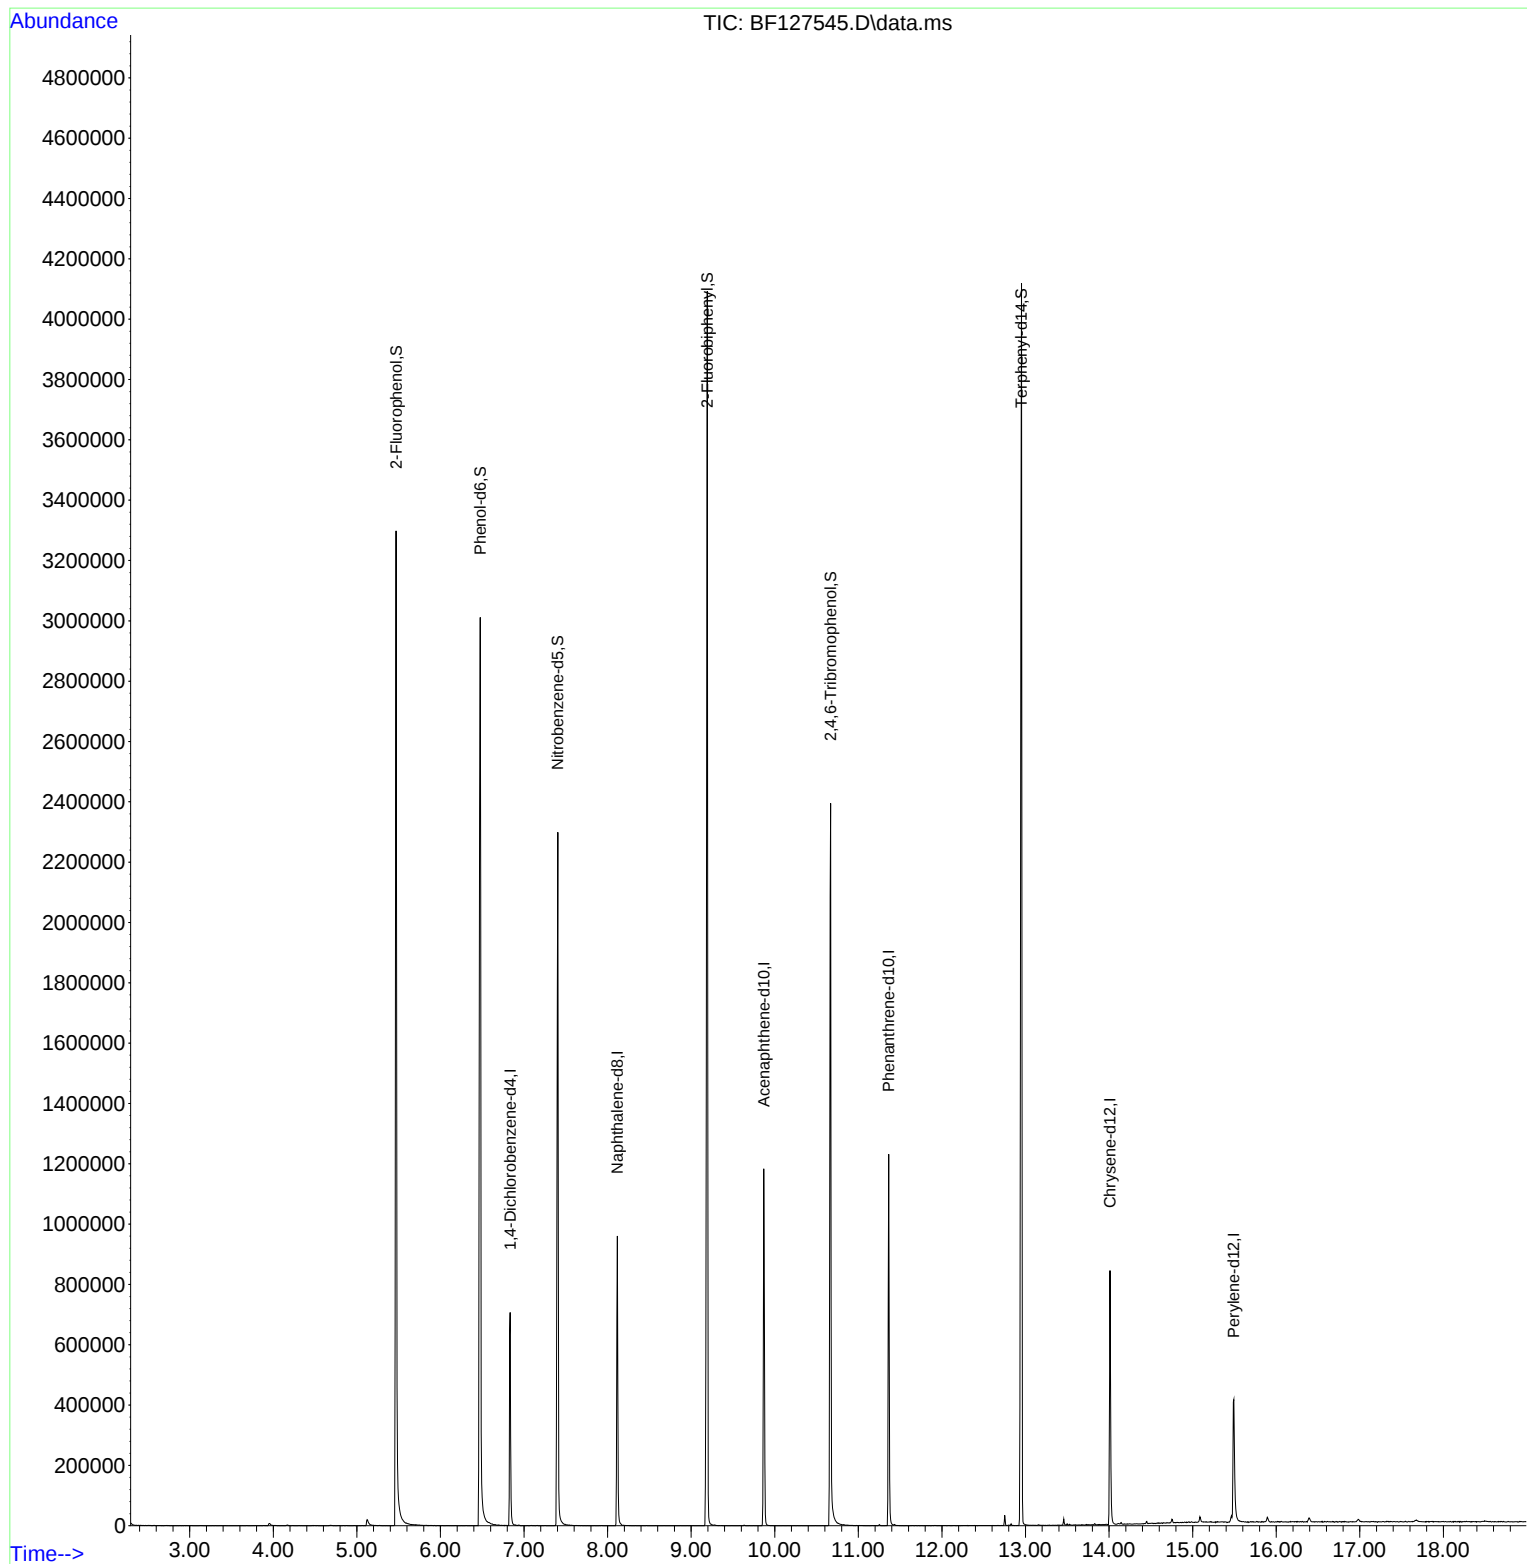




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.834 min Scan# 71
Delta R.T. 0.001 min
Lab File: BF127545.D
Acq: 28 Mar 2022 16:40




Instrument :
BNA_F
ClientSampleId :
PB143554TB


Tgt Ion:152 Resp: 107017
Ion Ratio Lower Upper
152 100
150 147.4 117.2 175.8
115 60.8 49.8 74.6

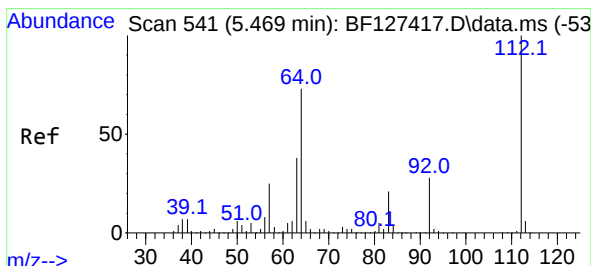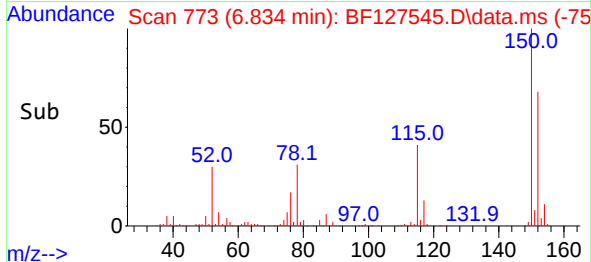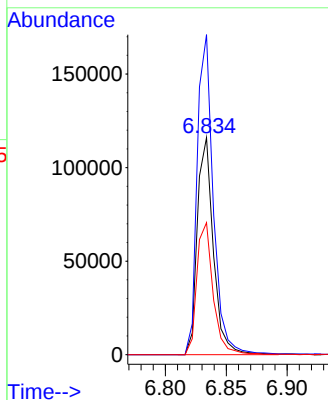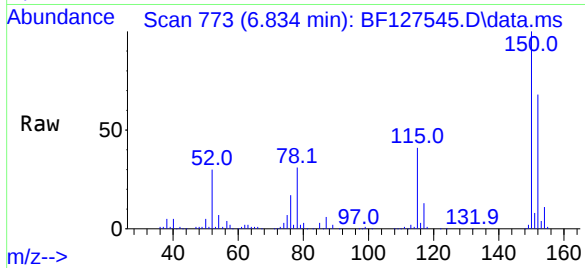

#5
2-Fluorophenol
Concen: 125.957 ng
RT: 5.469 min Scan# 541
Delta R.T. 0.012 min
Lab File: BF127545.D
Acq: 28 Mar 2022 16:40

Tgt Ion:112 Resp: 844464
Ion Ratio Lower Upper
112 100
64 76.0 58.4 87.6
63 39.1 30.1 45.1

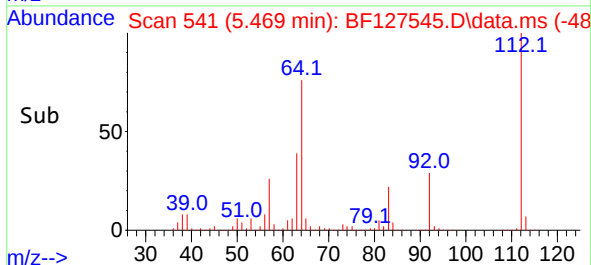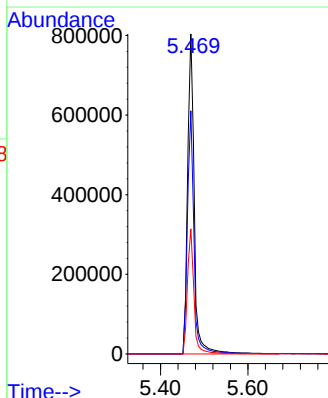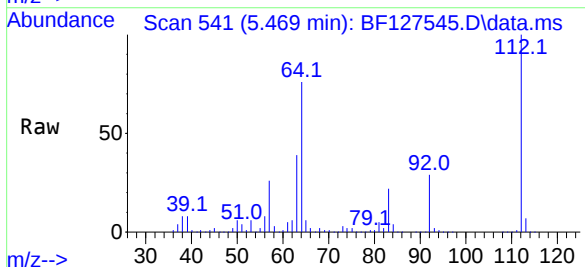




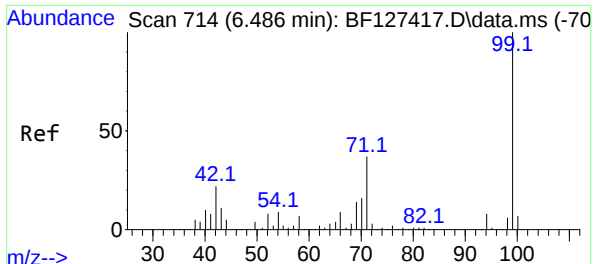


#7
Phenol-d6
Concen: 126.083 ng
RT: 6.475 min Scan# 714
Delta R.T. -0.006 min
Lab File: BF127545.D
Acq: 28 Mar 2022 16:40

Instrument :
BNA_F
ClientSampleId :
PB143554TB

Tgt Ion: 99 Resp: 1155472




Ion	Ratio	Lower	Upper
99	100		
42	22.9	17.8	26.6
71	38.7	29.6	44.4

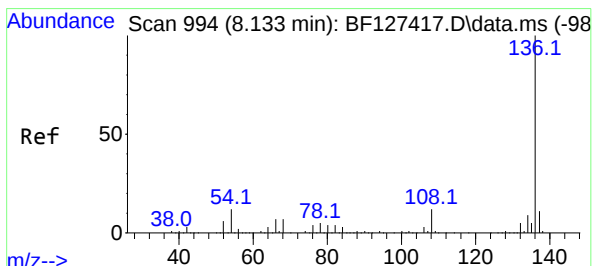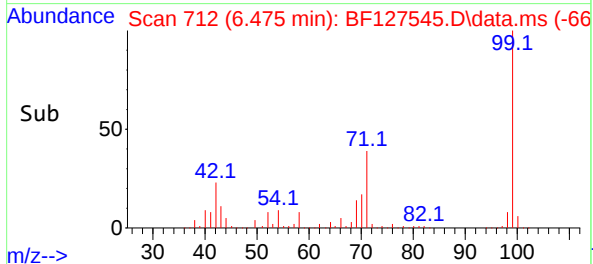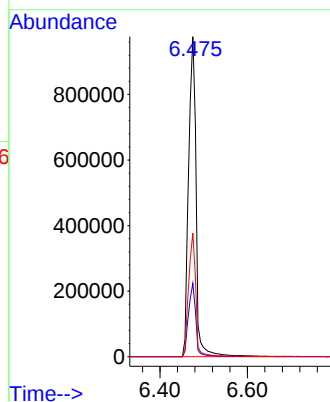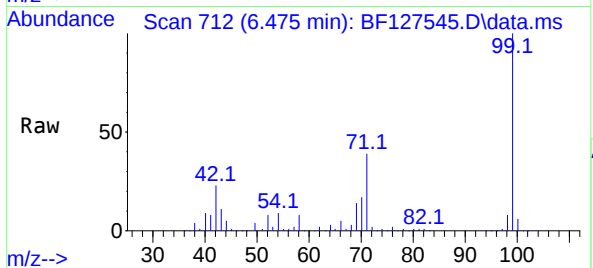


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.116 min Scan# 991
Delta R.T. 0.000 min
Lab File: BF127545.D
Acq: 28 Mar 2022 16:40

Tgt Ion: 136 Resp: 400821

Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.6	13.0
54	11.6	9.2	13.8
68	7.1	5.4	8.0


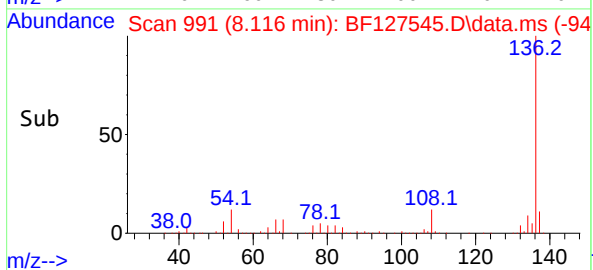
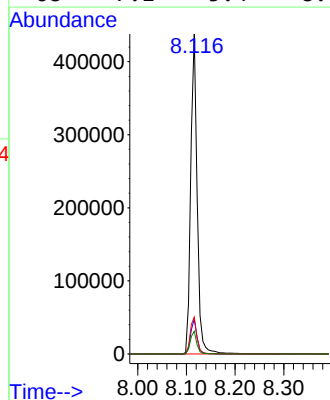
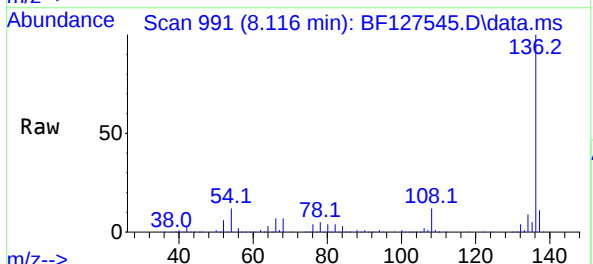


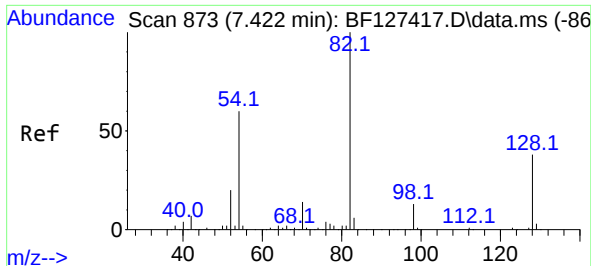

#23
Nitrobenzene-d5
Concen: 84.076 ng
RT: 7.404 min Scan# 81
Delta R.T. -0.006 min
Lab File: BF127545.D
Acq: 28 Mar 2022 16:40




Instrument :
BNA_F
ClientSampleId :
PB143554TB

Tgt Ion: 82 Resp: 788370
Ion Ratio Lower Upper
82 100
128 38.4 30.6 45.8
54 61.9 48.2 72.2

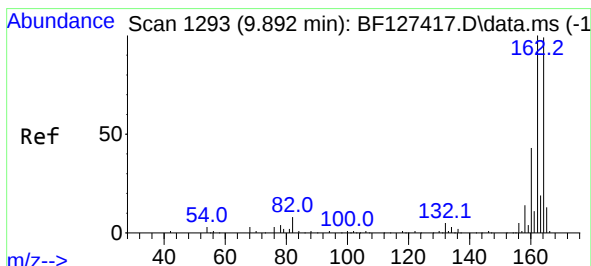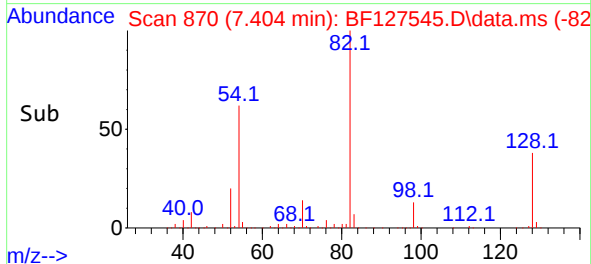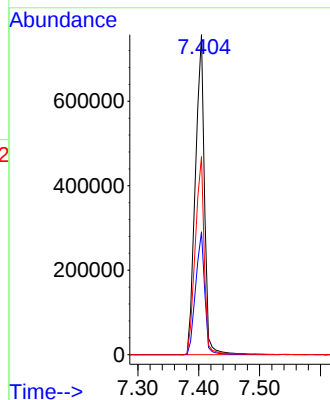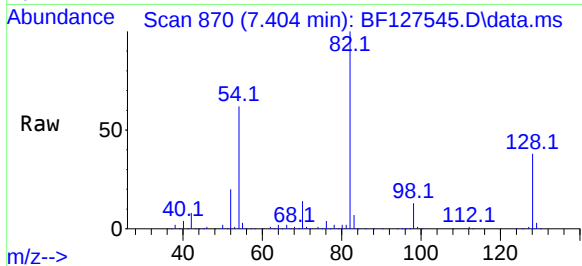

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.869 min Scan# 1289
Delta R.T. -0.006 min
Lab File: BF127545.D
Acq: 28 Mar 2022 16:40

Tgt Ion:164 Resp: 236316
Ion Ratio Lower Upper
164 100
162 100.5 81.2 121.8
160 44.0 34.6 52.0

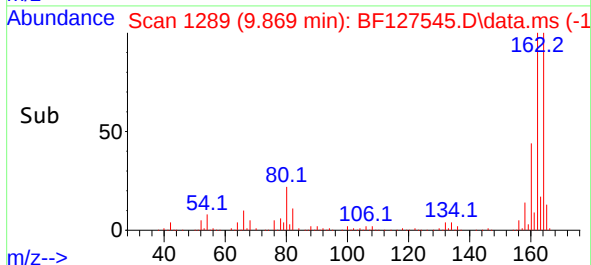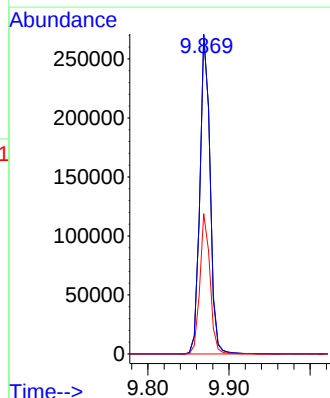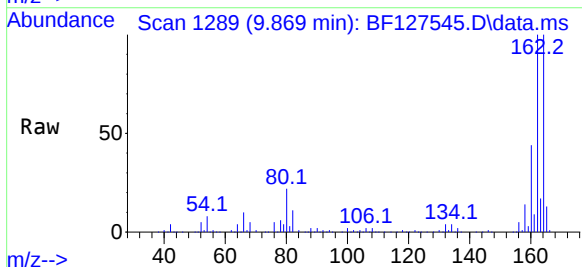



#42

2,4,6-Tribromophenol

Concen: 120.575 ng

RT: 10.669 min Scan# 1428

Delta R.T. 0.000 min

Lab File: BF127545.D

Acq: 28 Mar 2022 16:40

Instrument :

BNA_F

ClientSampleId :

PB143554TB




Tgt Ion:330 Resp: 303532

Ion Ratio Lower Upper

330 100

332 96.5 79.1 118.7

141 31.6 26.2 39.4

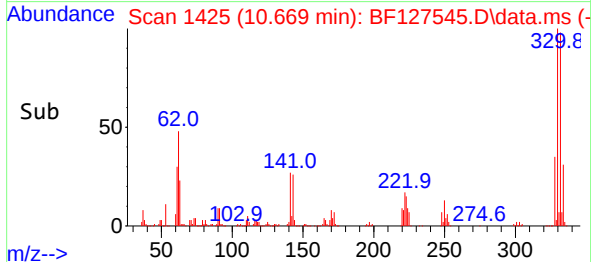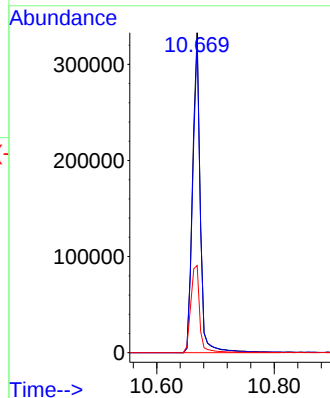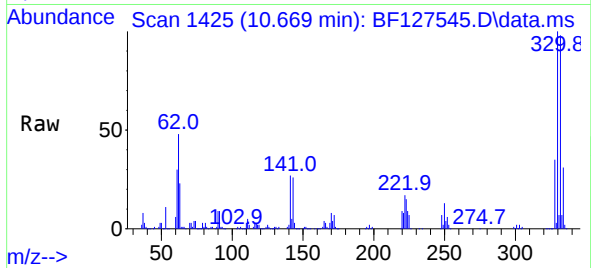

#45

2-Fluorobiphenyl

Concen: 82.509 ng

RT: 9.192 min Scan# 1174

Delta R.T. 0.000 min

Lab File: BF127545.D

Acq: 28 Mar 2022 16:40




Tgt Ion:172 Resp: 1335282

Ion Ratio Lower Upper

172 100

171 35.2 28.4 42.6

170 23.5 18.6 27.8


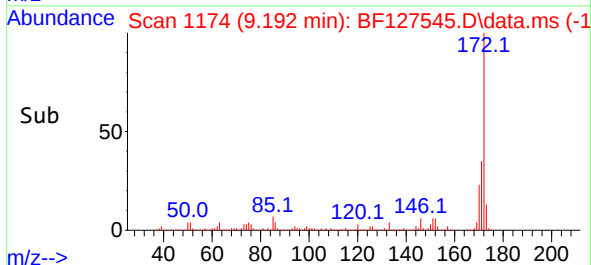
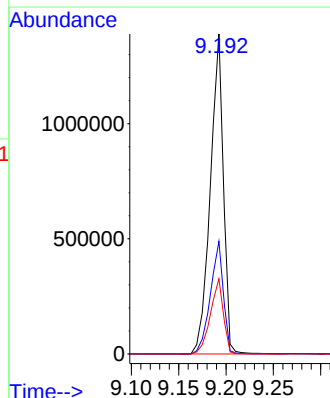
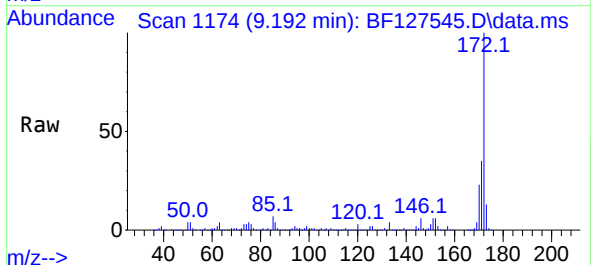




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.363 min Scan# 11
Delta R.T. 0.000 min
Lab File: BF127545.D
Acq: 28 Mar 2022 16:40




Instrument :
BNA_F
ClientSampleId :
PB143554TB

Tgt Ion:188 Resp: 419987
Ion Ratio Lower Upper
188 100
94 10.2 7.4 11.0
80 11.3 8.0 12.0

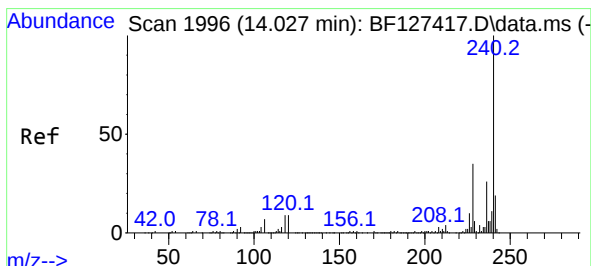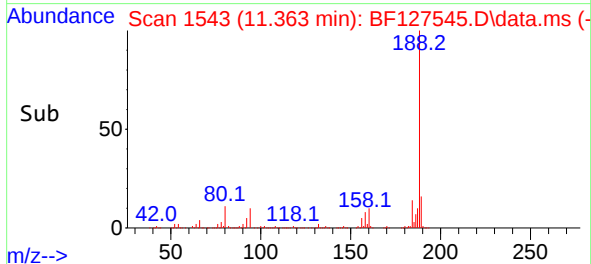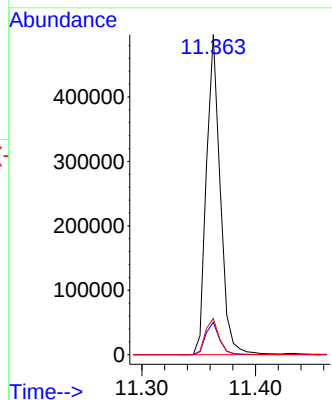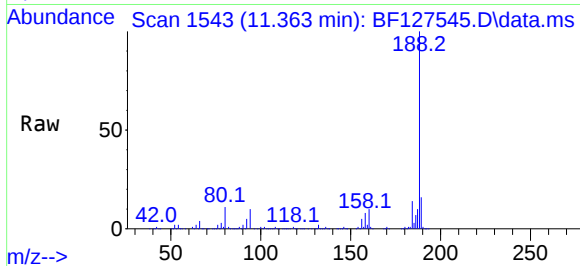

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.010 min Scan# 1993
Delta R.T. -0.006 min
Lab File: BF127545.D
Acq: 28 Mar 2022 16:40


Tgt Ion:240 Resp: 288987
Ion Ratio Lower Upper
240 100
120 10.6 7.1 10.7
236 24.7 20.7 31.1

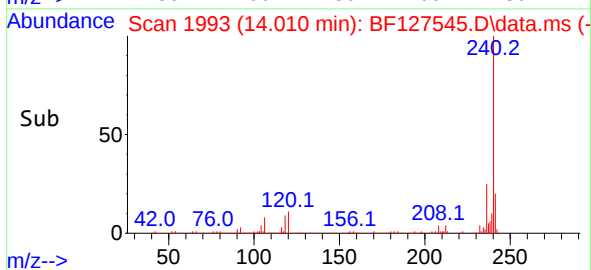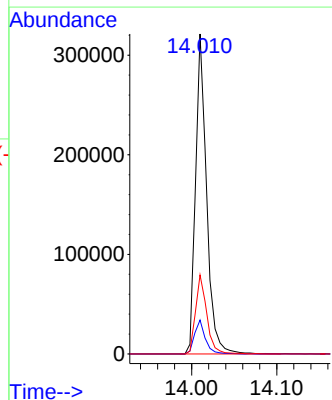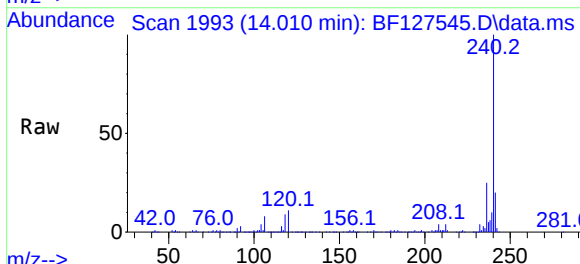





#79
 Terphenyl-d14
 Concen: 85.071 ng
 RT: 12.951 min Scan# 1813
 Delta R.T. 0.000 min
 Lab File: BF127545.D
 Acq: 28 Mar 2022 16:40

Instrument :
 BNA_F
 ClientSampleId :
 PB143554TB

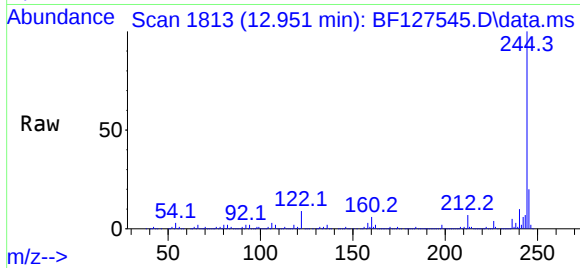

Tgt Ion:244 Resp: 1501775
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.7 8.5
 122 9.2 6.2 9.2

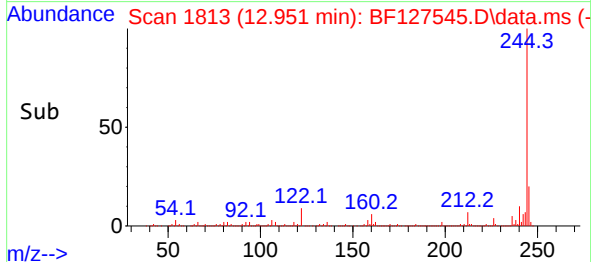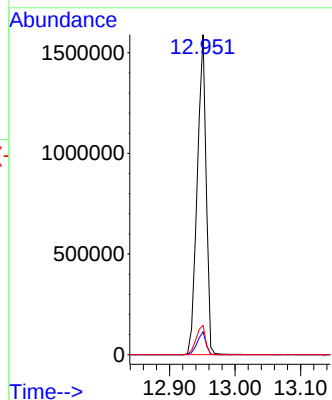

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.492 min Scan# 2245
 Delta R.T. 0.000 min
 Lab File: BF127545.D
 Acq: 28 Mar 2022 16:40

Tgt Ion:264 Resp: 212396
 Ion Ratio Lower Upper
 264 100
 260 24.2 19.1 28.7
 265 20.6 17.4 26.2

