

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
 Data File : BF127543.D
 Acq On : 28 Mar 2022 15:44
 Operator : CG\JU
 Sample : PB143603BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143603BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127543.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.128	479	483	494	rBV	22230	43526	1.04%	0.171%
2	5.469	538	541	564	rBV	3145605	3565409	85.49%	14.034%
3	6.475	708	712	715	rBV	3020660	3571923	85.65%	14.059%
4	6.834	770	773	787	rVB	760880	705927	16.93%	2.779%
5	7.404	865	870	873	rBV	2367388	2484978	59.59%	9.781%
6	8.116	987	991	1005	rBV	977871	934685	22.41%	3.679%
7	9.192	1168	1174	1177	rBV	4158878	4170464	100.00%	16.415%
8	9.869	1285	1289	1302	rVB	1241955	1081446	25.93%	4.257%
9	10.669	1420	1425	1428	rBV	2589367	2431408	58.30%	9.570%
10	11.363	1540	1543	1552	rBV	1283101	1070059	25.66%	4.212%
11	12.951	1808	1813	1816	rBV	4104190	4003324	95.99%	15.757%
12	14.010	1990	1993	2005	rBV	846567	760972	18.25%	2.995%
13	15.492	2241	2245	2259	rVB	416752	581833	13.95%	2.290%




Sum of corrected areas: 25405954

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
Data File : BF127543.D
Acq On : 28 Mar 2022 15:44
Operator : CG\JU
Sample : PB143603BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143603BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

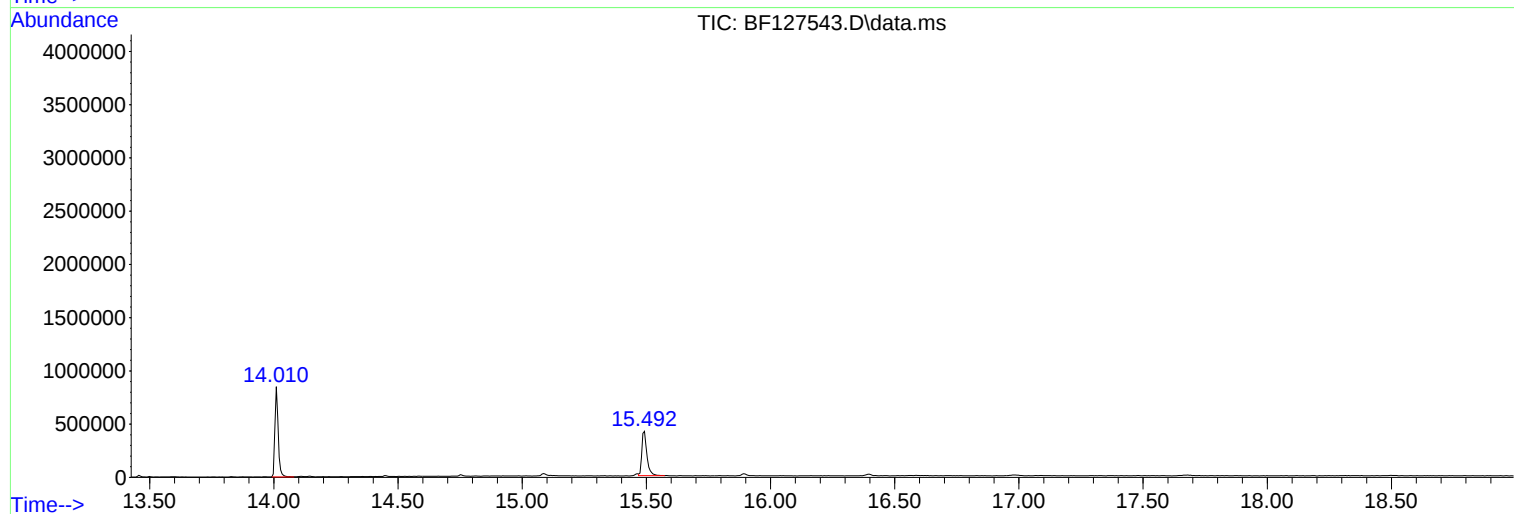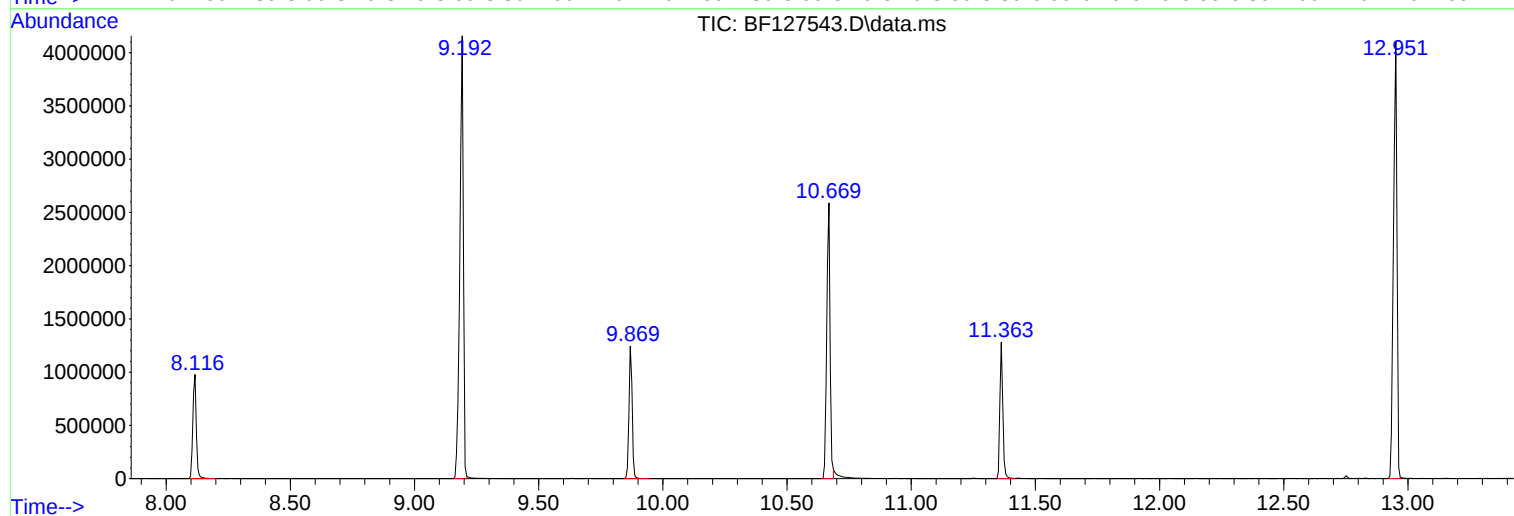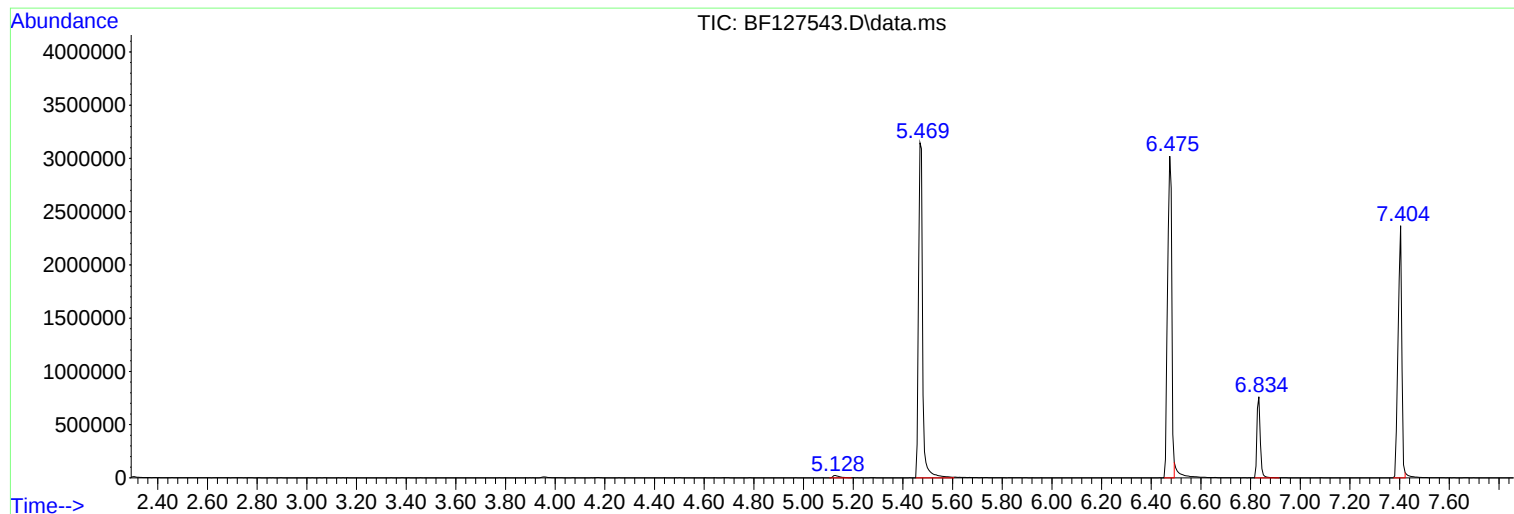

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
Data File : BF127543.D
Acq On : 28 Mar 2022 15:44
Operator : CG\JU
Sample : PB143603BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143603BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
Data File : BF127543.D
Acq On : 28 Mar 2022 15:44
Operator : CG\JU
Sample : PB143603BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143603BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------