

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
 Data File : BF127544.D
 Acq On : 28 Mar 2022 16:12
 Operator : CG\JU
 Sample : PB143610BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143610BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127544.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.122	479	482	495	rBV	21541	39119	1.01%	0.162%
2	5.469	537	541	566	rBV	3179243	3377685	86.83%	13.987%
3	6.475	708	712	715	rBV	2974487	3346685	86.03%	13.859%
4	6.834	770	773	783	rBV	730877	659689	16.96%	2.732%
5	7.404	865	870	873	rBV	2272219	2308845	59.35%	9.561%
6	8.116	987	991	1001	rBV	969990	871554	22.40%	3.609%
7	9.192	1168	1174	1177	rBV	4054784	3883378	99.82%	16.081%
8	9.869	1285	1289	1300	rBV	1162826	1014368	26.07%	4.200%
9	10.669	1421	1425	1447	rBV	2445773	2408729	61.92%	9.974%
10	11.363	1540	1543	1553	rBV	1230421	1032171	26.53%	4.274%
11	12.951	1808	1813	1816	rBV	4078845	3890198	100.00%	16.109%
12	14.010	1990	1993	2002	rBV	822863	748495	19.24%	3.099%
13	15.492	2241	2245	2256	rVB	432319	568042	14.60%	2.352%




Sum of corrected areas: 24148958

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
Data File : BF127544.D
Acq On : 28 Mar 2022 16:12
Operator : CG\JU
Sample : PB143610BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143610BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

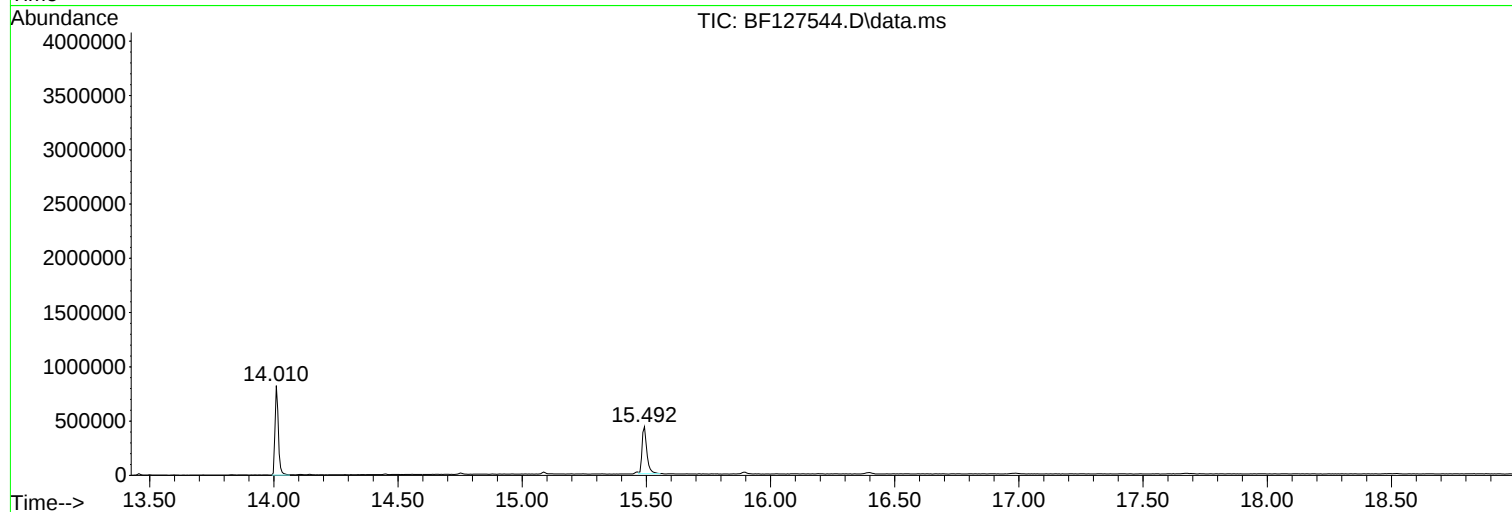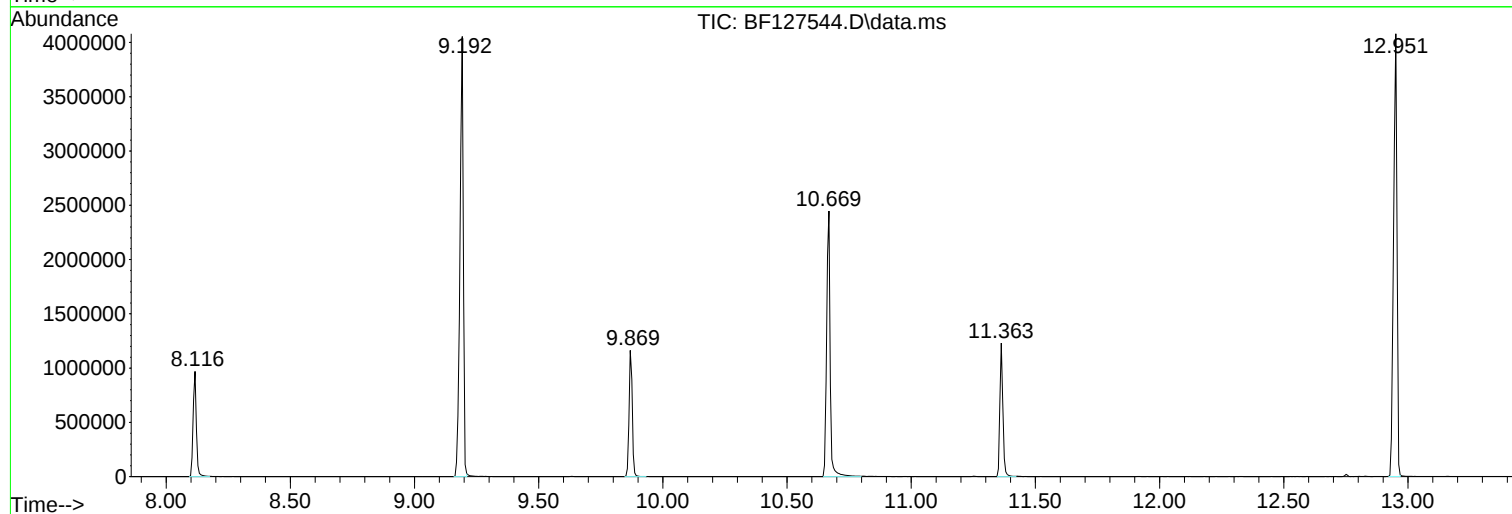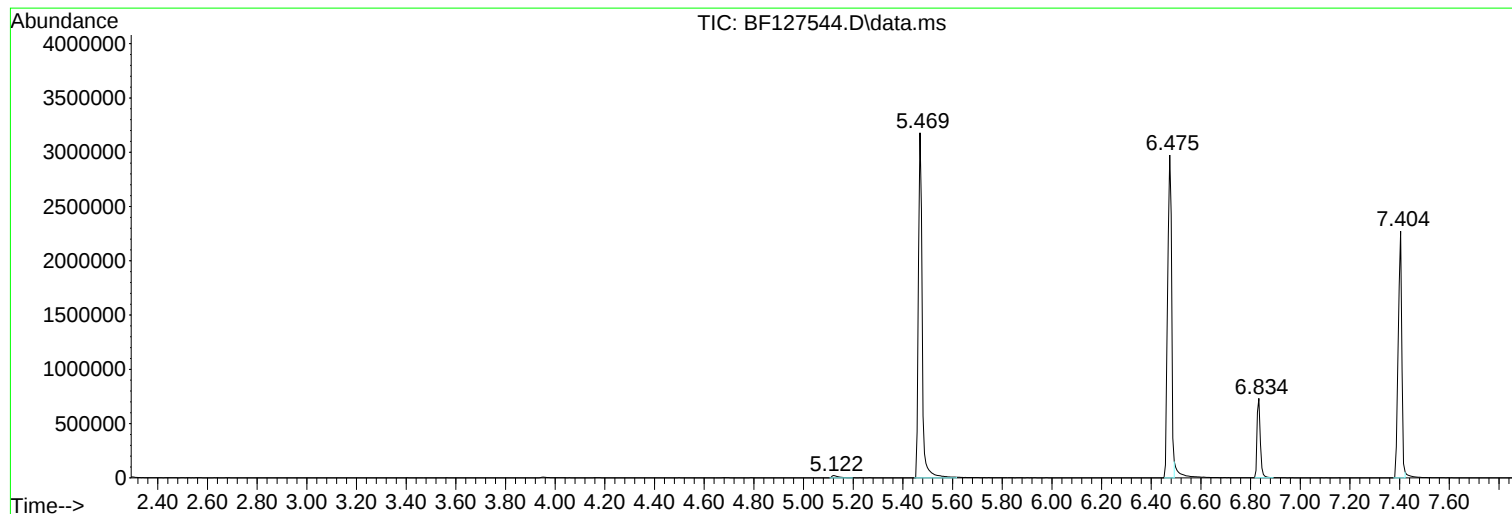

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
Data File : BF127544.D
Acq On : 28 Mar 2022 16:12
Operator : CG\JU
Sample : PB143610BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143610BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
Data File : BF127544.D
Acq On : 28 Mar 2022 16:12
Operator : CG\JU
Sample : PB143610BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143610BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------