

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
 Data File : BF127549.D
 Acq On : 28 Mar 2022 18:39
 Operator : CG\JU
 Sample : N2107-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SS2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127549.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	536	539	567	rBV	2084893	2289820	82.98%	12.785%
2	6.475	708	712	738	rBV	2372005	2373698	86.02%	13.253%
3	6.834	770	773	782	rBV	615132	550901	19.97%	3.076%
4	7.398	866	869	882	rBV	1629421	1594813	57.80%	8.904%
5	8.116	987	991	1000	rBV	808063	715965	25.95%	3.997%
6	9.186	1169	1173	1177	rBV	2852212	2676116	96.98%	14.941%
7	9.869	1286	1289	1298	rVB	1029777	830603	30.10%	4.637%
8	10.663	1420	1424	1438	rBV	1832468	1675004	60.70%	9.352%
9	11.363	1539	1543	1551	rBV	1004105	857878	31.09%	4.790%
10	11.880	1627	1631	1635	rBV2	24394	27713	1.00%	0.155%
11	12.945	1808	1812	1816	rBV	2892301	2759329	100.00%	15.406%
12	13.845	1959	1965	1984	rBV2	105279	347101	12.58%	1.938%
13	14.010	1990	1993	2004	rBV	752651	669476	24.26%	3.738%
14	15.492	2241	2245	2255	rVB	403086	542361	19.66%	3.028%




Sum of corrected areas: 17910778

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
Data File : BF127549.D
Acq On : 28 Mar 2022 18:39
Operator : CG\JU
Sample : N2107-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

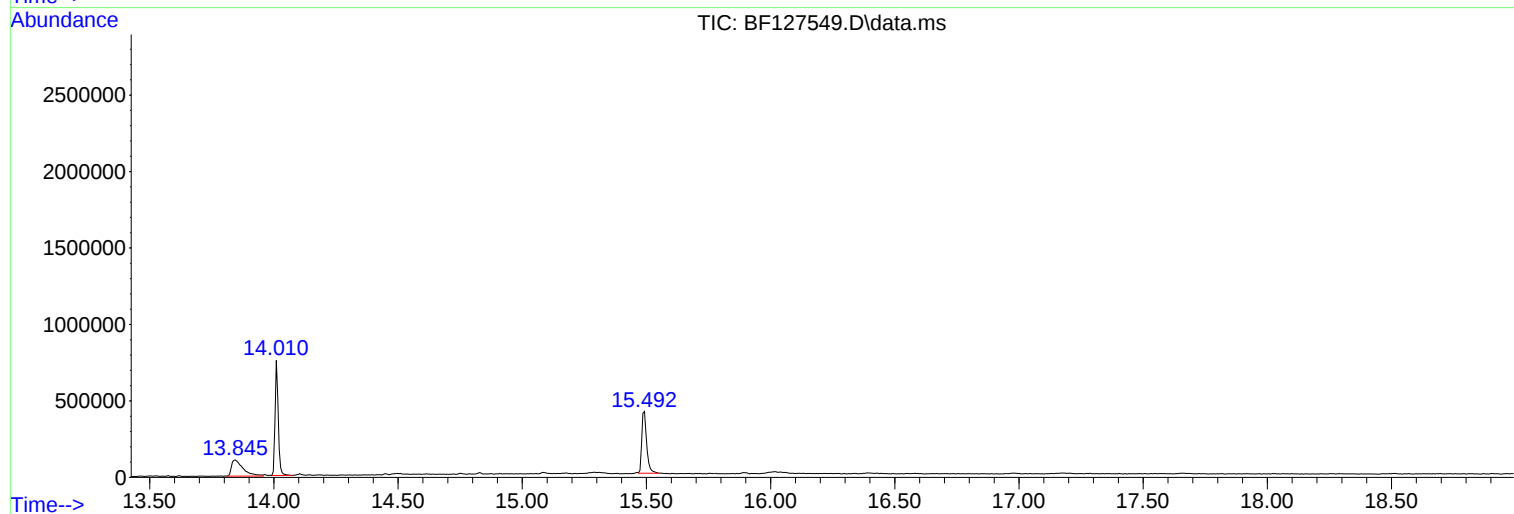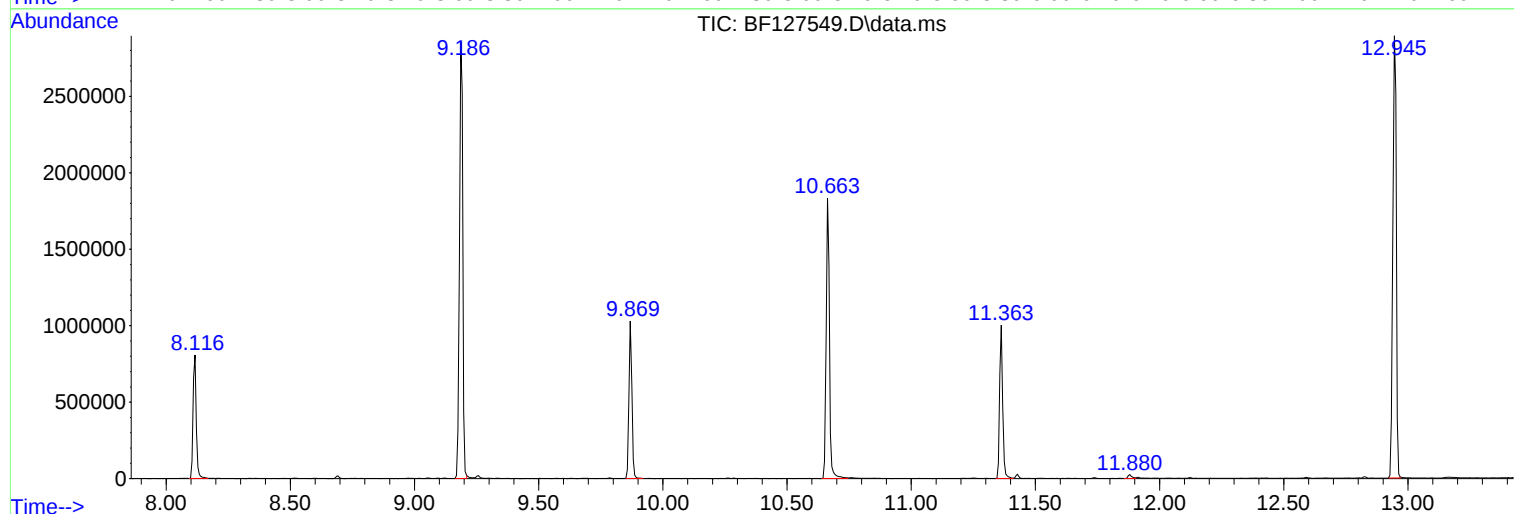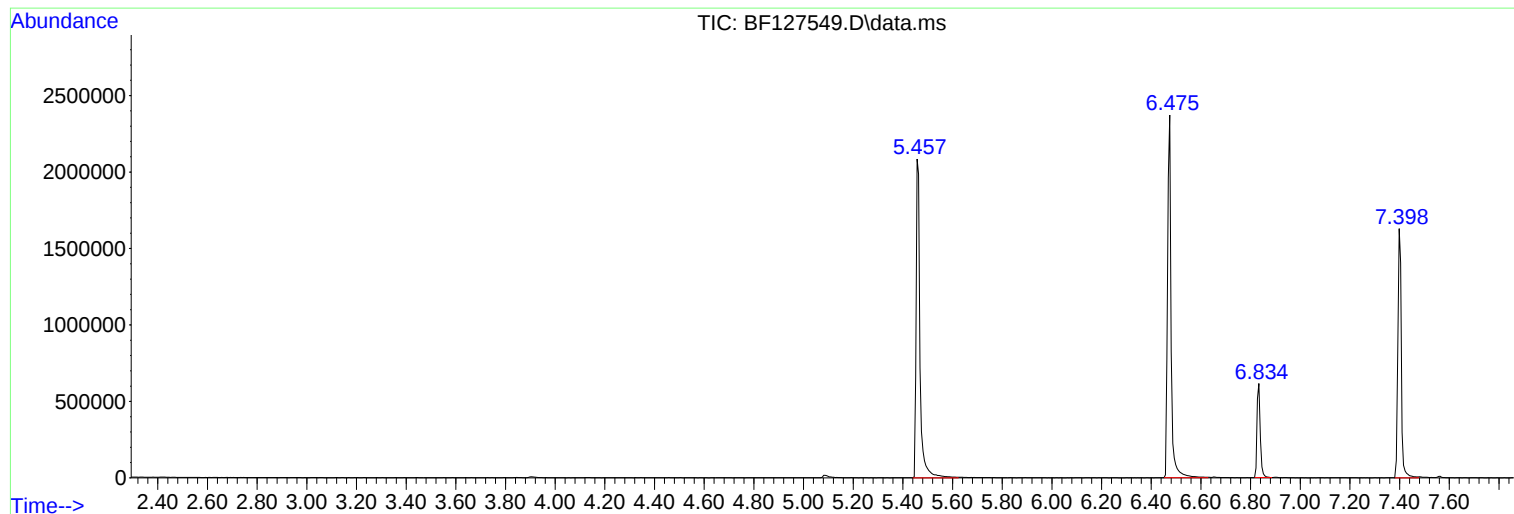

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
Data File : BF127549.D
Acq On : 28 Mar 2022 18:39
Operator : CG\JU
Sample : N2107-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 n-Nonadecanol-1 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.845	10.37 ng	347101	Chrysene-d12	14.010

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			n-Nonadecanol-1	284	C19H40O	001454-84-8	95
2			Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94
3			Bromoacetic acid, hexadecyl ester	362	C18H35BrO2	005454-48-8	94
4			Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	94
5			Trifluoroacetic acid, pentadecyl...	324	C17H31F3O2	959010-23-2	94

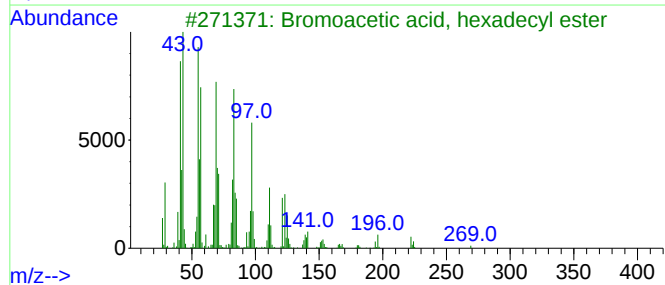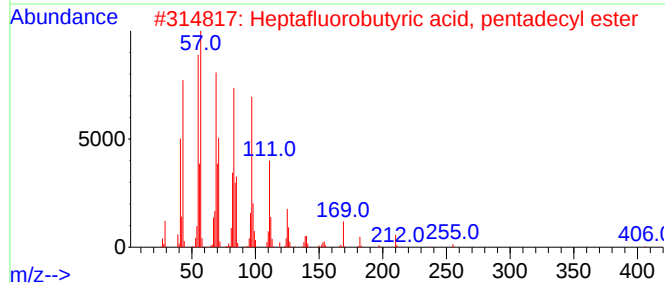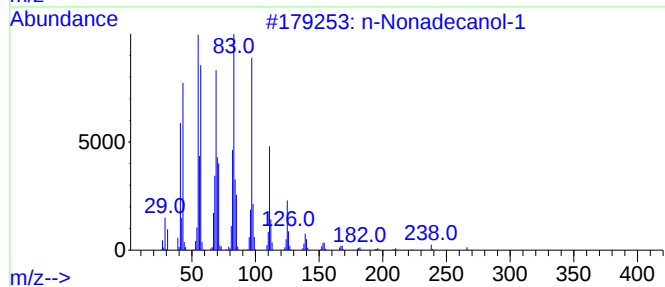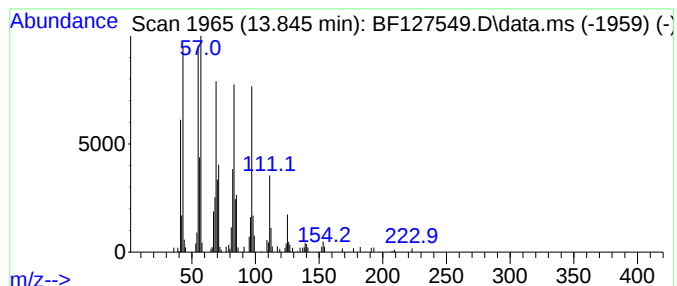

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
Data File : BF127549.D
Acq On : 28 Mar 2022 18:39
Operator : CG\JU
Sample : N2107-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
n-Nonadecanol-1	13.845	10.4	ng	347101	5	14.010	669476	20.0