

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
 Data File : BF127551.D
 Acq On : 28 Mar 2022 19:35
 Operator : CG\JU
 Sample : N2107-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SS5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127551.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	536	539	561	rBV	2112509	2244609	83.64%	12.510%
2	6.475	708	712	737	rBV	2337435	2354047	87.71%	13.120%
3	6.834	770	773	782	rBV	639269	570656	21.26%	3.180%
4	7.398	866	869	881	rBV	1587264	1559199	58.10%	8.690%
5	8.116	987	991	1003	rBV	806393	742210	27.66%	4.137%
6	9.186	1169	1173	1177	rBV	2816738	2662845	99.22%	14.841%
7	9.869	1286	1289	1301	rVB	1064804	862212	32.13%	4.805%
8	10.663	1420	1424	1440	rBV	1845187	1677134	62.49%	9.347%
9	11.363	1539	1543	1551	rBV	1032869	887770	33.08%	4.948%
10	11.880	1627	1631	1635	rBV	44098	49020	1.83%	0.273%
11	12.945	1808	1812	1816	rBV	2921686	2683770	100.00%	14.957%
12	13.845	1959	1965	1981	rBV3	112986	393389	14.66%	2.192%
13	14.010	1990	1993	2004	rVB	700744	642608	23.94%	3.581%
14	15.486	2241	2244	2259	rVB	422835	573885	21.38%	3.198%
15	16.015	2324	2334	2338	rBV	12582	39326	1.47%	0.219%




Sum of corrected areas: 17942680

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
Data File : BF127551.D
Acq On : 28 Mar 2022 19:35
Operator : CG\JU
Sample : N2107-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

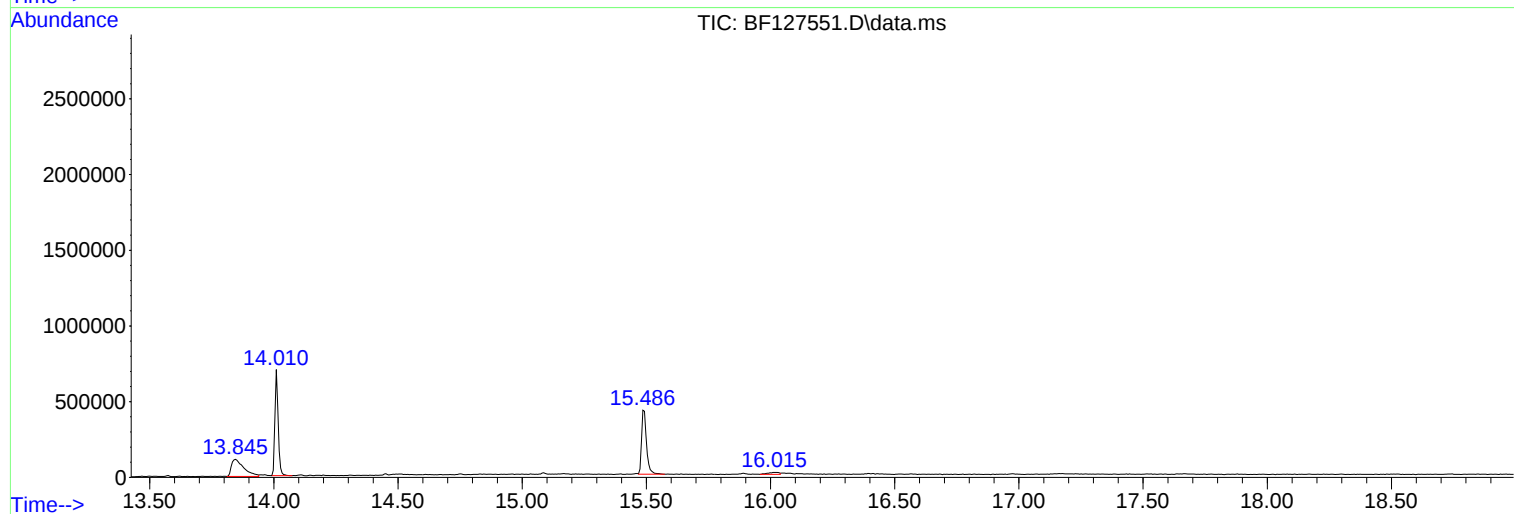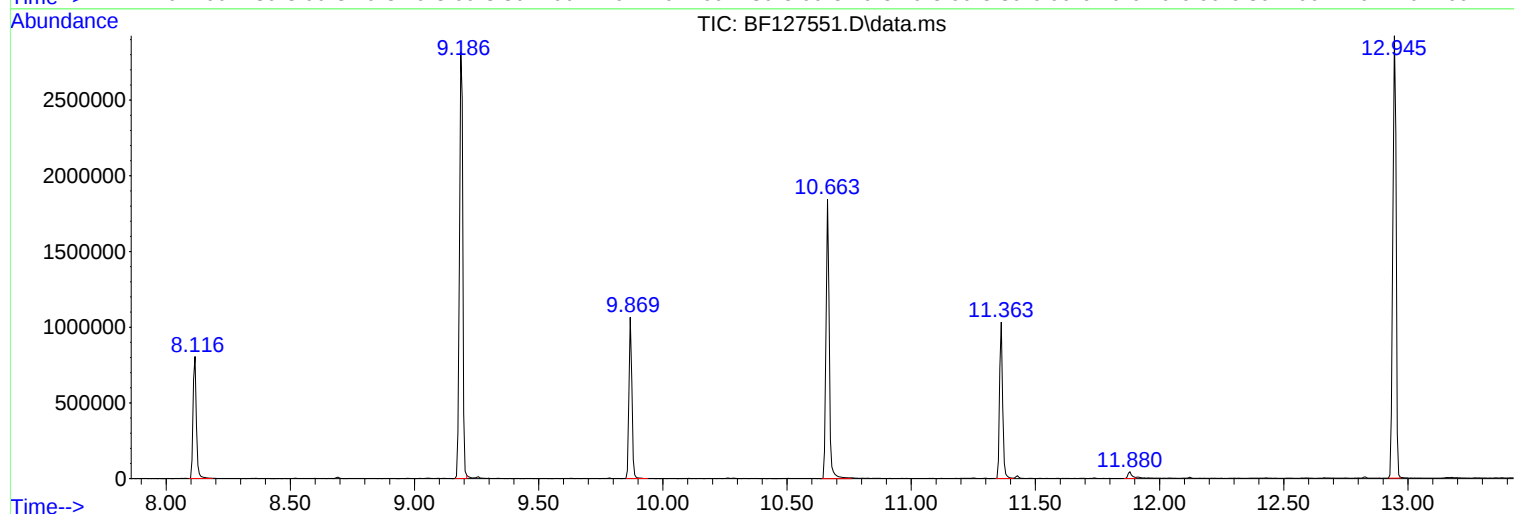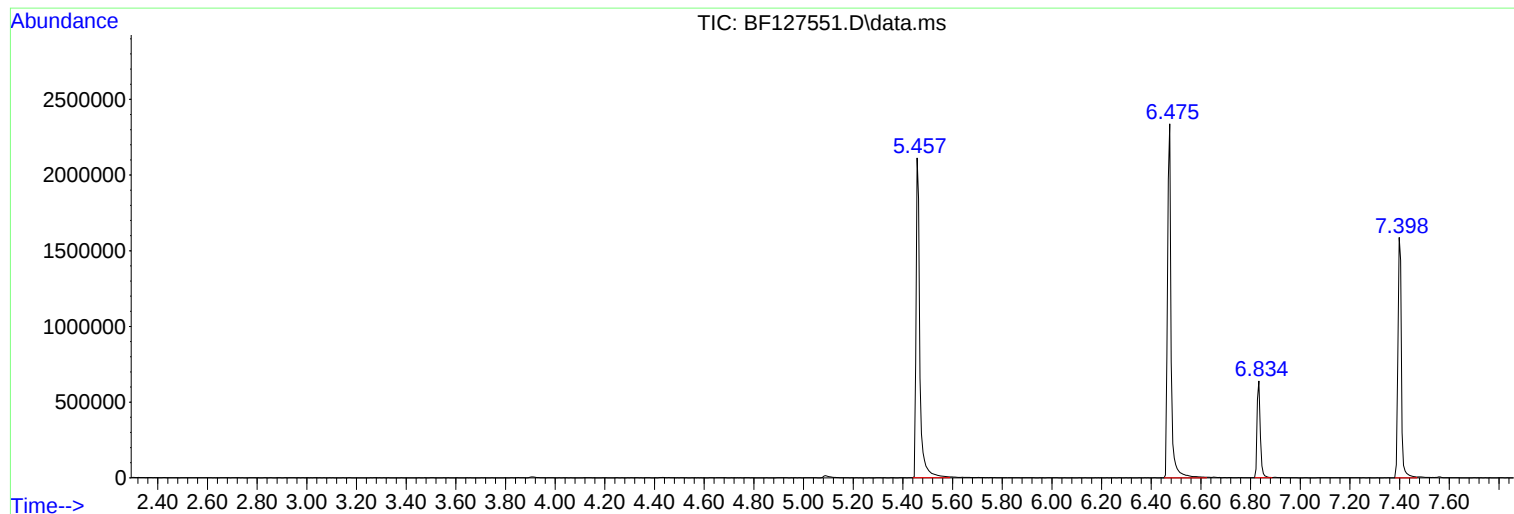

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
Data File : BF127551.D
Acq On : 28 Mar 2022 19:35
Operator : CG\JU
Sample : N2107-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dichloroacetic acid, heptad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.845	12.24 ng	393389	Chrysene-d12	14.010

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	95
2			1-Heneicosanol	312	C21H44O	015594-90-8	94
3			Bromoacetic acid, hexadecyl ester	362	C18H35BrO2	005454-48-8	91
4			2- Chloropropionic acid, octadec...	360	C21H41ClO2	088104-31-8	91
5			1-Docosene	308	C22H44	001599-67-3	91

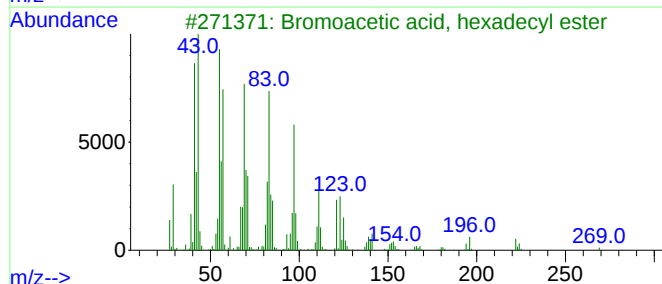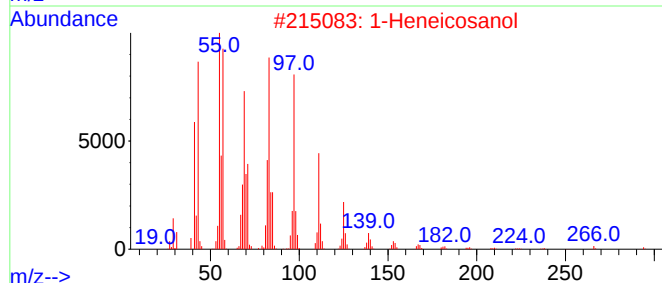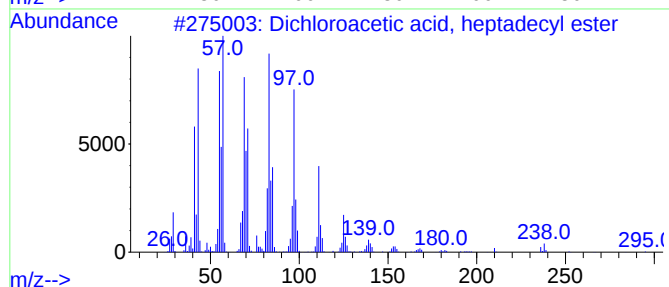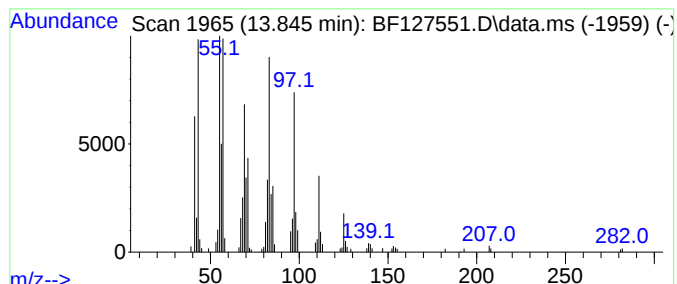

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
Data File : BF127551.D
Acq On : 28 Mar 2022 19:35
Operator : CG\JU
Sample : N2107-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dichloroacetic ...	13.845	12.2	ng	393389	5	14.010	642608	20.0