
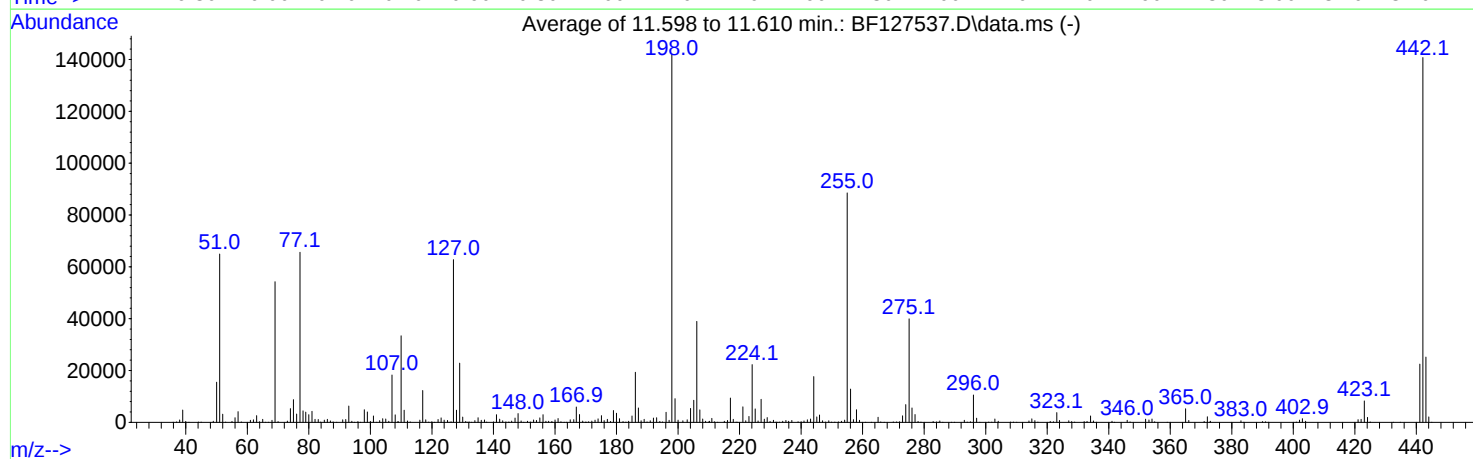


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
 Data File : BF127537.D
 Acq On : 28 Mar 2022 12:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 29 07:13:31 2022

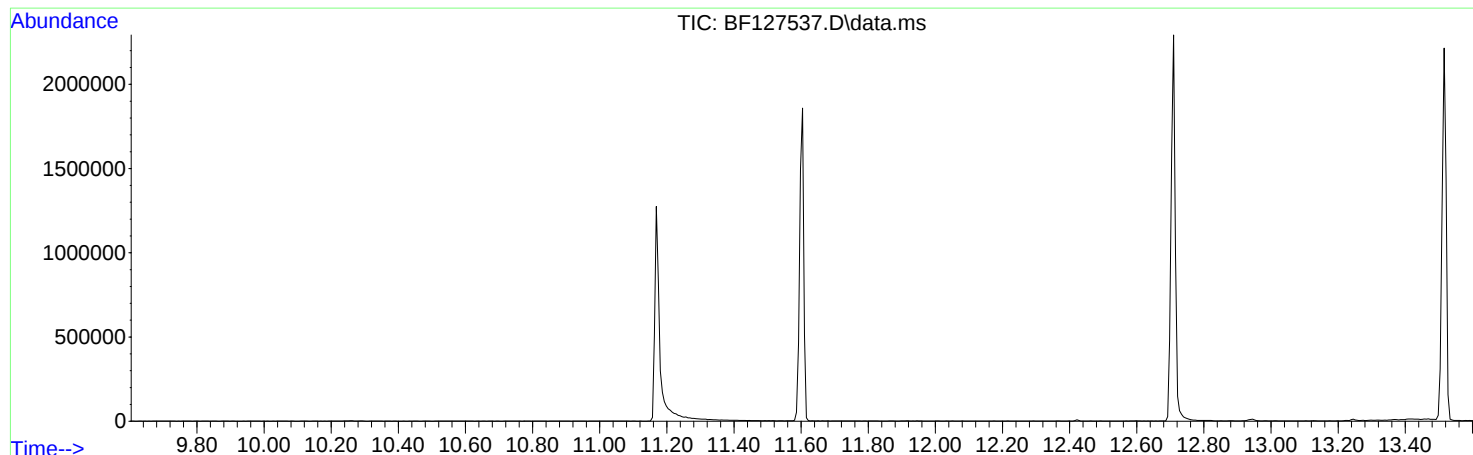




AutoFind: Scans 1583, 1584, 1585; Background Corrected with Scan 1577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.8	64943	PASS
68	69	0.00	2	1.5	803	PASS
69	198	0.00	100	38.2	54262	PASS
70	69	0.00	2	0.6	336	PASS
127	198	10	80	44.2	62760	PASS
197	198	0.00	2	0.6	829	PASS
198	198	100	100	100.0	141933	PASS
199	198	5	9	6.4	9126	PASS
275	198	10	60	28.1	39925	PASS
365	198	1	100	3.7	5252	PASS
441	198	0.01	100	15.8	22459	PASS
442	442	50	100	100.0	140739	PASS
443	442	15	24	17.9	25219	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
 Data File : BF127537.D
 Acq On : 28 Mar 2022 12:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 29 08:33:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 29 07:13:31 2022
 Response via : Initial Calibration

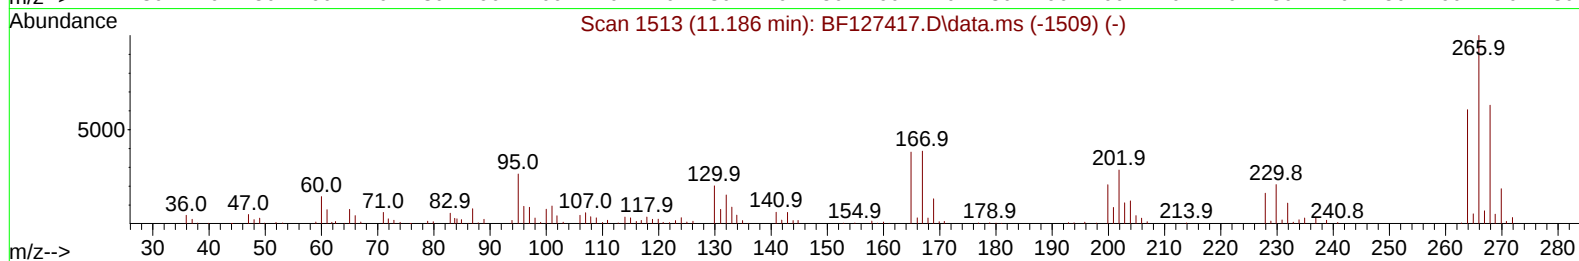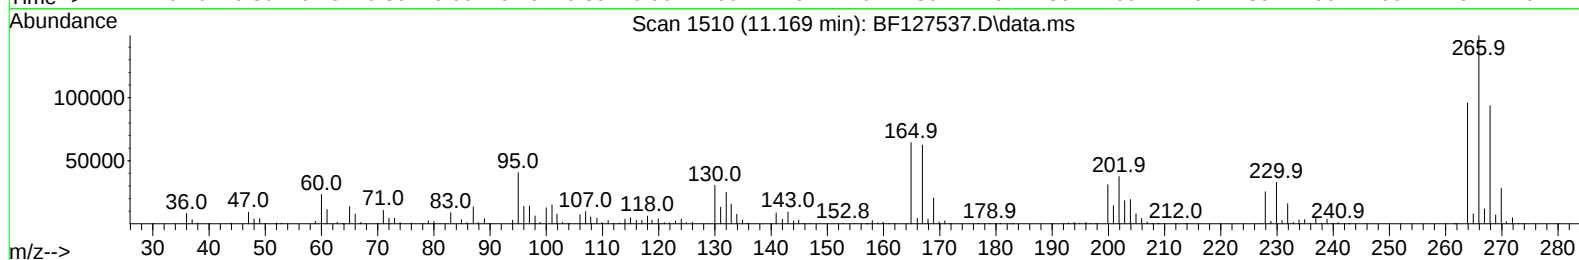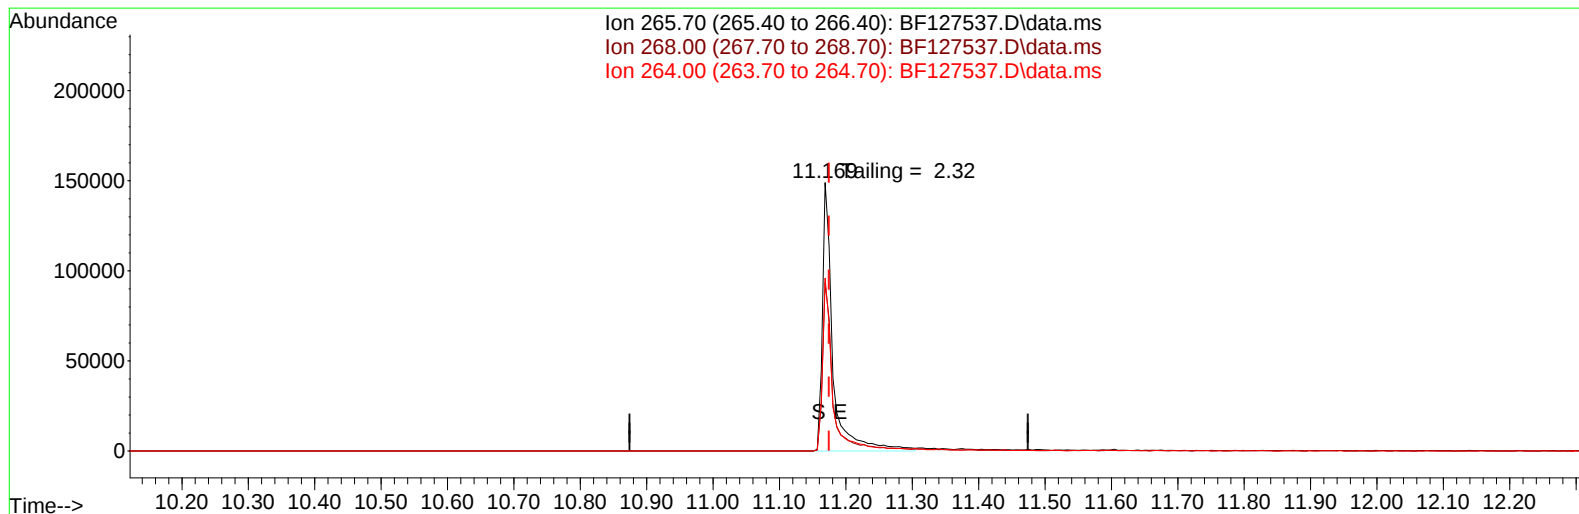

TIC: BF127537.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.006) 41418.78 ng




response 163996

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.78
264.00	60.60	64.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032822\
Data File : BF127537.D
Acq On : 28 Mar 2022 12:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 29 08:33:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 29 07:13:31 2022
Response via : Initial Calibration

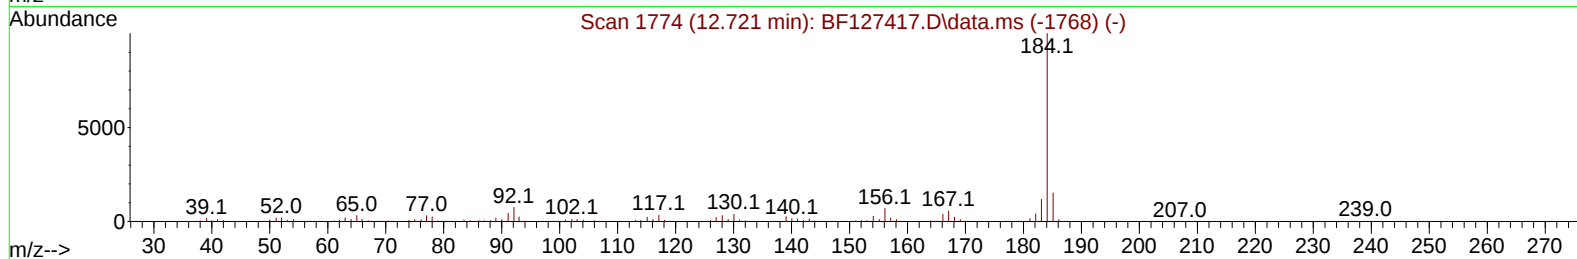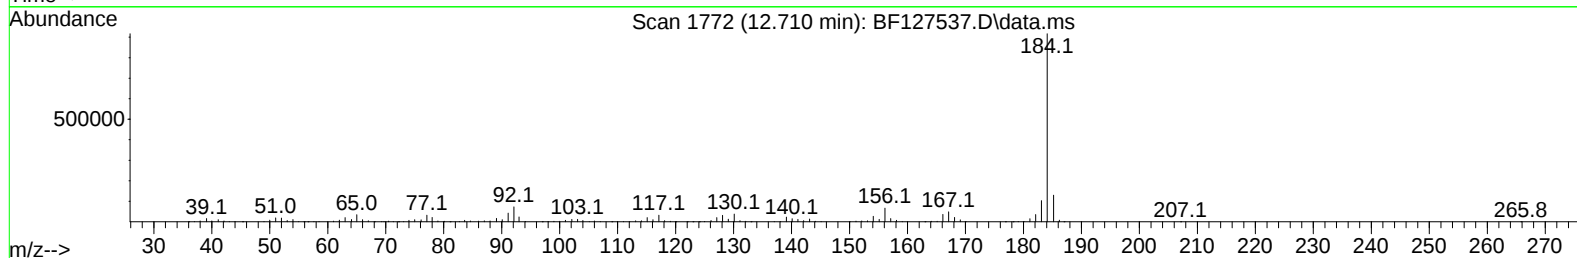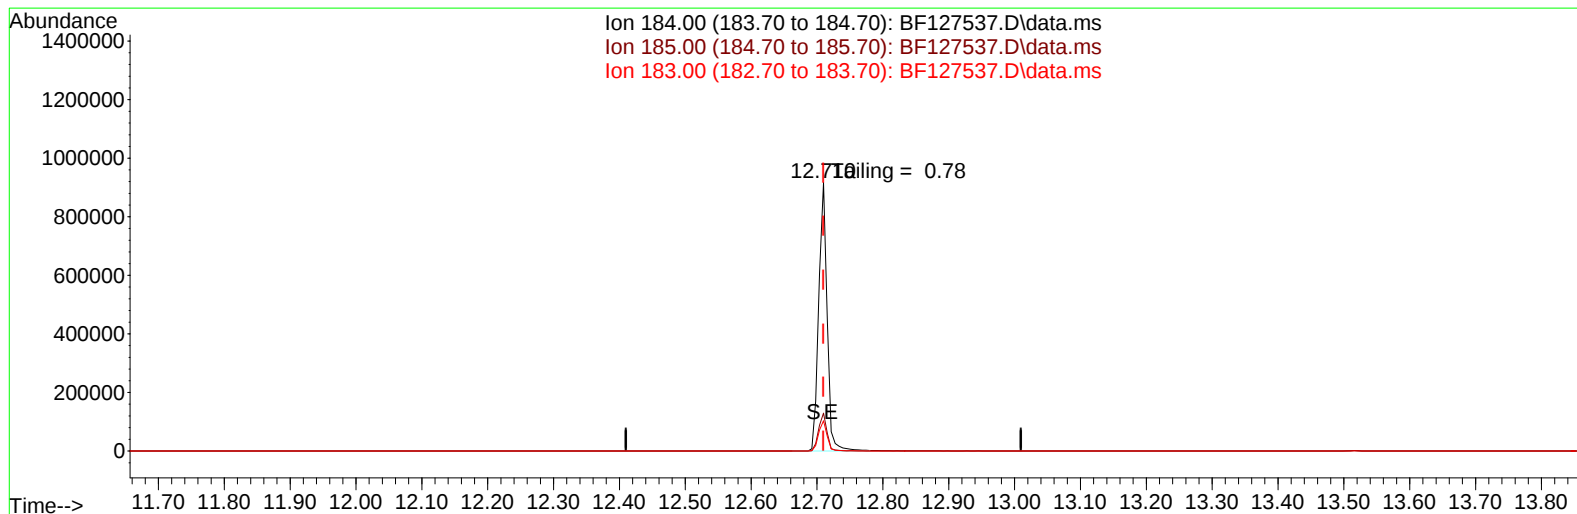

TIC: BF127537.D\data.ms

(77) Benzidine

12.710min (+ 0.000) 66870.32 ng

response 814765

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.12
183.00	11.70	11.30
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/28/2022	BNA_F	<u>BF127537.D</u>
Compound Name	Response	Retention Time
DDT	386854	13.516
DDD	3171	13.245
DDE	219	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3390	390244	0.87

Instrument :
BNA_F
ClientSampleId :
DFTPP