
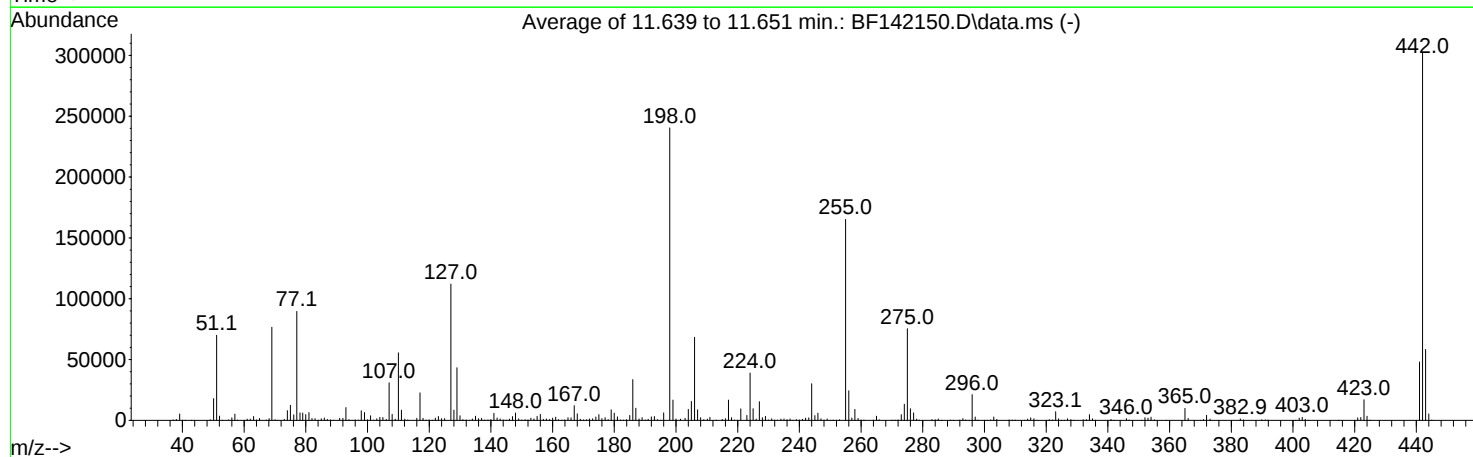


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032825\
Data File : BF142150.D
Acq On : 28 Mar 2025 10:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

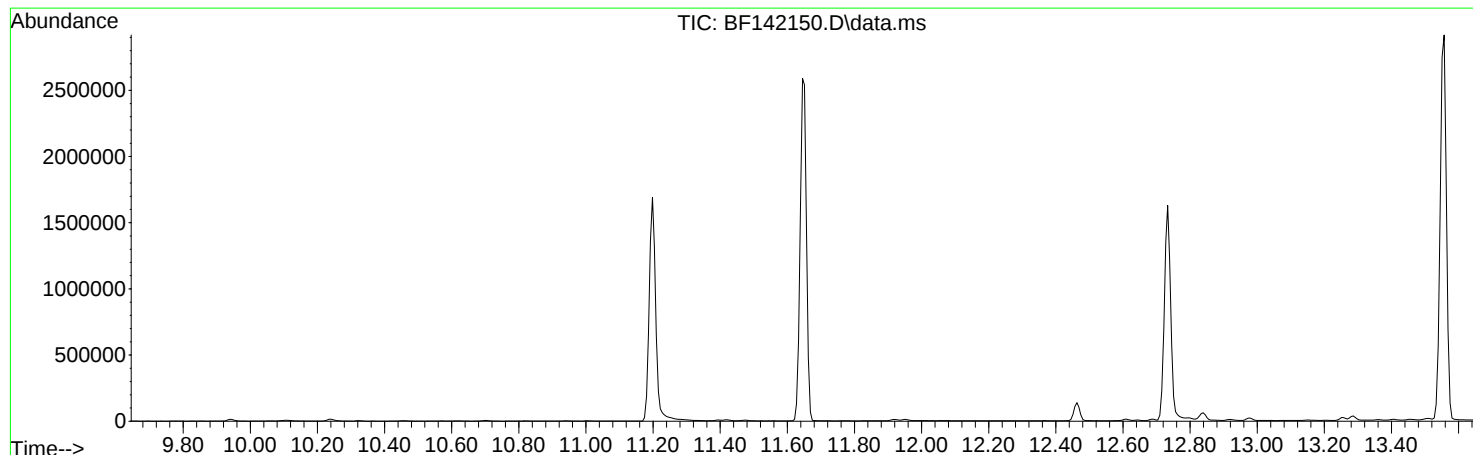




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	69931	PASS
68	69	0.00	2	1.8	1397	PASS
69	198	0.00	100	31.9	76622	PASS
70	69	0.00	2	0.7	502	PASS
127	198	10	80	46.6	112069	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	240448	PASS
199	198	5	9	6.9	16689	PASS
275	198	10	60	31.4	75413	PASS
365	198	1	100	4.1	9901	PASS
441	198	0.01	100	19.9	47960	PASS
442	442	50	100	100.0	302400	PASS
443	442	15	24	19.3	58237	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032825\
Data File : BF142150.D
Acq On : 28 Mar 2025 10:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 28 11:43:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

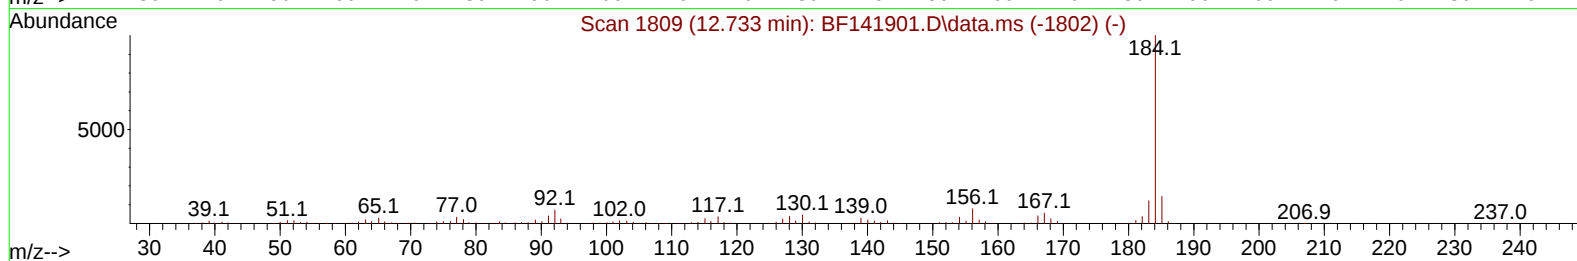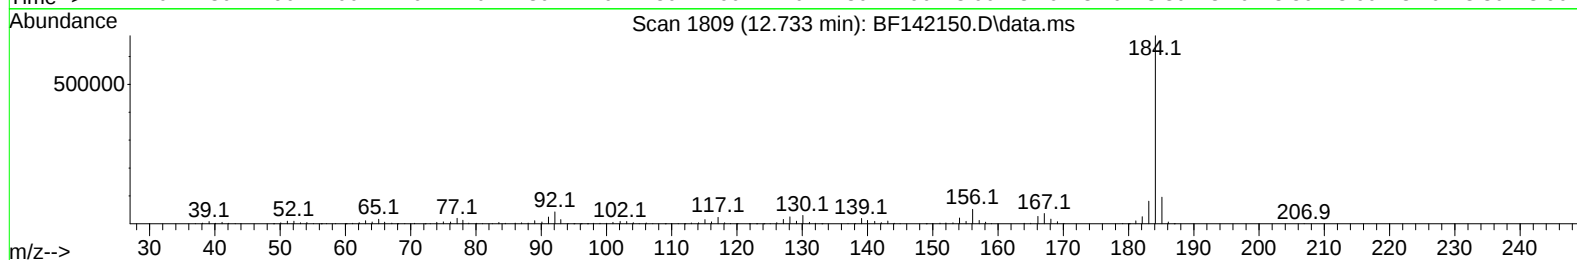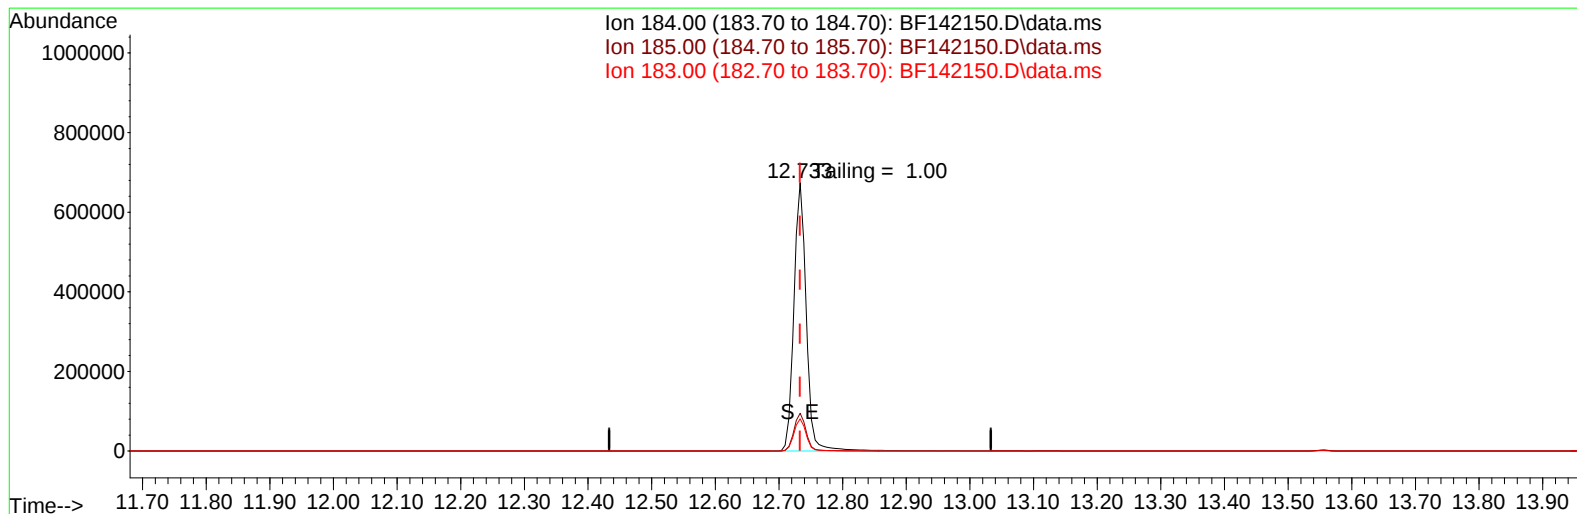

TIC: BF142150.D\data.ms

(77) Benzidine

12.733min (+ 0.000) 26876.26 ng

response 911563

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.11
183.00	12.10	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/28/2025	BNA_F	<u>BF142150.D</u>
Compound Name	Response	Retention Time
DDT	776493	13.557
DDD	14732	13.286
DDE	2062	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16794	793287	2.12

Instrument :
BNA_F
ClientSampleId :
DFTPP