
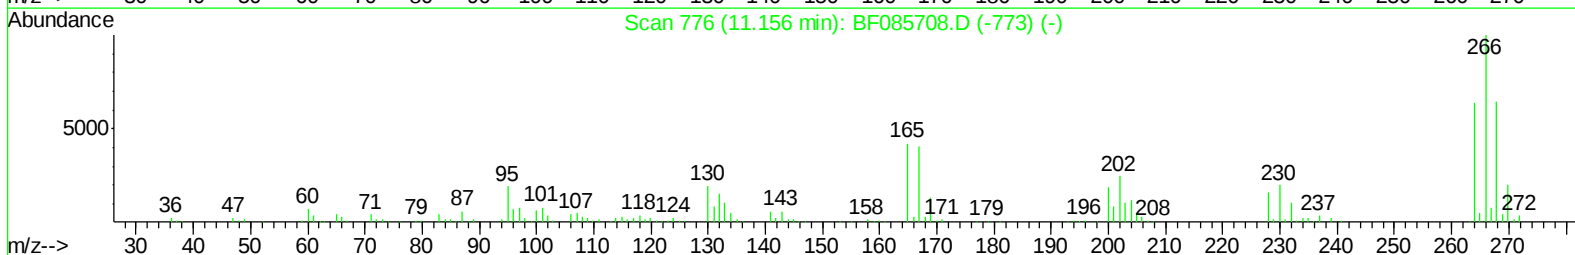
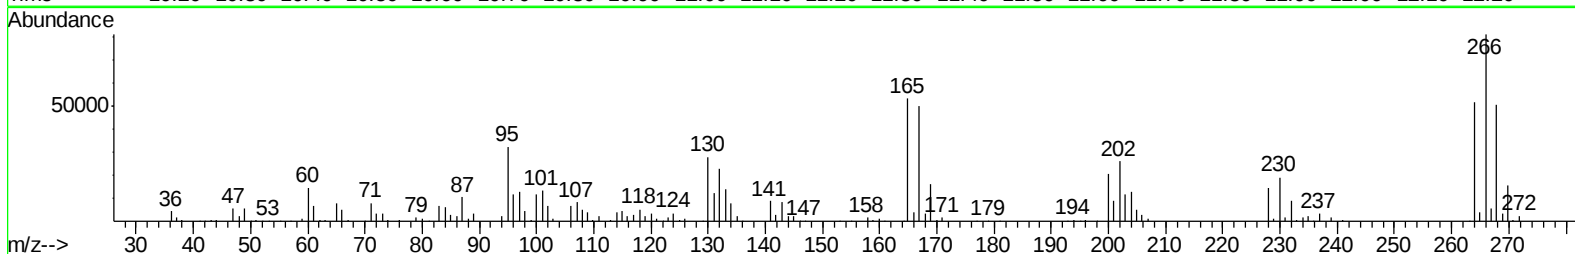


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032916\
Data File : BF085852.D
Acq On : 29 Mar 2016 15:52
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 06:40:44 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 15:27:05 2016
Response via : Initial Calibration

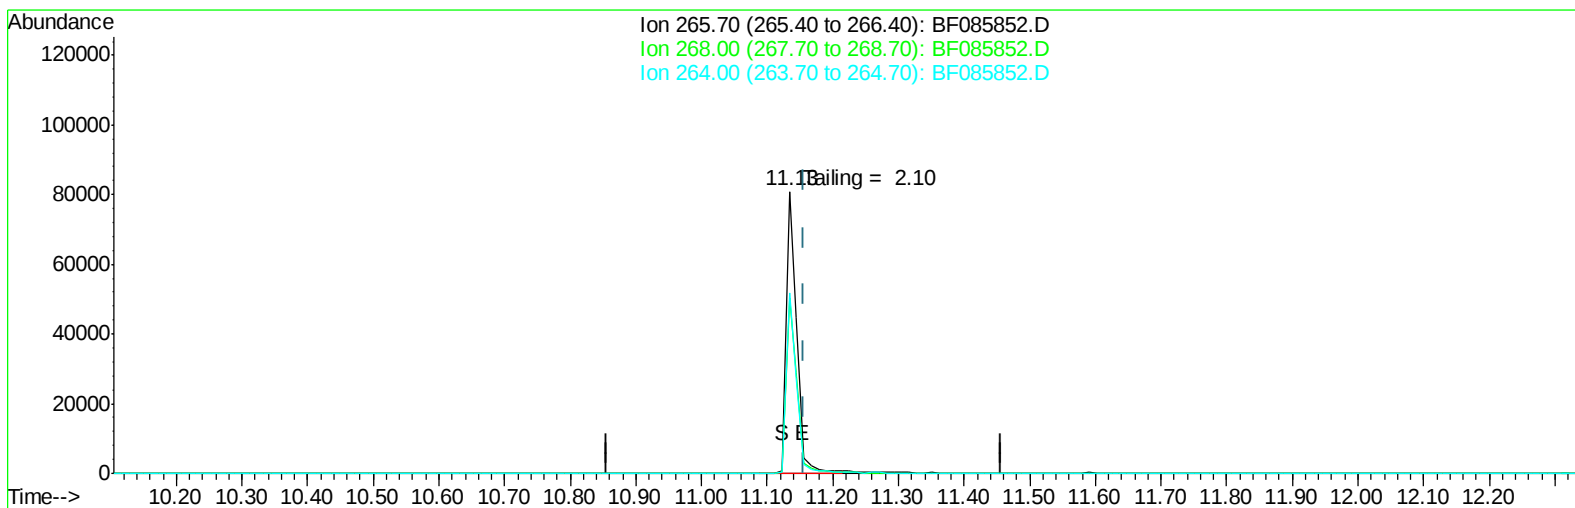

TIC: BF085852.D

(69) Pentachlorophenol (C)




11.133min (-0.023) 46142.48ng

response 96221

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.23
264.00	63.30	64.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032916\
 Data File : BF085852.D
 Acq On : 29 Mar 2016 15:52
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 06:40:44 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 15:27:05 2016
 Response via : Initial Calibration

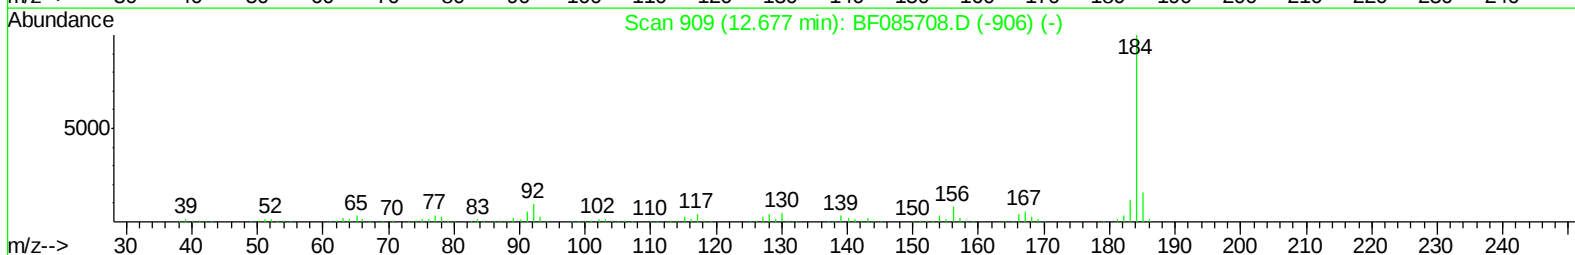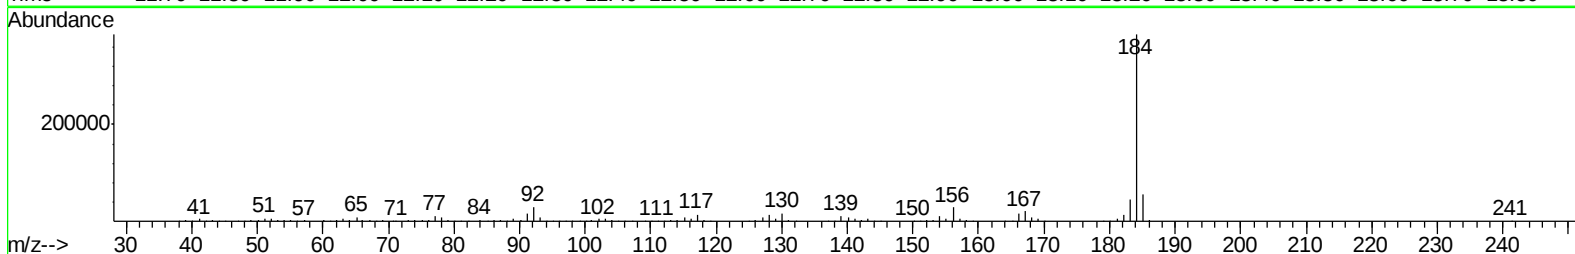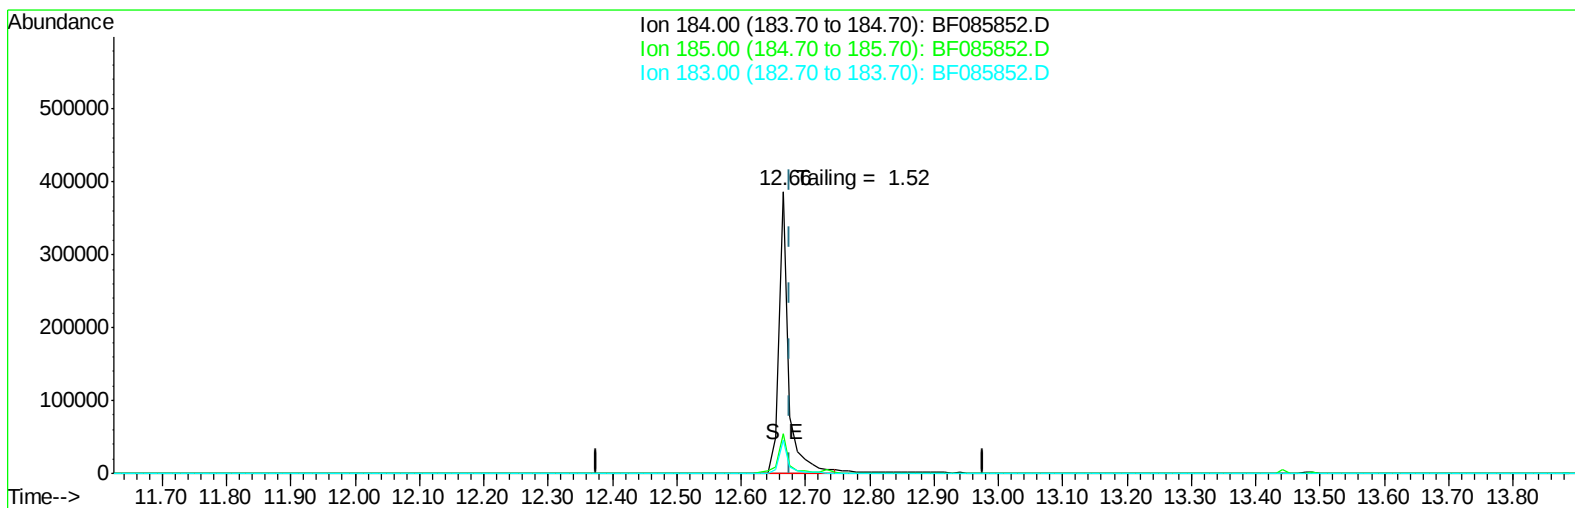

TIC: BF085852.D

(76) Benzidine

12.665min (-0.012) 12798.54ng

response 424592

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.32
183.00	11.80	11.65
0.00	0.00	0.00