


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032916\
 Data File : BF085852.D
 Acq On : 29 Mar 2016 15:52
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 30 12:31:18 2016

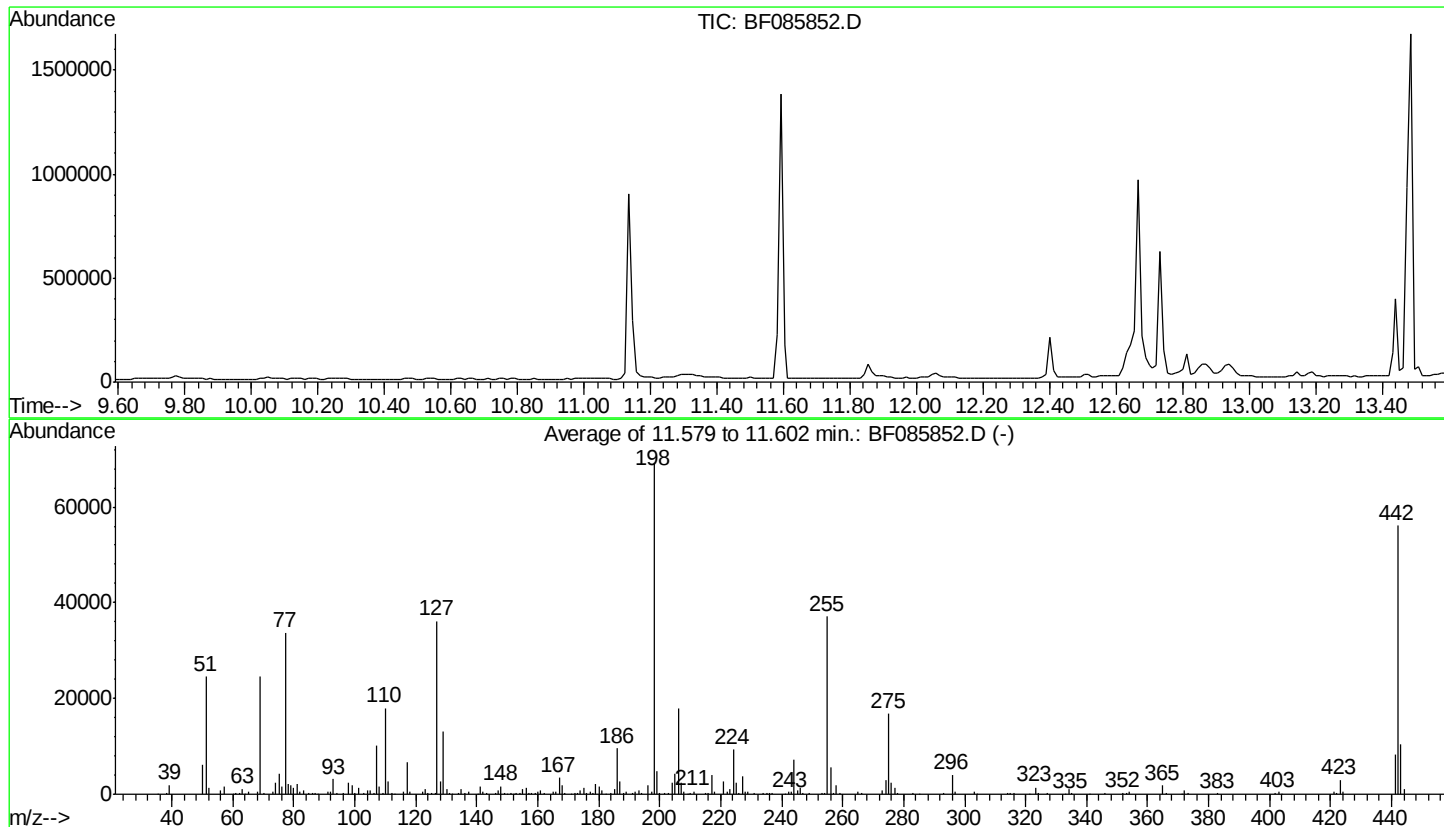

AutoFind: Scans 813, 814, 815; Background Corrected with Scan 810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	24540	PASS
68	69	0.00	2	2.0	490	PASS
69	198	0.00	100	35.4	24519	PASS
70	69	0.00	2	0.7	175	PASS
127	198	10	80	52.2	36173	PASS
197	198	0.00	2	0.7	484	PASS
198	198	100	100	100.0	69243	PASS
199	198	5	9	6.8	4690	PASS
275	198	10	60	24.2	16767	PASS
365	198	1	100	2.7	1837	PASS
441	442	0.01	24	15.0	8413	PASS
442	198	50	100	80.9	56048	PASS
443	442	15	24	18.8	10543	PASS