

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032917\
 Data File : BF094029.D
 Acq On : 29 Mar 2017 20:12
 Operator : SJ/MA
 Sample : I2443-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-BB10-ESW

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.569	101	116	121	rBV	34486	67224	1.86%	0.164%
2	4.063	366	370	376	rVB	260025	337021	9.31%	0.820%
3	4.451	426	436	439	rBV	2870699	2904174	80.18%	7.065%
4	4.681	472	475	483	rVB2	95690	111940	3.09%	0.272%
5	5.404	594	598	604	rVB3	62755	98516	2.72%	0.240%
6	5.516	611	617	620	rBV	2715607	2995911	82.72%	7.288%
7	5.663	635	642	645	rBV	2982255	3166549	87.43%	7.703%
8	5.728	650	653	655	rVV	82670	76020	2.10%	0.185%
9	5.916	681	685	689	rVV	1022014	946952	26.15%	2.304%
10	6.098	711	716	719	rBV	2592077	2538580	70.09%	6.176%
11	6.381	759	764	767	rBV3	53963	75989	2.10%	0.185%
12	6.563	785	795	799	rBV	1797571	2203011	60.83%	5.359%
13	6.857	841	845	851	rVB4	59813	77888	2.15%	0.189%
14	6.992	860	868	871	rBV4	46859	67223	1.86%	0.164%
15	7.422	936	941	943	rBV	1257384	1307666	36.10%	3.181%
16	7.445	943	945	948	rVB	245493	207607	5.73%	0.505%
17	7.592	965	970	974	rVB4	40303	64324	1.78%	0.156%
18	7.981	1029	1036	1041	rVB	129455	157922	4.36%	0.384%
19	8.187	1065	1071	1077	rBV2	73480	107150	2.96%	0.261%
20	8.287	1084	1088	1094	rVB	261287	270768	7.48%	0.659%
21	8.404	1105	1108	1112	rBV	185341	179143	4.95%	0.436%
22	8.745	1158	1166	1169	rBV	3351469	3621856	100.00%	8.811%
23	8.881	1187	1189	1195	rVB	71749	74327	2.05%	0.181%
24	9.057	1216	1219	1223	rVB2	53107	73682	2.03%	0.179%
25	9.145	1228	1234	1237	rBV	117656	162627	4.49%	0.396%
26	9.181	1237	1240	1243	rVV	124227	114385	3.16%	0.278%
27	9.239	1247	1250	1253	rVV	210685	198076	5.47%	0.482%
28	9.281	1253	1257	1264	rVB3	125306	234847	6.48%	0.571%
29	9.386	1271	1275	1280	rBV3	76685	98584	2.72%	0.240%
30	9.563	1301	1305	1309	rVB	1339422	1369951	37.82%	3.333%
31	9.716	1325	1331	1334	rBV6	45307	92086	2.54%	0.224%
32	9.816	1344	1348	1353	rVV2	97862	157727	4.35%	0.384%
33	9.869	1353	1357	1362	rVV3	67268	109556	3.02%	0.267%
34	9.928	1364	1367	1370	rVV3	55160	65691	1.81%	0.160%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032917\
 Data File : BF094029.D
 Acq On : 29 Mar 2017 20:12
 Operator : SJ/MA
 Sample : I2443-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-BB10-ESW

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	9.963	1370	1373	1377	rVV2	64818	105484	2.91%	0.257%
36	10.075	1387	1392	1397	rBV3	90946	125764	3.47%	0.306%
37	10.151	1401	1405	1408	rVV	177615	169923	4.69%	0.413%
38	10.233	1416	1419	1423	rVB	108914	106500	2.94%	0.259%
39	10.428	1448	1452	1455	rBV2	110804	145773	4.02%	0.355%
40	10.533	1464	1470	1476	rVV	1677845	1844659	50.93%	4.487%
41	10.739	1501	1505	1506	rBV	177127	181705	5.02%	0.442%
42	10.757	1506	1508	1512	rVB	177383	172487	4.76%	0.420%
43	11.080	1560	1563	1569	rVB5	58799	97830	2.70%	0.238%
44	11.139	1569	1573	1576	rBV	62297	71630	1.98%	0.174%
45	11.292	1595	1599	1602	rVB	160289	152283	4.20%	0.370%
46	11.327	1602	1605	1609	rVB2	59323	62566	1.73%	0.152%
47	11.386	1610	1615	1617	rBV	1318592	1326410	36.62%	3.227%
48	11.410	1617	1619	1623	rVB	328328	308785	8.53%	0.751%
49	11.475	1627	1630	1634	rVB	55278	63003	1.74%	0.153%
50	11.610	1649	1653	1657	rVB3	37744	64312	1.78%	0.156%
51	11.798	1681	1685	1687	rBV4	58085	81029	2.24%	0.197%
52	11.822	1687	1689	1694	rVB	121517	121487	3.35%	0.296%
53	12.010	1717	1721	1723	rVV	129218	134727	3.72%	0.328%
54	12.039	1723	1726	1732	rVB	237705	280445	7.74%	0.682%
55	12.139	1739	1743	1746	rVV	204994	225977	6.24%	0.550%
56	12.169	1746	1748	1752	rVB	89963	92028	2.54%	0.224%
57	12.327	1772	1775	1778	rVB	91463	90577	2.50%	0.220%
58	12.380	1780	1784	1786	rBV	117774	147856	4.08%	0.360%
59	12.486	1797	1802	1808	rBV6	26402	64927	1.79%	0.158%
60	12.563	1812	1815	1819	rVV	88525	101391	2.80%	0.247%
61	12.598	1819	1821	1824	rVV	87299	90749	2.51%	0.221%
62	12.627	1824	1826	1829	rVB	91584	85049	2.35%	0.207%
63	12.692	1833	1837	1840	rVV	249881	304374	8.40%	0.740%
64	12.727	1840	1843	1846	rVV	110414	148326	4.10%	0.361%
65	12.757	1846	1848	1851	rVV	89709	95850	2.65%	0.233%
66	12.804	1852	1856	1861	rVB2	154489	207756	5.74%	0.505%
67	12.874	1861	1868	1871	rBV	463316	500551	13.82%	1.218%
68	12.904	1871	1873	1878	rVV	70289	75052	2.07%	0.183%
69	12.951	1878	1881	1885	rVV4	72663	103464	2.86%	0.252%
70	13.045	1893	1897	1901	rBV5	46744	74573	2.06%	0.181%
71	13.151	1911	1915	1918	rVB	449748	500054	13.81%	1.216%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032917\
 Data File : BF094029.D
 Acq On : 29 Mar 2017 20:12
 Operator : SJ/MA
 Sample : I2443-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-BB10-ESW

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	13.204	1921	1924	1929	rVB4	48881	85124	2.35%	0.207%
73	13.251	1929	1932	1933	rBV	74566	77004	2.13%	0.187%
74	13.363	1945	1951	1955	rBV	2383786	2788399	76.99%	6.783%
75	13.439	1960	1964	1974	rVB5	73883	169488	4.68%	0.412%
76	13.527	1975	1979	1980	rBV4	56797	65943	1.82%	0.160%
77	13.692	2004	2007	2013	rVB4	115606	198779	5.49%	0.484%
78	13.804	2023	2026	2029	rVB	79656	81420	2.25%	0.198%
79	13.839	2029	2032	2040	rBV4	49202	93617	2.58%	0.228%
80	14.133	2079	2082	2085	rVV2	79407	82115	2.27%	0.200%
81	14.186	2088	2091	2098	rVB	131048	171815	4.74%	0.418%
82	14.321	2110	2114	2119	rBV2	100568	132249	3.65%	0.322%
83	14.527	2145	2149	2160	rBV5	172441	376641	10.40%	0.916%
84	14.639	2162	2168	2171	rVV	1041315	1400634	38.67%	3.407%
85	14.663	2171	2172	2176	rVB	210760	183165	5.06%	0.446%
86	14.751	2184	2187	2191	rVB3	50491	69824	1.93%	0.170%
87	14.833	2198	2201	2205	rVB4	40474	64490	1.78%	0.157%
88	14.933	2213	2218	2220	rBV3	73107	102437	2.83%	0.249%
89	15.115	2244	2249	2253	rBV	89279	132626	3.66%	0.323%
90	15.157	2253	2256	2260	rVV2	62833	69770	1.93%	0.170%
91	15.310	2280	2282	2287	rVB	79051	83242	2.30%	0.203%
92	15.674	2340	2344	2347	rBV	74954	87160	2.41%	0.212%
93	15.857	2371	2375	2378	rBV	192366	272443	7.52%	0.663%
94	16.027	2401	2404	2409	rBV	65647	74643	2.06%	0.182%
95	16.145	2421	2424	2428	rVB	106858	114528	3.16%	0.279%
96	16.204	2431	2434	2438	rVB	127804	143423	3.96%	0.349%
97	16.268	2440	2445	2449	rBV	702791	814818	22.50%	1.982%
98	17.268	2611	2615	2625	rBV5	34319	90892	2.51%	0.221%
99	17.615	2669	2674	2683	rVB3	58632	117738	3.25%	0.286%
100	18.015	2736	2742	2748	rVB	50834	102140	2.82%	0.248%


Sum of corrected areas: 41106896

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032917\
Data File : BF094029.D
Acq On : 29 Mar 2017 20:12
Operator : SJ/MA
Sample : I2443-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-BB10-ESW

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

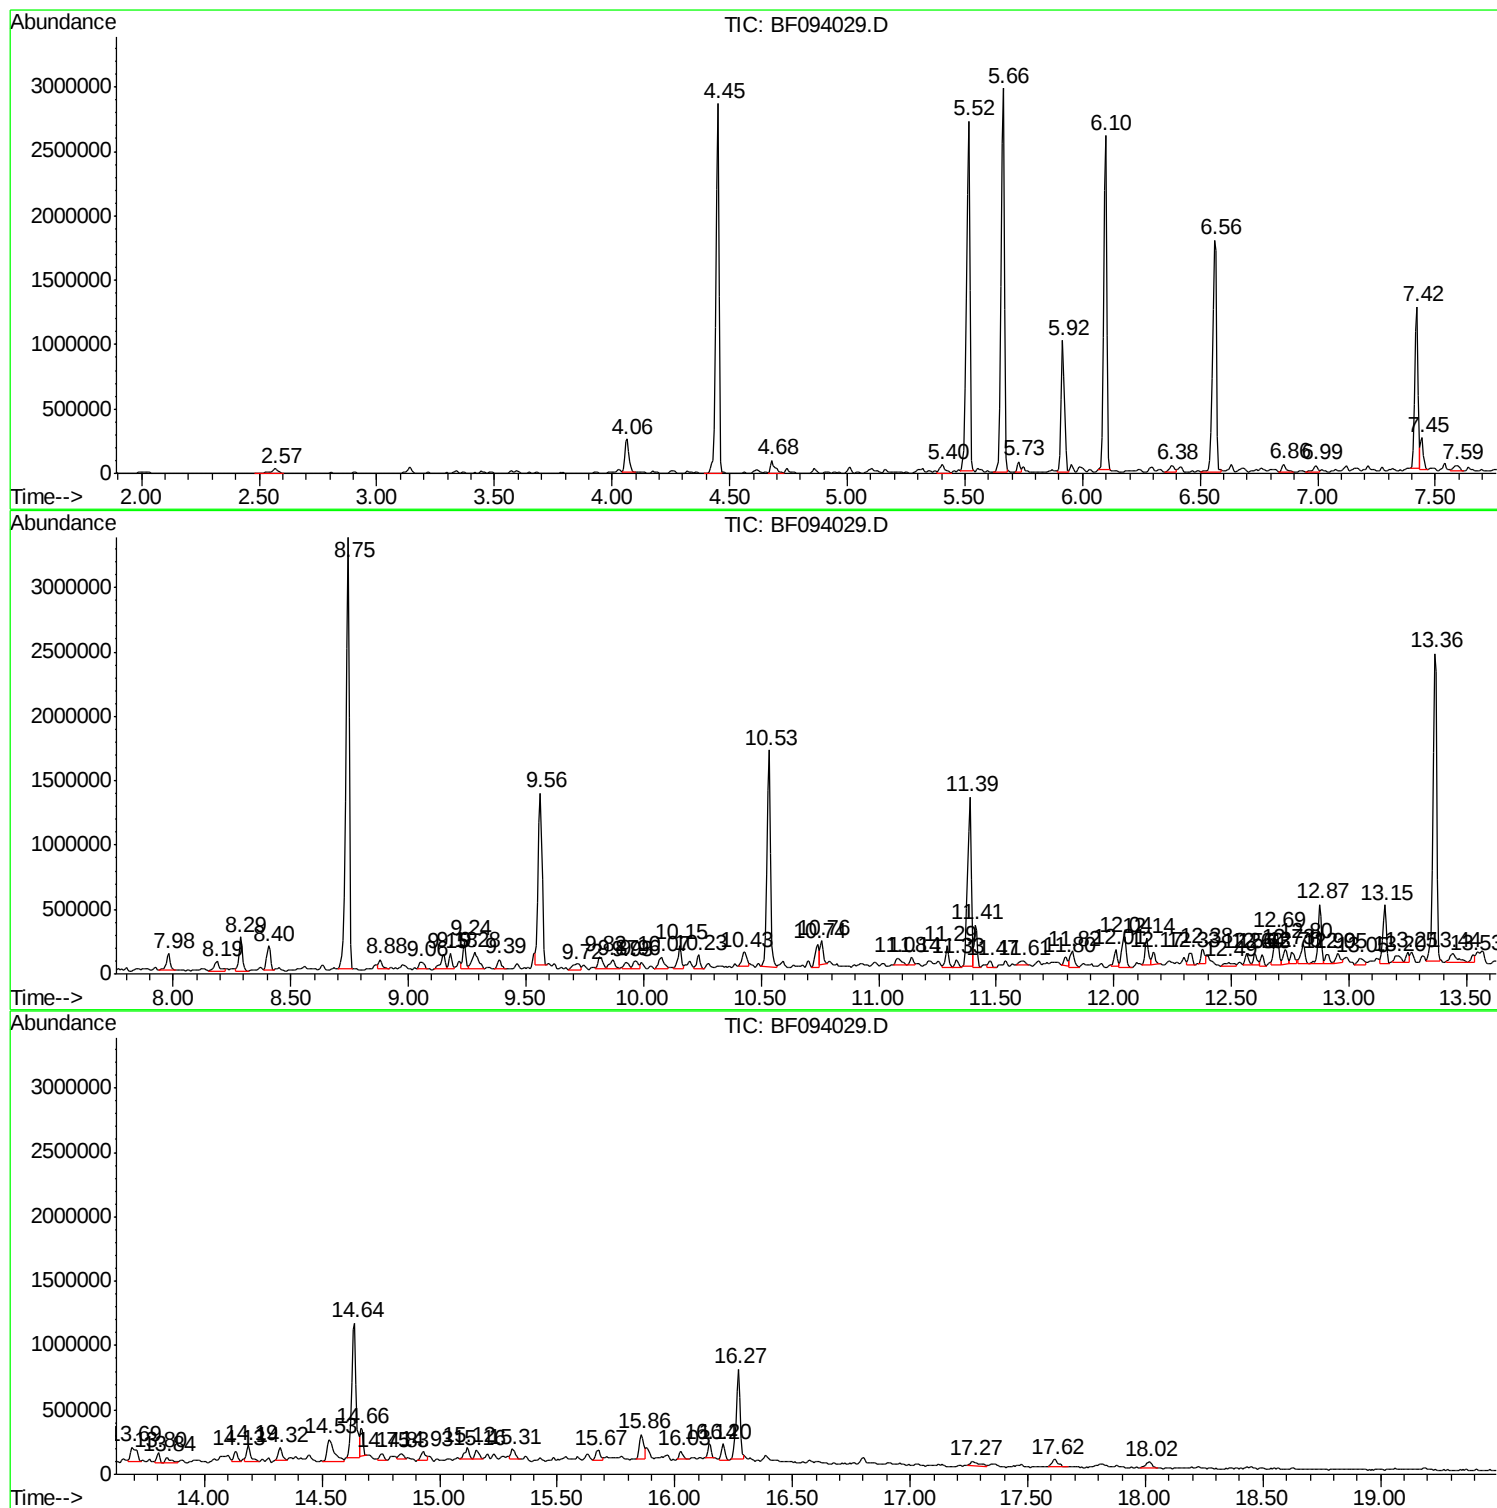

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF032917\
Data_File : BF094029.D
Acq_On : 29-Mar-2017 20:122
Operator : SJ/MAA
Sample : I2443-077
Misc :
ALS_Vial : 13 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
E2-BB10-ESW

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
