


Data Path : Z:\HPCHEM1\BNA F\DATA\BF032917\
 Data File : BF094017.D
 Acq On : 29 Mar 2017 14:16
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 27 16:10:49 2017

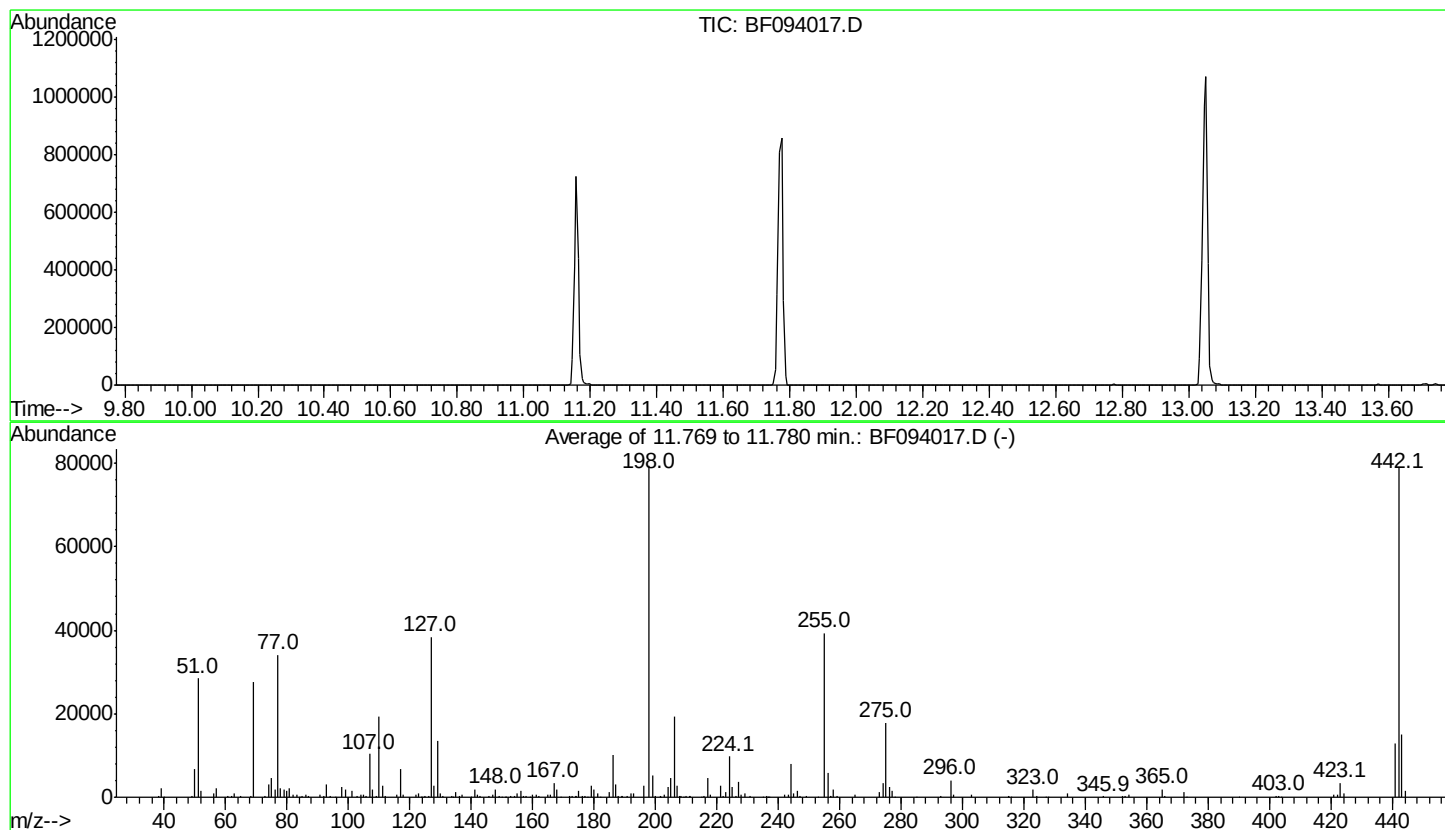

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1674

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	28511	PASS
68	69	0.00	2	1.5	420	PASS
69	198	0.00	100	34.9	27699	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.3	38398	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	79434	PASS
199	198	5	9	6.5	5187	PASS
275	198	10	60	22.5	17871	PASS
365	198	1	100	2.4	1939	PASS
441	442	0.01	24	16.2	12780	PASS
442	198	50	100	99.4	78970	PASS
443	442	15	24	19.0	14982	PASS