


Data Path : Z:\HPCHEM1\BNA F\DATA\BF032917\
 Data File : BF094043.D
 Acq On : 30 Mar 2017 4:25
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 27 16:10:49 2017

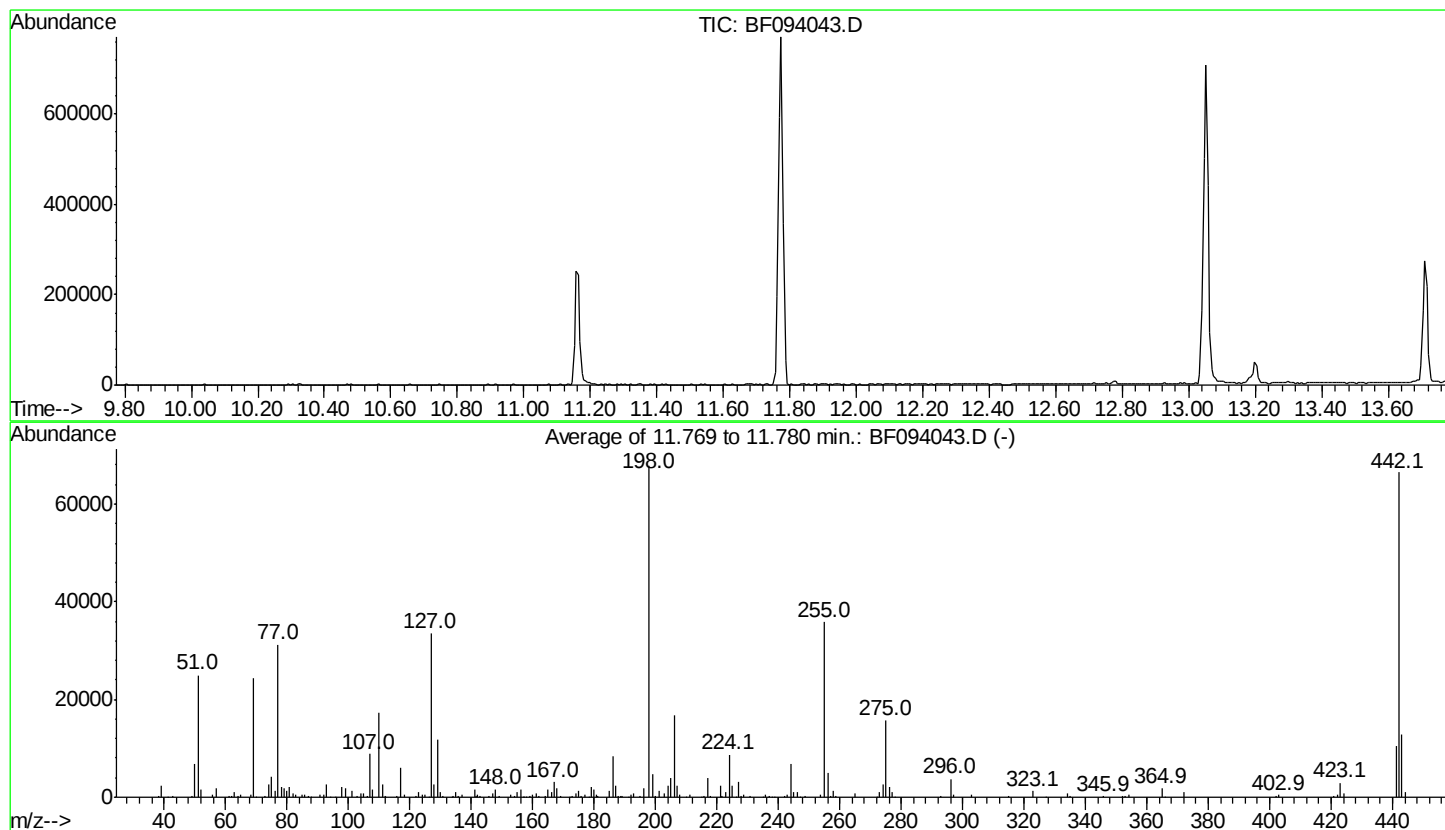

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1674

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	24980	PASS
68	69	0.00	2	1.7	413	PASS
69	198	0.00	100	36.0	24460	PASS
70	69	0.00	2	0.5	111	PASS
127	198	10	80	49.4	33528	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67858	PASS
199	198	5	9	6.8	4615	PASS
275	198	10	60	23.0	15608	PASS
365	198	1	100	2.6	1795	PASS
441	442	0.01	24	15.8	10525	PASS
442	198	50	100	97.9	66432	PASS
443	442	15	24	19.2	12734	PASS