
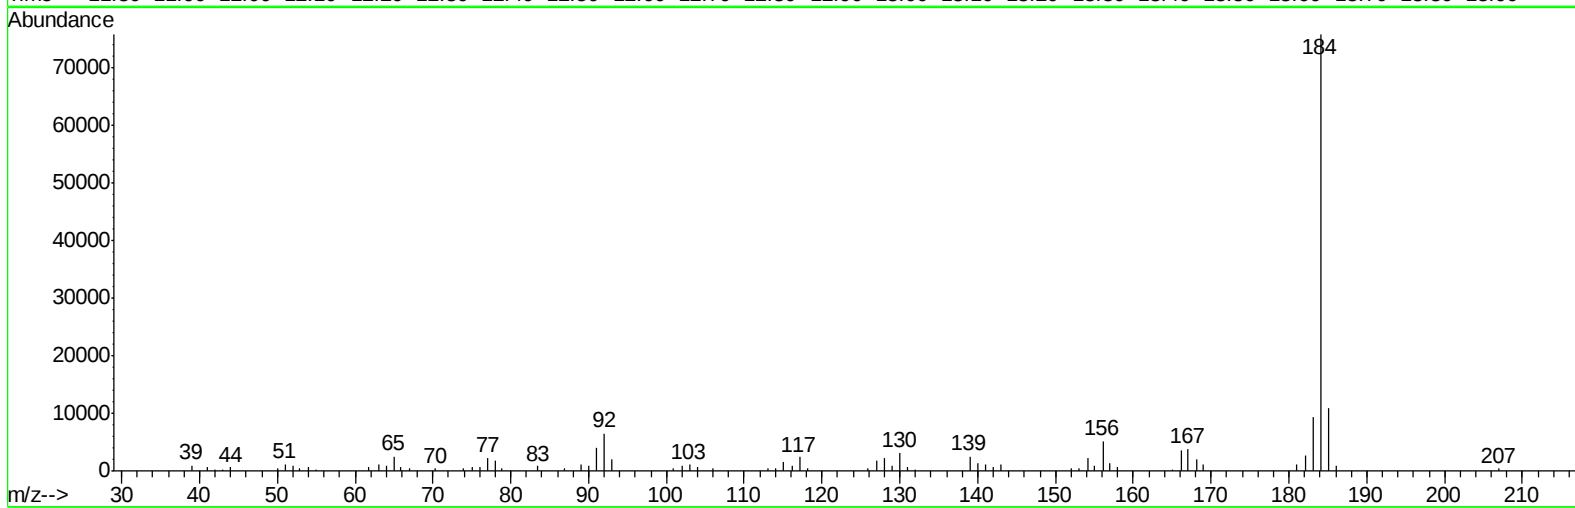


Data Path : Z:\HPCHEM1\BNA F\DATA\BF032918\
Data File : BF104070.D
Acq On : 30 Mar 2018 00:38
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 08:59:18 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 13:41:47 2018
Response via : Initial Calibration

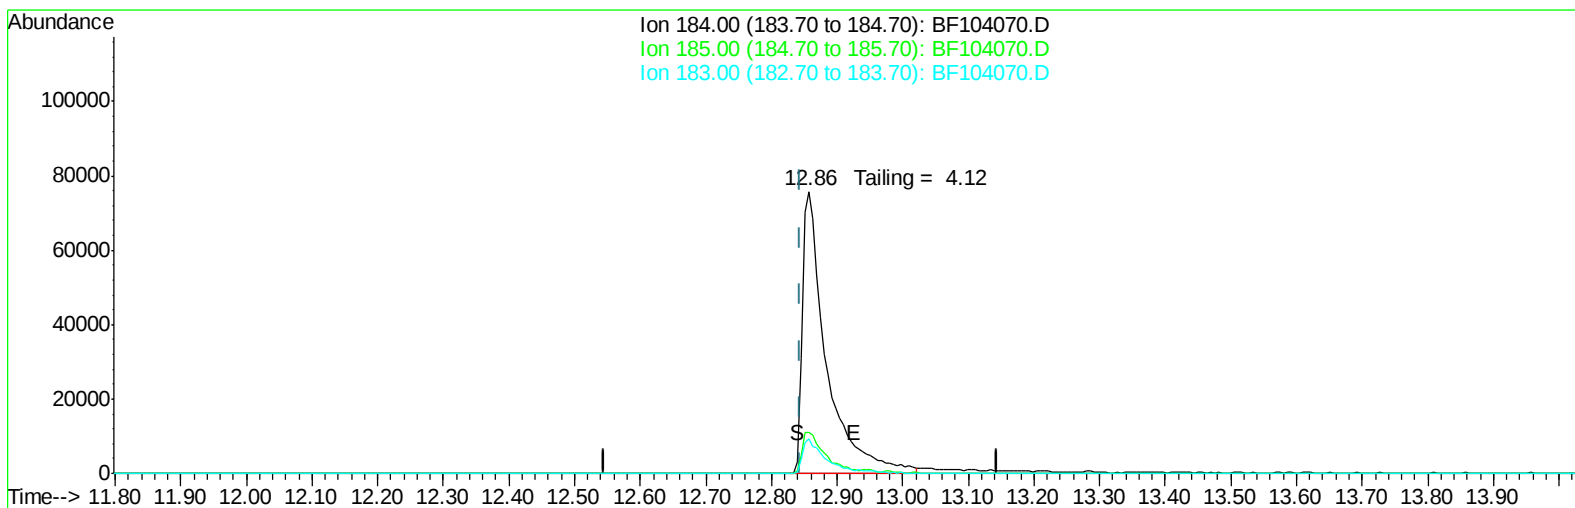

TIC: BF104070.D

(76) Benzidine



12.857min (+0.012) 0.00ng

response 193978

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.39
183.00	11.60	12.37
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032918\
Data File : BF104070.D
Acq On : 30 Mar 2018 00:38
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 08:59:18 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 13:41:47 2018
Response via : Initial Calibration

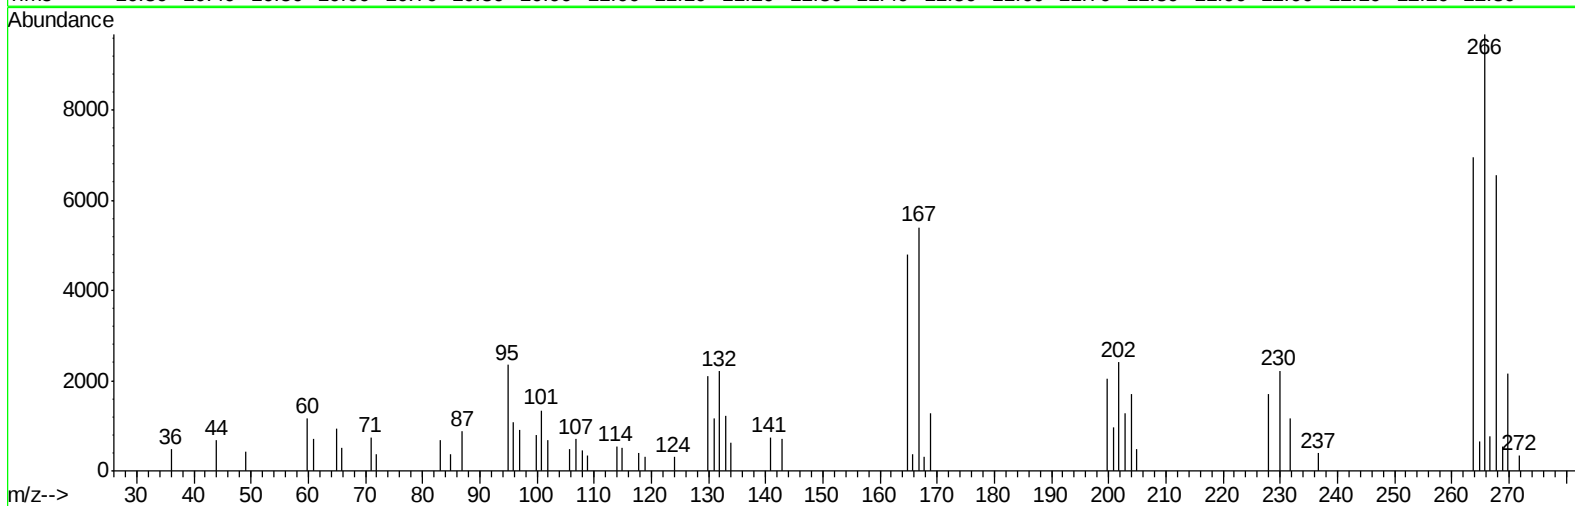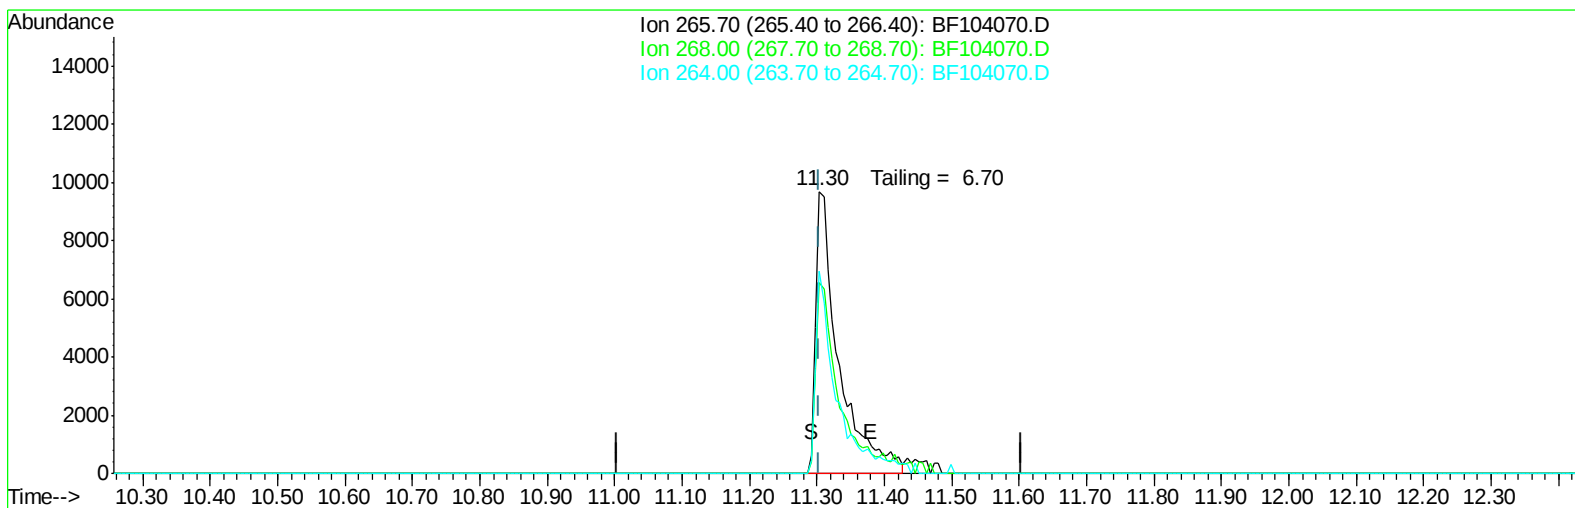

TIC: BF104070.D

(69) Pentachlorophenol (C)

11.304min (-0.000) 27876.50ng

response 22465

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.80
264.00	61.90	71.93
0.00	0.00	0.00