

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032918\
 Data File : BF104080.D
 Acq On : 30 Mar 2018 5:17
 Operator : JU/SJ
 Sample : J2092-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-01-B02-B02A-C02-C02A

Quant Time: Mar 30 07:27:13 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 28 13:41:47 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	97672	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	396595	20.00	ng	0.00
38) Acenaphthene-d10	10.00	164	165640	20.00	ng	0.00
63) Phenanthrene-d10	11.50	188	242338	20.00	ng	0.00
75) Chrysene-d12	14.16	240	218363	20.00	ng	0.00
86) Perylene-d12	15.70	264	204696	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	596566	97.40	ng	0.00
7) Phenol-d6	6.60	99	806887	107.08	ng	0.00
23) Nitrobenzene-d5	7.53	82	471173	72.66	ng	0.00
41) 2,4,6-Tribromophenol	10.80	330	143786	77.96	ng	0.00
44) 2-Fluorobiphenyl	9.32	172	846052	80.55	ng	0.00
78) Terphenyl-d14	13.08	244	558794	59.09	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.71	163	50027	3.825	ng	Qvalue # 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032918\
Data File : BF104080.D
Acq On : 30 Mar 2018 5:17
Operator : JU/SJ
Sample : J2092-01
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-BPM-01-B02-B02A-C02-C02A

Quant Time: Mar 30 07:27:13 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 13:41:47 2018
Response via : Initial Calibration

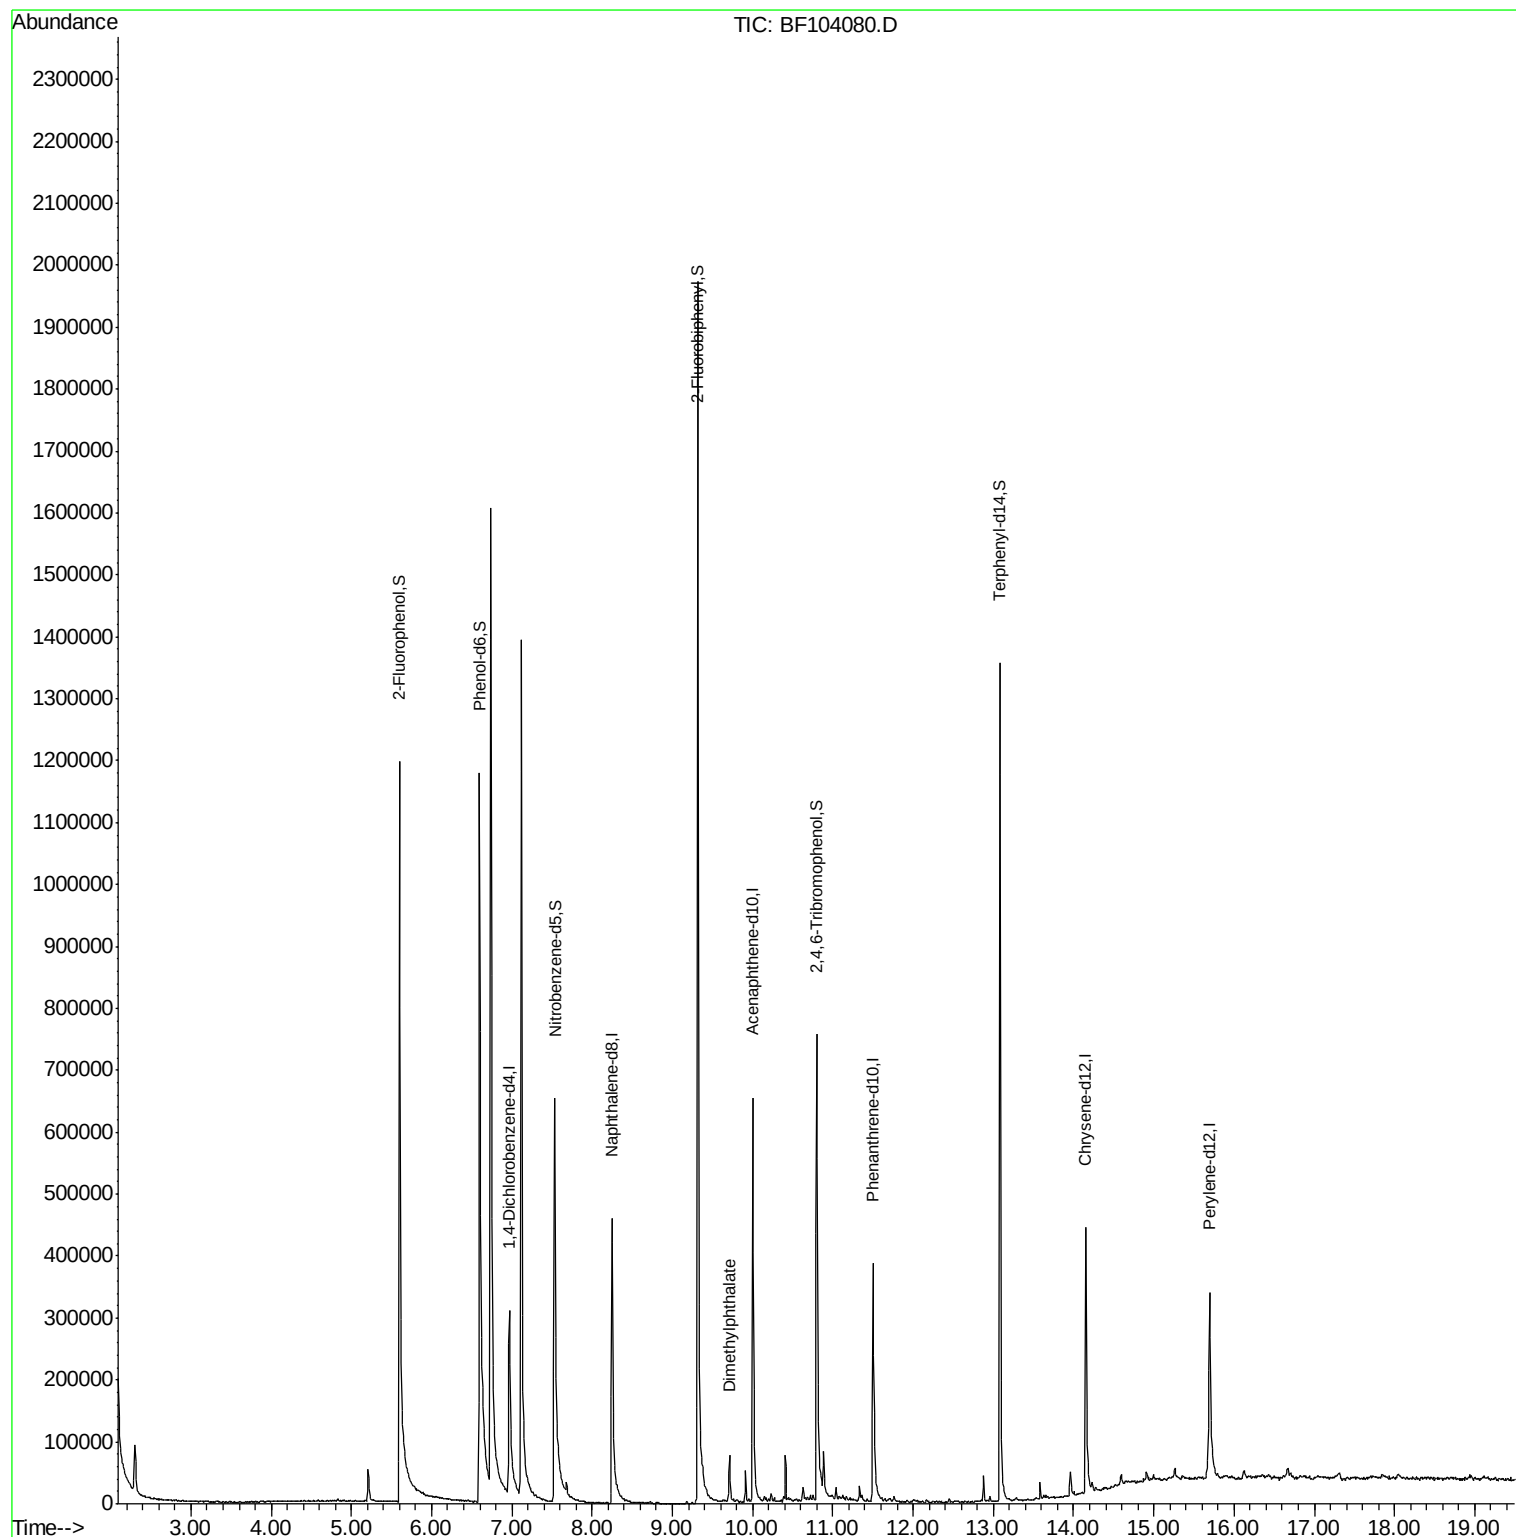

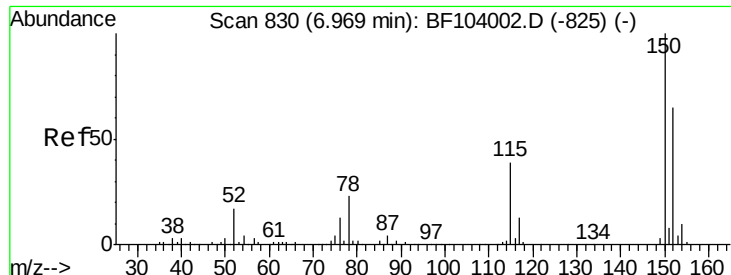


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 830
Delta R.T. -0.00 min
Lab File: BF104080.D
Acq: 30 Mar 2018 5:17

Instrument :
BNA_F
ClientSampleId :
FK-BPM-01-B02-B02A-C02-C02A

Tot Ion:152 Resp: 97672
Ion Ratio Lower Upper
152 100
150 157.9 124.6 186.8
115 59.8 50.1 75.1

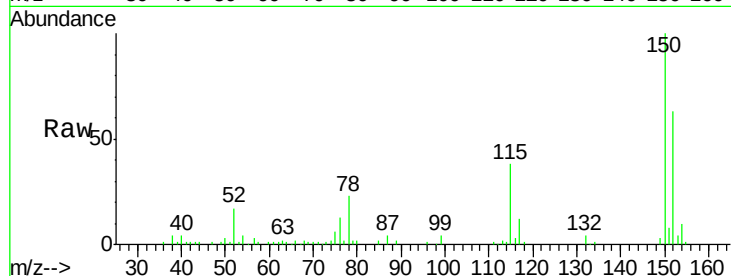


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

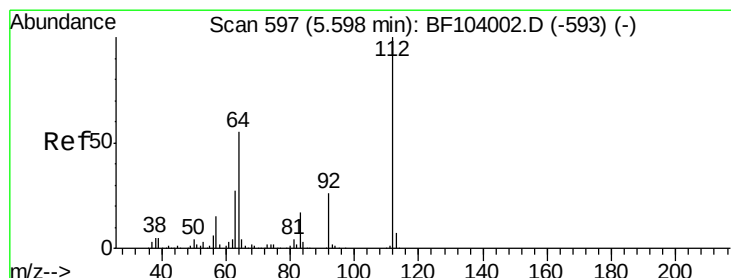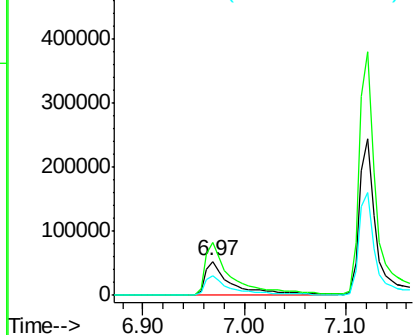



#5


2-Fluorophenol
Concen: 97.405 ng
RT: 5.60 min Scan# 597
Delta R.T. -0.00 min
Lab File: BF104080.D
Acq: 30 Mar 2018 5:17

Tgt Ion:112 Resp: 596566
Ion Ratio Lower Upper
112 100
64 55.5 47.9 71.9
63 28.3 23.7 35.5

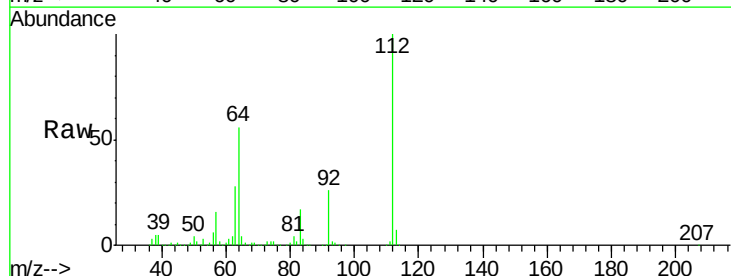

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

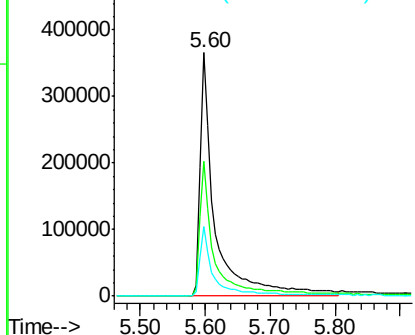

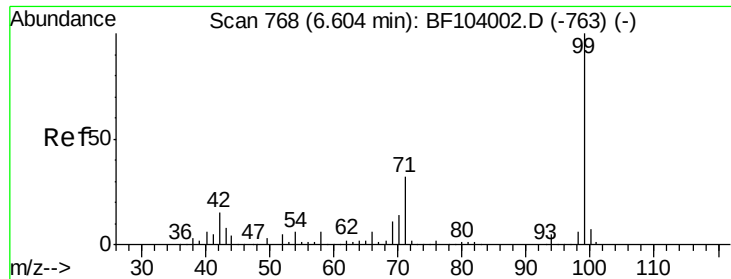

#7

Phenol-d6

Concen: 107.084 ng

RT: 6.60 min Scan# 767

Delta R.T. -0.01 min

Lab File: BF104080.D

Acq: 30 Mar 2018 5:17

Instrument :

BNA_F

ClientSampleId :

FK-BPM-01-B02-B02A-C02-C02A


Tot Ion: 99 Resp: 806887

Ion Ratio Lower Upper




99 100

42 14.6 14.5 21.7

71 32.3 25.4 38.0

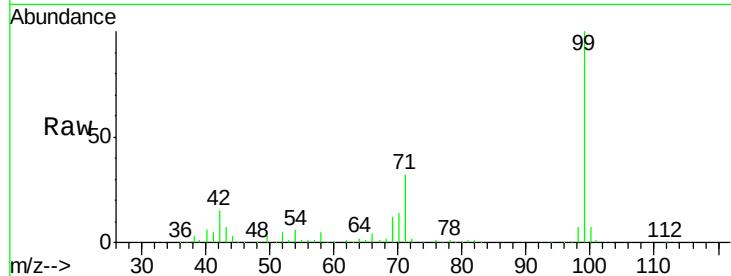

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

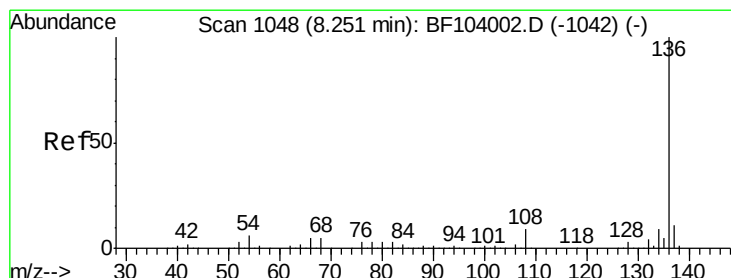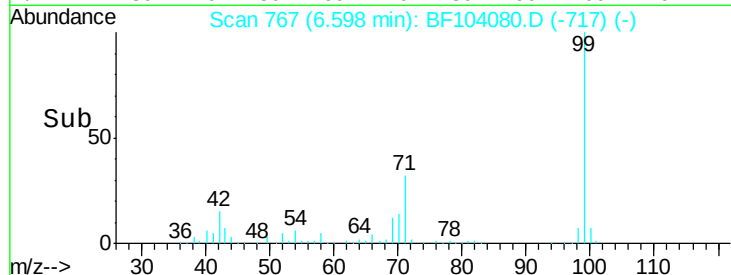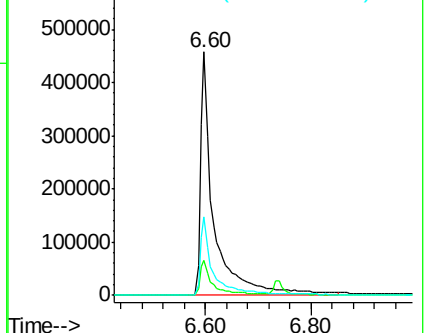

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.25 min Scan# 1047

Delta R.T. -0.01 min

Lab File: BF104080.D

Acq: 30 Mar 2018 5:17

Tgt Ion: 136 Resp: 396595


Ion Ratio Lower Upper

136 100



137 11.0 8.9 13.3


54 7.2 6.6 9.8

68 5.9 5.0 7.4

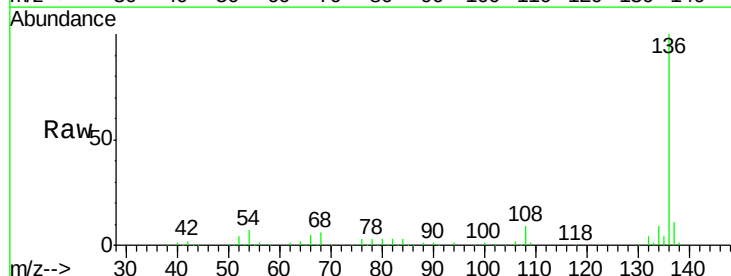

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

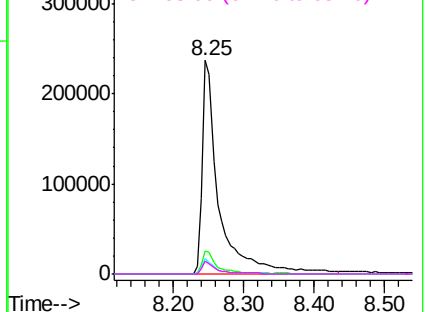


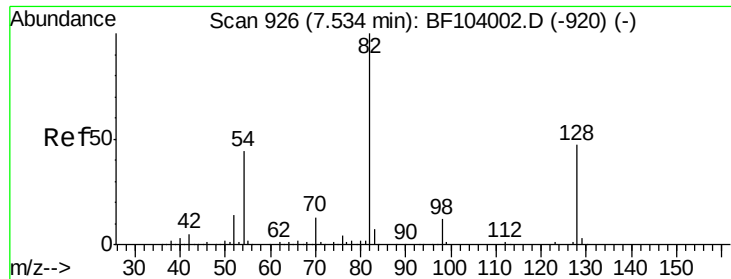




#23
Nitrobenzene-d5
Concen: 72.656 ng
RT: 7.53 min Scan# 926
Delta R.T. -0.00 min
Lab File: BF104080.D
Acq: 30 Mar 2018 5:17

Instrument :
BNA_F
ClientSampleId :
FK-BPM-01-B02-B02A-C02-C02A

Tot Ion: 82 Resp: 471173
Ion Ratio Lower Upper
82 100
128 49.3 36.1 54.1
54 43.1 41.4 62.2

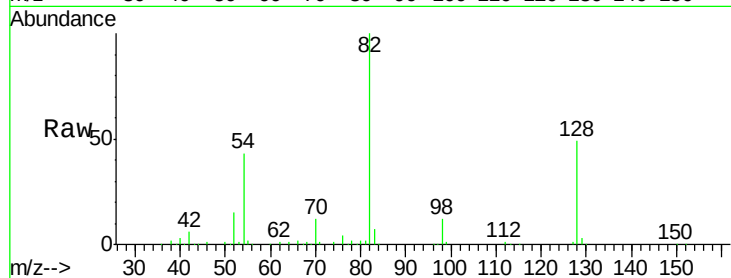


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

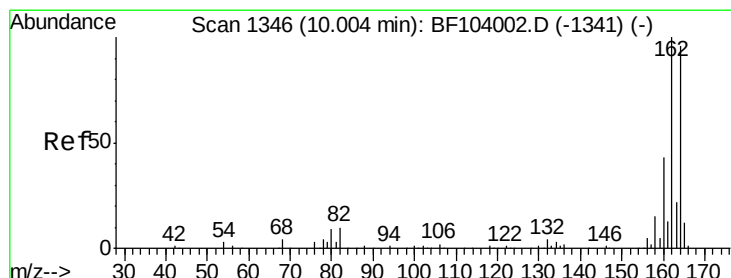
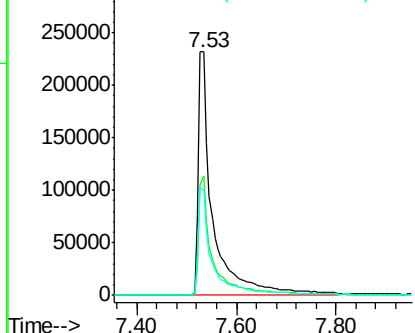



#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.00 min Scan# 1346
Delta R.T. -0.00 min
Lab File: BF104080.D
Acq: 30 Mar 2018 5:17

Tgt Ion:164 Resp: 165640
Ion Ratio Lower Upper
164 100
162 104.4 86.1 129.1
160 45.0 38.3 57.5

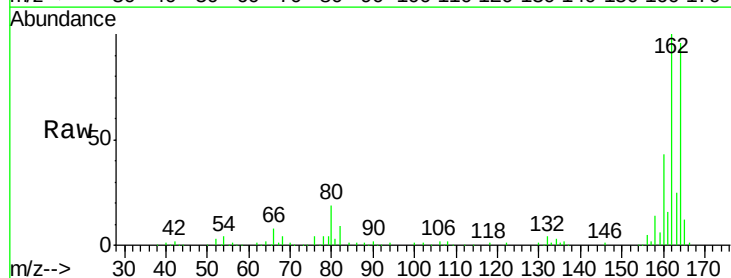

Abundance Ion 164.00 (163.70 to 164.70): BF1
Ion 162.00 (161.70 to 162.70): BF1
Ion 160.00 (159.70 to 160.70): BF1

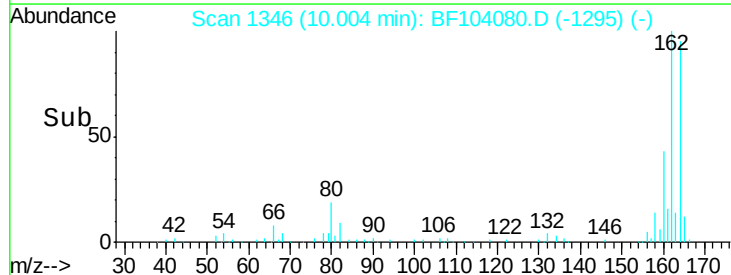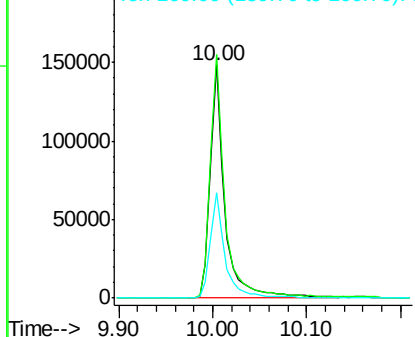







#41
 2,4,6-Tribromophenol
 Concen: 77.958 ng
 RT: 10.80 min Scan# 1481
 Delta R.T. -0.01 min
 Lab File: BF104080.D
 Acq: 30 Mar 2018 5:17

Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-01-B02-B02A-C02-C02A

Tot Ion:330 Resp: 143786
 Ion Ratio Lower Upper
 330 100
 332 97.3 77.0 115.6
 141 32.6 29.9 44.9

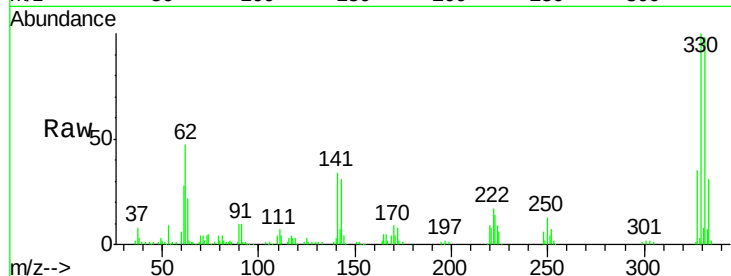


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

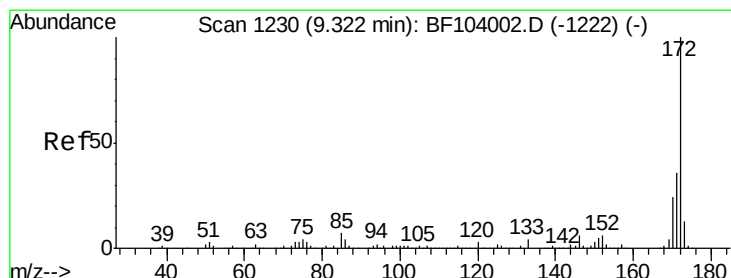
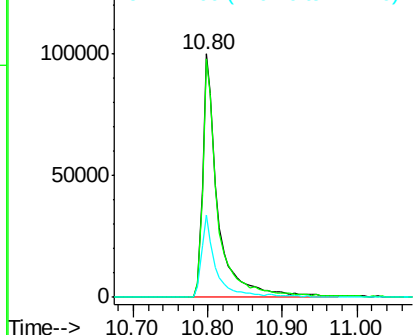



#44
 2-Fluorobiphenyl
 Concen: 80.545 ng
 RT: 9.32 min Scan# 1229
 Delta R.T. -0.01 min
 Lab File: BF104080.D
 Acq: 30 Mar 2018 5:17

Tgt Ion:172 Resp: 846052
 Ion Ratio Lower Upper
 172 100
 171 36.7 29.7 44.5
 170 23.1 19.6 29.4

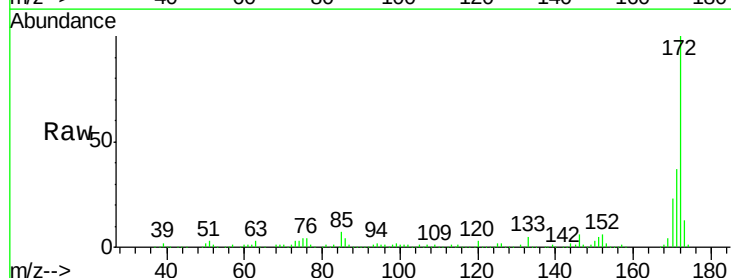

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

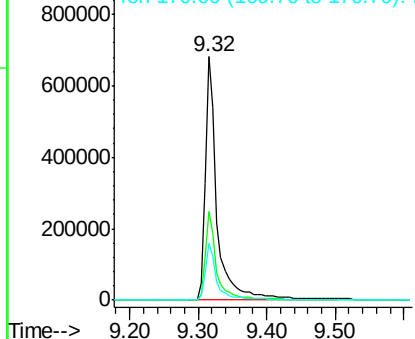



#49

Dimethylphthalate

Concen: 3.825 ng

RT: 9.71 min Scan# 1296

Delta R.T. -0.01 min

Lab File: BF104080.D

Acq: 30 Mar 2018 5:17

Instrument :

BNA_F

ClientSampleId :

FK-BPM-01-B02-B02A-C02-C02A


Tot Ion:163 Resp: 50027

Ion Ratio Lower Upper

163 100

194 4.5 2.7 4.1#




164 10.4 8.2 12.2

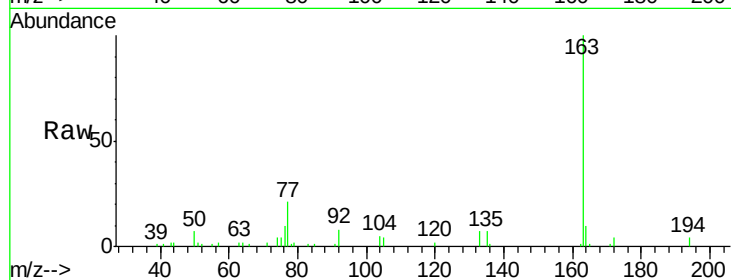

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

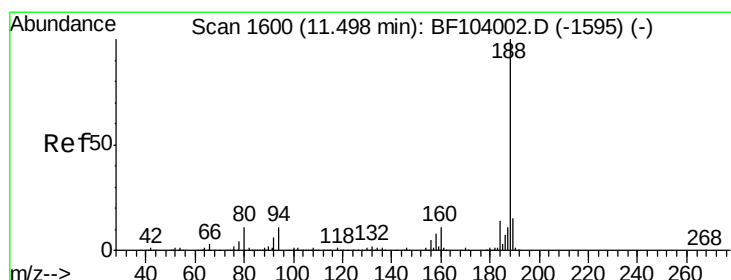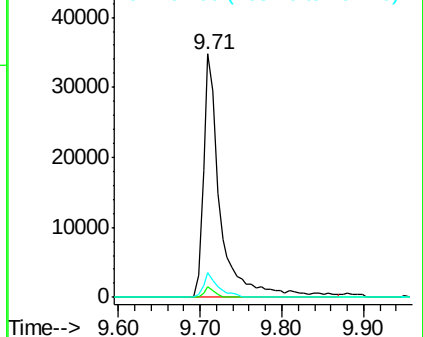

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.50 min Scan# 1601

Delta R.T. 0.01 min

Lab File: BF104080.D

Acq: 30 Mar 2018 5:17


Tgt Ion:188 Resp: 242338

Ion Ratio Lower Upper

188 100

94 9.1 8.5 12.7



80 10.0 9.2 13.8

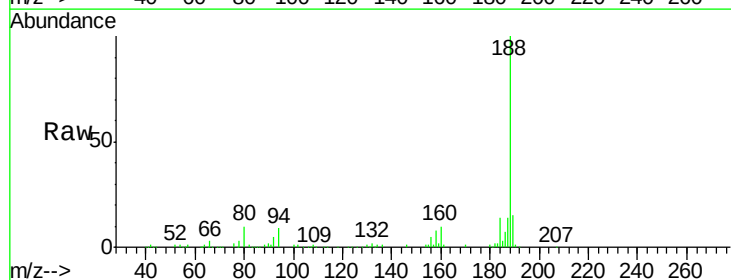


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

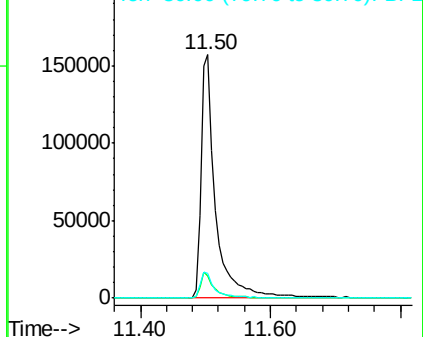

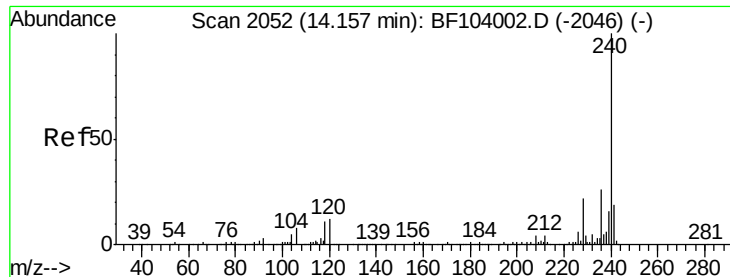

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.16 min Scan# 2052

Delta R.T. -0.00 min

Lab File: BF104080.D

Acq: 30 Mar 2018 5:17

Instrument :

BNA_F

ClientSampleId :

FK-BPM-01-B02-B02A-C02-C02A


Tot Ion:240 Resp: 218363

Ion Ratio Lower Upper

240 100

120 11.3 9.5 14.3




236 25.2 20.7 31.1

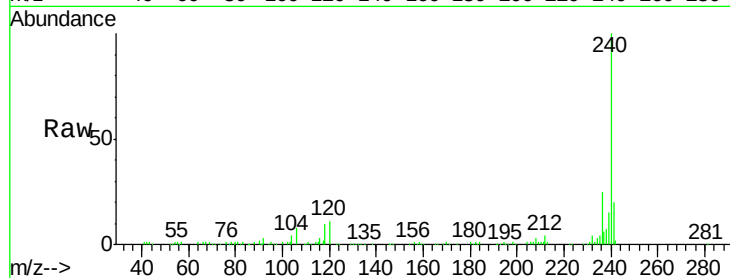

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

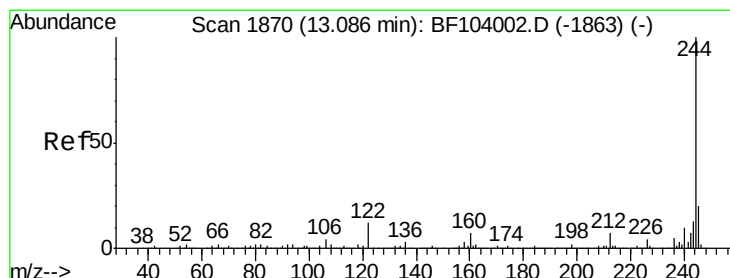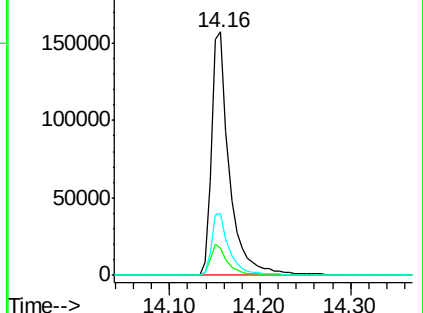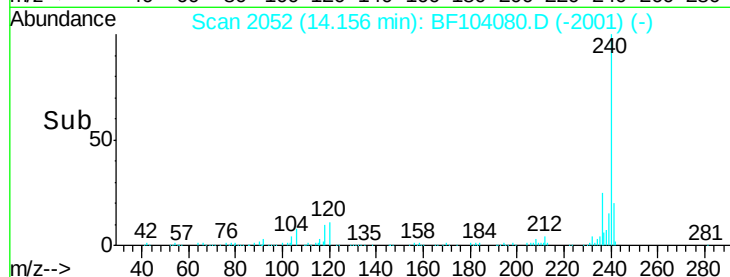

#78

Terphenyl-d14

Concen: 59.086 ng

RT: 13.08 min Scan# 1869

Delta R.T. -0.01 min

Lab File: BF104080.D

Acq: 30 Mar 2018 5:17


Tgt Ion:244 Resp: 558794

Ion Ratio Lower Upper

244 100

212 6.6 5.4 8.0



122 13.2 11.0 16.4

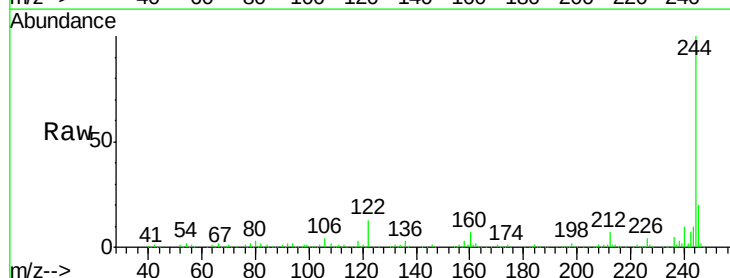


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

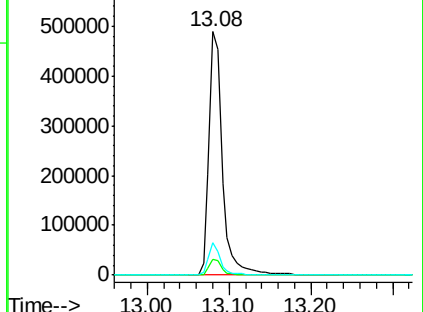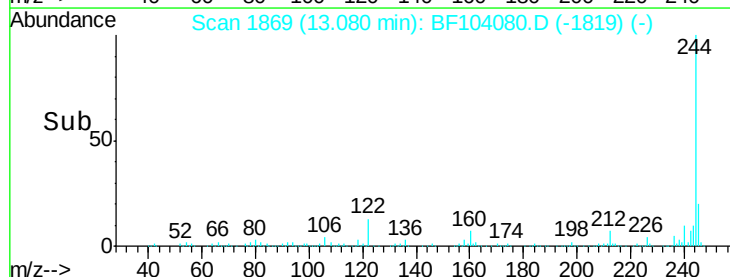


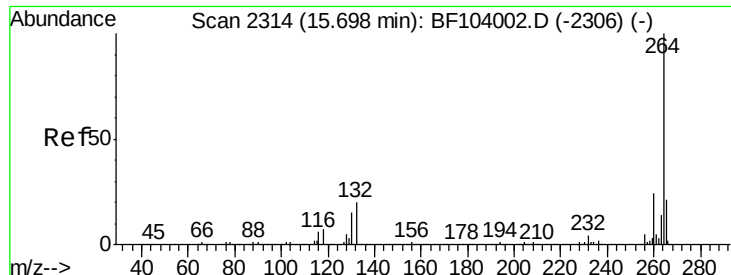

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.70 min Scan# 2314
 Delta R.T. -0.00 min
 Lab File: BF104080.D
 Acq: 30 Mar 2018 5:17

Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-01-B02-B02A-C02-C02A

Tot Ion:	264	Resp:	204696
Ion	Ratio	Lower	Upper
264	100		
260	23.6	19.2	28.8
265	21.6	17.5	26.3

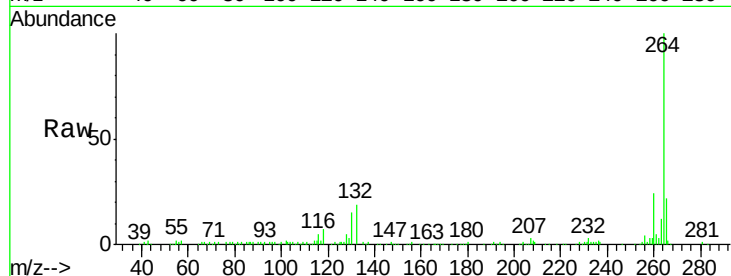

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

