

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032918\
 Data File : BF104052.D
 Acq On : 29 Mar 2018 15:49
 Operator : JU/SJ
 Sample : J2120-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BES-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.293	30	35	45	rVB	73615	102510	3.98%	0.447%
2	5.198	525	529	538	rBV	201183	270659	10.50%	1.181%
3	5.598	593	597	625	rBV	822417	1509667	58.58%	6.587%
4	6.598	763	767	787	rBV	1077206	1893110	73.46%	8.260%
5	6.734	787	790	822	rVV	1366005	2167485	84.11%	9.457%
6	6.969	826	830	852	rVV	354741	635310	24.65%	2.772%
7	7.122	852	856	879	rVV	1330527	1672570	64.90%	7.297%
8	7.528	922	925	949	rBV	703333	1262216	48.98%	5.507%
9	7.681	949	951	962	rVB3	20037	30710	1.19%	0.134%
10	8.245	1044	1047	1069	rBV	626539	889148	34.50%	3.879%
11	9.316	1225	1229	1245	rBV	2180622	2577079	100.00%	11.244%
12	9.710	1289	1296	1303	rBV	140075	159755	6.20%	0.697%
13	9.910	1327	1330	1334	rBV	49049	42250	1.64%	0.184%
14	10.004	1340	1346	1359	rBV	913979	1017179	39.47%	4.438%
15	10.386	1408	1411	1413	rBV	30622	30267	1.17%	0.132%
16	10.410	1413	1415	1419	rVB	83526	68064	2.64%	0.297%
17	10.633	1446	1453	1455	rBV	23092	31625	1.23%	0.138%
18	10.798	1477	1481	1493	rBV	682954	895571	34.75%	3.907%
19	10.886	1493	1496	1501	rVB	85513	92639	3.59%	0.404%
20	11.333	1570	1572	1575	rBV	63543	52837	2.05%	0.231%
21	11.498	1597	1600	1603	rBV	712305	806935	31.31%	3.521%
22	11.580	1611	1614	1617	rVB	36531	37126	1.44%	0.162%
23	11.763	1643	1645	1648	rVB	58459	44389	1.72%	0.194%
24	12.116	1702	1705	1708	rBV2	21478	27376	1.06%	0.119%
25	12.169	1711	1714	1717	rVB2	41584	35872	1.39%	0.157%
26	12.333	1739	1742	1746	rVB4	21224	27220	1.06%	0.119%
27	12.516	1770	1773	1777	rBV4	23884	30130	1.17%	0.131%
28	12.557	1777	1780	1784	rBV2	32329	33407	1.30%	0.146%
29	12.721	1804	1808	1815	rVB	271029	310975	12.07%	1.357%
30	12.951	1841	1847	1852	rBV	201800	286599	11.12%	1.250%
31	13.086	1865	1870	1877	rBV	1865396	2048903	79.50%	8.939%
32	13.286	1901	1904	1907	rVB2	81109	84517	3.28%	0.369%
33	13.633	1960	1963	1965	rBV	113333	88826	3.45%	0.388%
34	13.963	2015	2019	2025	rBV	328313	347034	13.47%	1.514%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032918\
Data File : BF104052.D
Acq On : 29 Mar 2018 15:49
Operator : JU/SJ
Sample : J2120-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BES-2

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	14.104	2040	2043	2047	rBV	104738	91346	3.54%	0.399%
36	14.157	2047	2052	2055	rBV	623749	758600	29.44%	3.310%
37	14.280	2070	2073	2076	rVB	146452	127107	4.93%	0.555%
38	14.592	2123	2126	2133	rBV	201705	229584	8.91%	1.002%
39	14.915	2178	2181	2186	rVB	124517	132947	5.16%	0.580%
40	15.239	2233	2236	2238	rBV	70711	94253	3.66%	0.411%
41	15.268	2238	2241	2245	rVB	238685	282434	10.96%	1.232%
42	15.562	2289	2291	2296	rVB	48665	60082	2.33%	0.262%
43	15.674	2307	2310	2311	rBV2	58737	69292	2.69%	0.302%
44	15.704	2311	2315	2326	rVB	364513	623382	24.19%	2.720%
45	16.133	2384	2388	2395	rVB	111744	164689	6.39%	0.719%
46	18.468	2781	2785	2800	rVB9	88660	238681	9.26%	1.041%
47	18.739	2823	2831	2851	rVB6	128589	437966	16.99%	1.911%


Sum of corrected areas: 22920323

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032918\
Data File : BF104052.D
Acq On : 29 Mar 2018 15:49
Operator : JU/SJ
Sample : J2120-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
BES-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

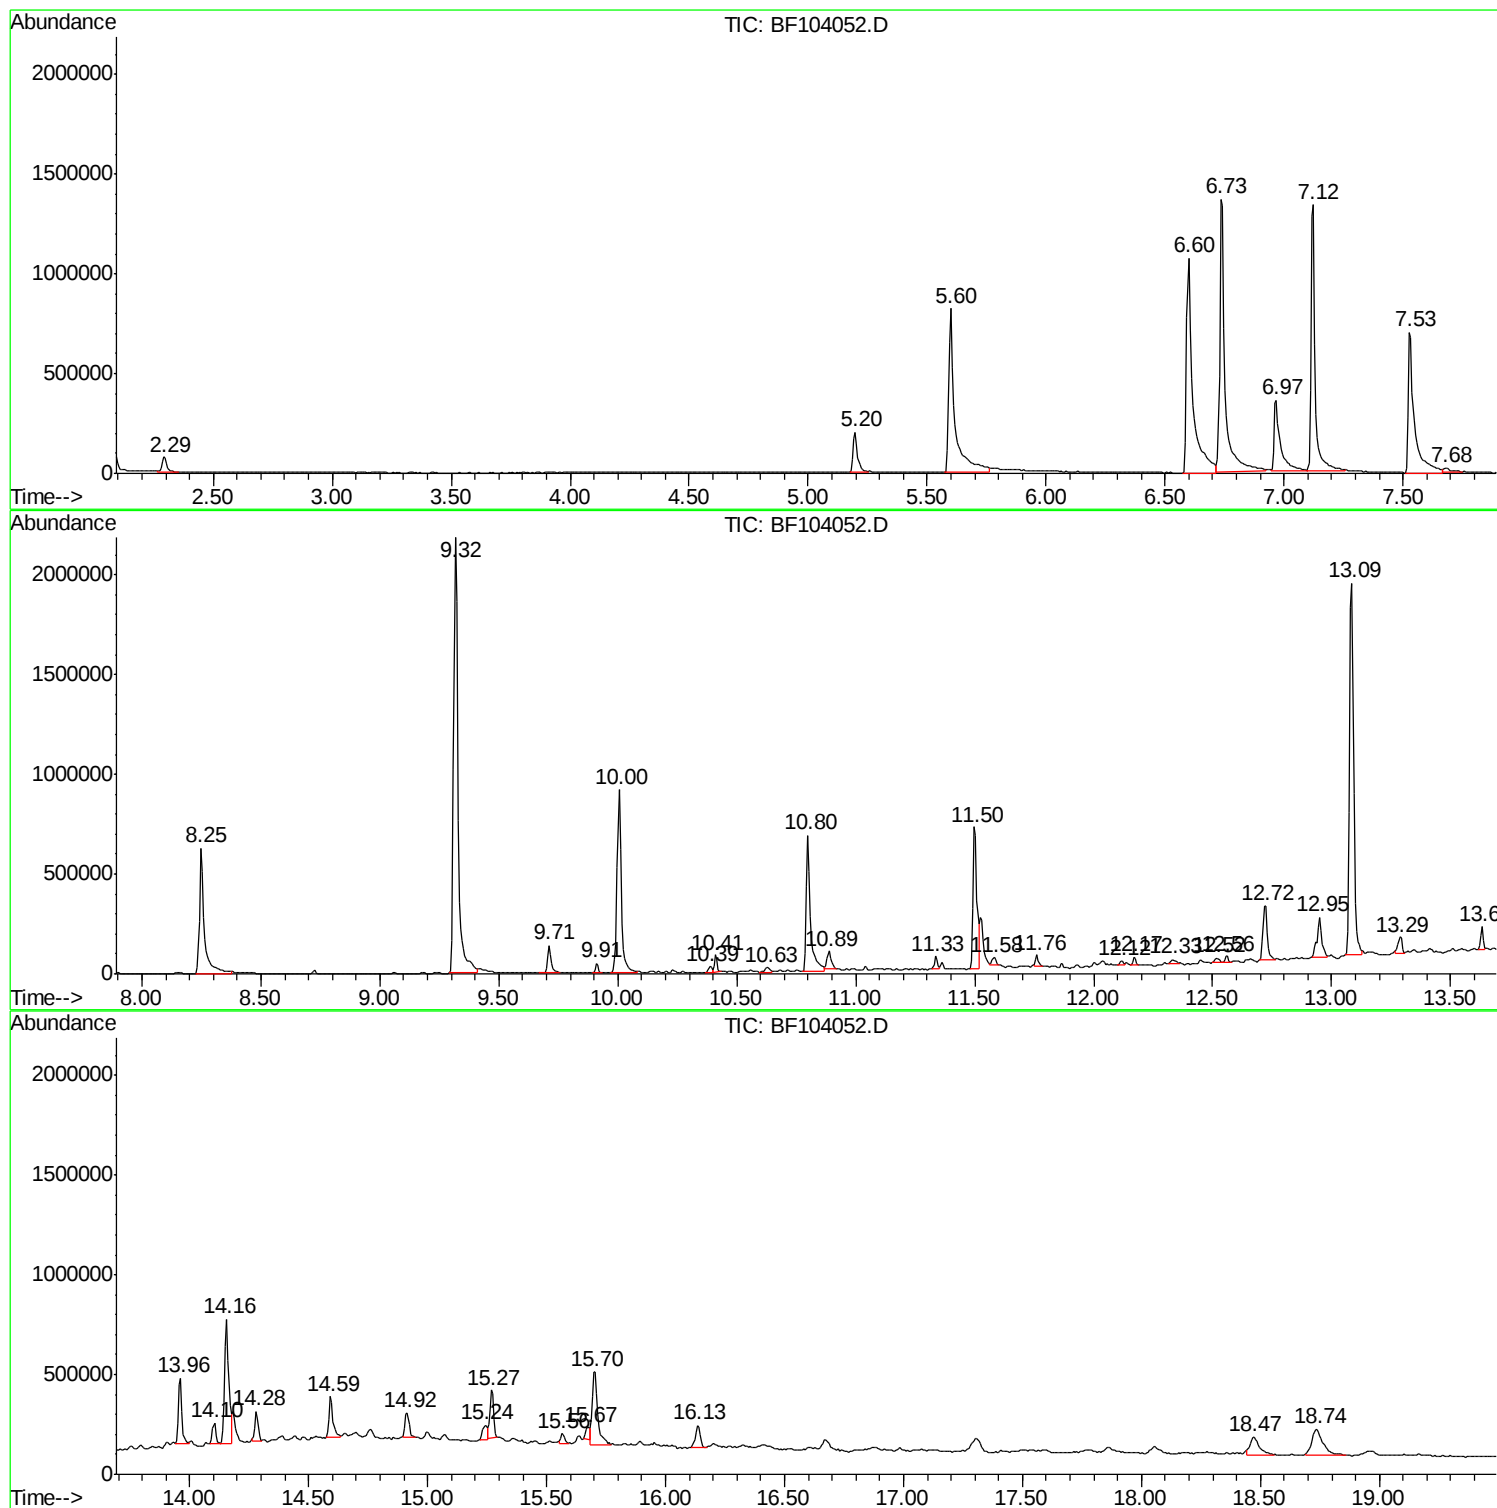

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF032918\
Data_File : BF104052.D
Acq_On : 29-Mar-2018 15:499
Operator : JU/SJJ
Sample : J2120-022
Misc :
ALS_Vial : 10 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
BES-2

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032818.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
