


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032918\
 Data File : BF104043.D
 Acq On : 29 Mar 2018 10:52
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 28 13:41:47 2018

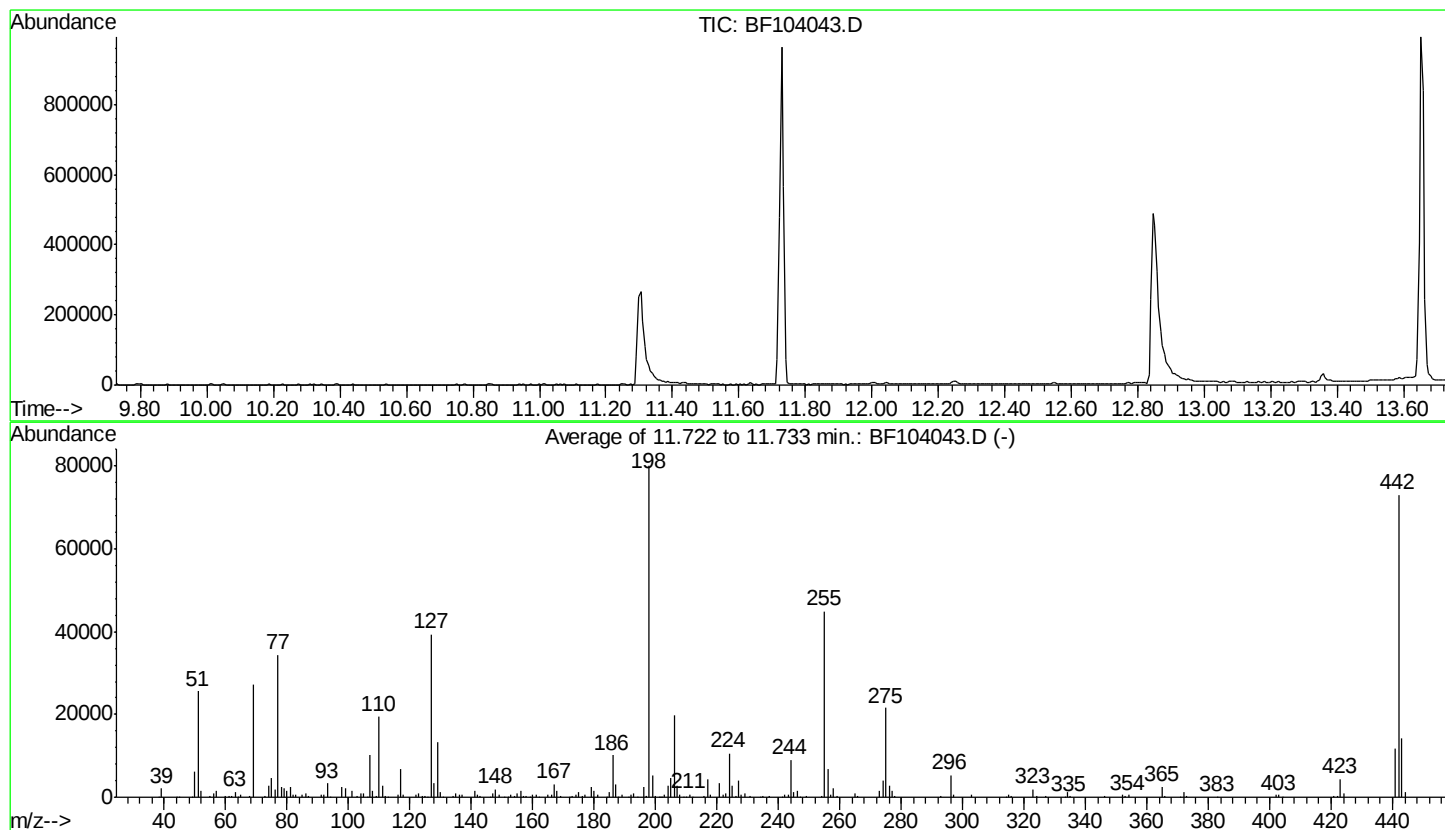

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	25569	PASS
68	69	0.00	2	1.7	458	PASS
69	198	0.00	100	34.2	27366	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.2	39386	PASS
197	198	0.00	2	0.2	193	PASS
198	198	100	100	100.0	80128	PASS
199	198	5	9	6.4	5154	PASS
275	198	10	60	26.9	21525	PASS
365	198	1	100	3.3	2637	PASS
441	443	0.01	100	81.8	11753	PASS
442	198	50	100	91.3	73122	PASS
443	442	15	24	19.6	14360	PASS