

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032922\
 Data File : BF127558.D
 Acq On : 29 Mar 2022 11:37
 Operator : CG\JU
 Sample : PB143673BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143673BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127558.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	537	541	560	rBV	3265060	3457643	83.58%	13.729%
2	6.475	708	712	715	rBV	2958723	3432277	82.97%	13.629%
3	6.834	769	773	787	rBV	737418	690171	16.68%	2.740%
4	7.404	865	870	873	rBV	2349405	2394879	57.89%	9.509%
5	8.116	987	991	1002	rBV	960172	910602	22.01%	3.616%
6	9.192	1168	1174	1177	rBV	4038289	4073498	98.47%	16.175%
7	9.869	1285	1289	1299	rBV	1225271	1073848	25.96%	4.264%
8	10.669	1420	1425	1428	rBV	2584765	2407530	58.20%	9.560%
9	11.363	1539	1543	1552	rBV	1287917	1112428	26.89%	4.417%
10	12.751	1776	1779	1782	rBV	57738	41946	1.01%	0.167%
11	12.951	1808	1813	1816	rBV	4175004	4136955	100.00%	16.427%
12	14.010	1990	1993	2001	rBV	868470	844231	20.41%	3.352%
13	15.492	2242	2245	2257	rVB	463448	608228	14.70%	2.415%




Sum of corrected areas: 25184236

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032922\
Data File : BF127558.D
Acq On : 29 Mar 2022 11:37
Operator : CG\JU
Sample : PB143673BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143673BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

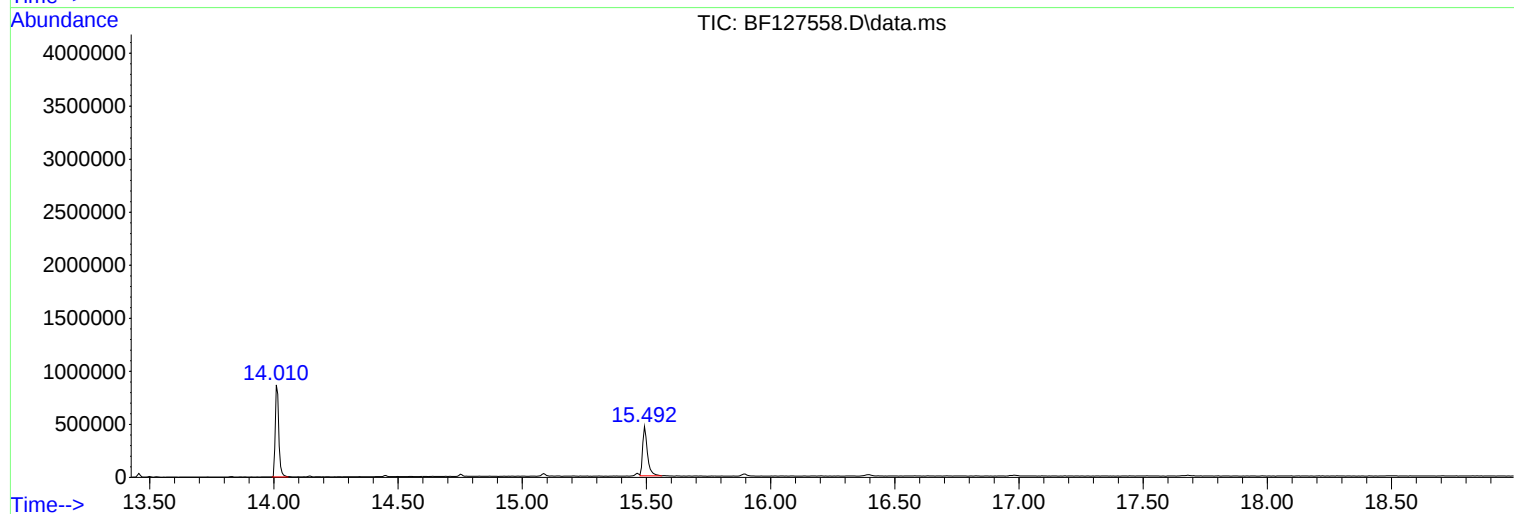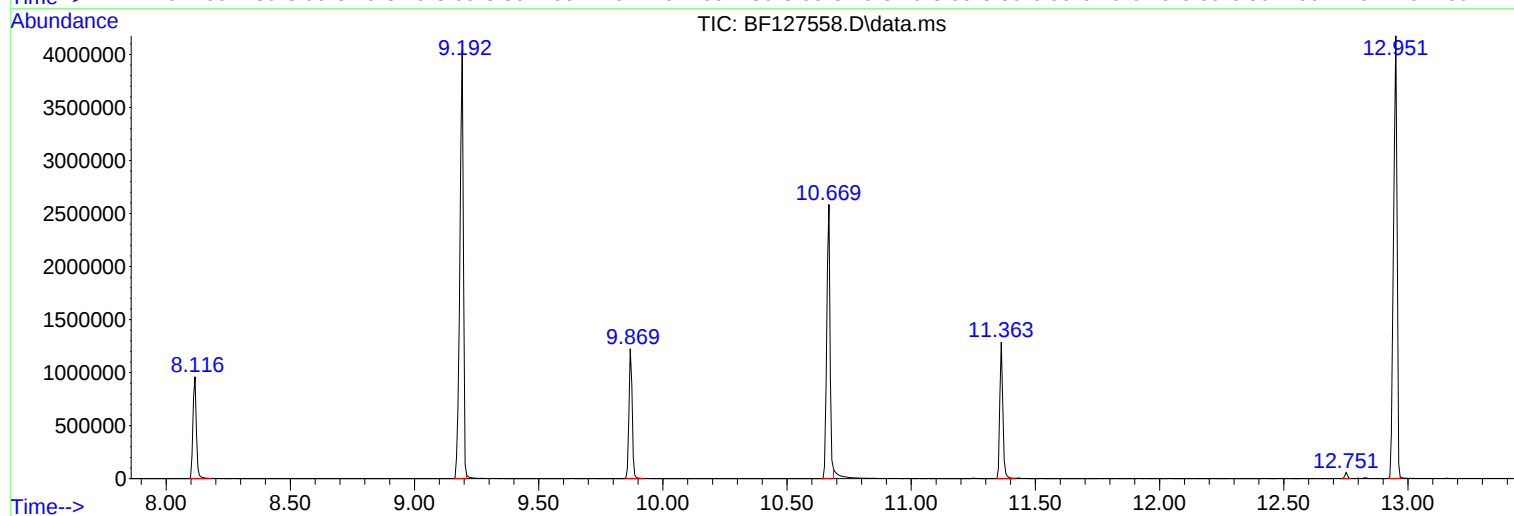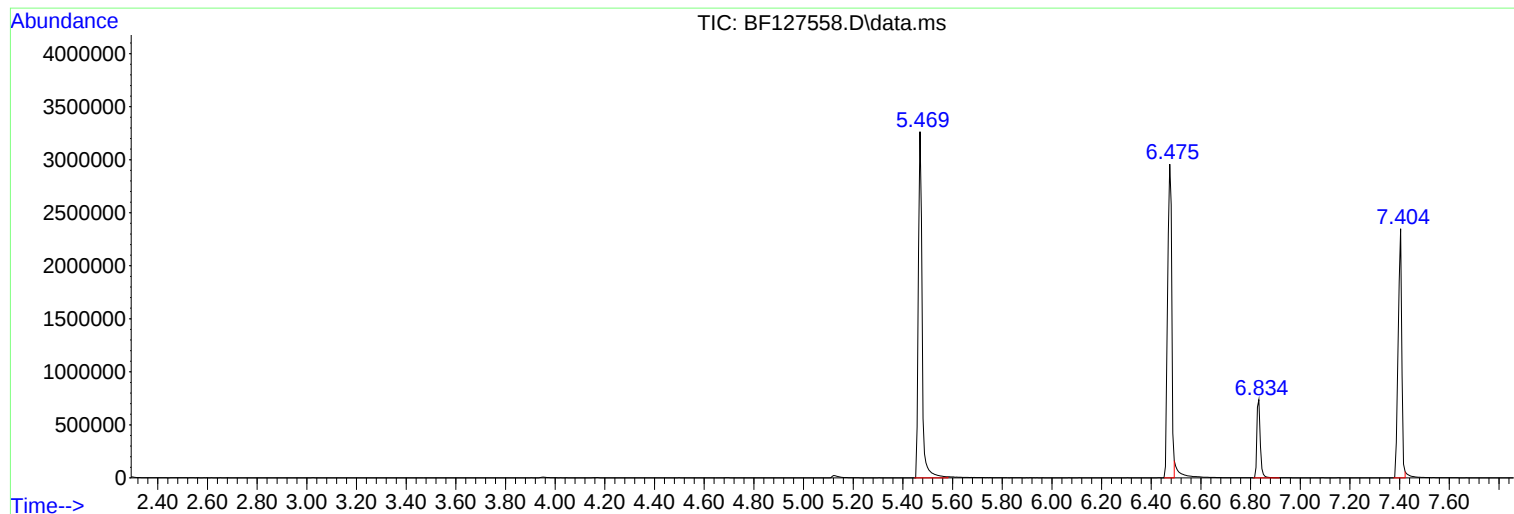

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032922\
Data File : BF127558.D
Acq On : 29 Mar 2022 11:37
Operator : CG\JU
Sample : PB143673BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143673BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032922\
Data File : BF127558.D
Acq On : 29 Mar 2022 11:37
Operator : CG\JU
Sample : PB143673BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143673BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------