

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032922\
 Data File : BF127574.D
 Acq On : 29 Mar 2022 19:21
 Operator : CG\JU
 Sample : N2157-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127574.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.069	470	473	488	rBV	44941	69833	3.43%	0.532%
2	5.457	536	539	558	rBV	1704484	1885719	92.74%	14.363%
3	6.475	709	712	733	rBV	2011132	1926450	94.74%	14.673%
4	6.834	769	773	781	rBV	521863	484650	23.83%	3.691%
5	7.398	866	869	880	rBV	1384104	1270426	62.48%	9.676%
6	8.116	987	991	1006	rBV	680796	611468	30.07%	4.657%
7	9.186	1169	1173	1182	rBV	2272138	2033366	100.00%	15.487%
8	9.257	1182	1185	1190	rVB	32610	30564	1.50%	0.233%
9	9.869	1286	1289	1298	rBV	800186	657537	32.34%	5.008%
10	10.663	1421	1424	1438	rBV	1112779	1014754	49.91%	7.729%
11	11.363	1539	1543	1551	rBV	656144	578905	28.47%	4.409%
12	12.945	1808	1812	1815	rBV	1702744	1470019	72.29%	11.197%
13	13.851	1959	1966	1974	rBV9	32140	110878	5.45%	0.845%
14	14.010	1990	1993	2003	rBV	522137	498408	24.51%	3.796%
15	15.492	2241	2245	2252	rVB	402530	486121	23.91%	3.703%




Sum of corrected areas: 13129098

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032922\
Data File : BF127574.D
Acq On : 29 Mar 2022 19:21
Operator : CG\JU
Sample : N2157-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

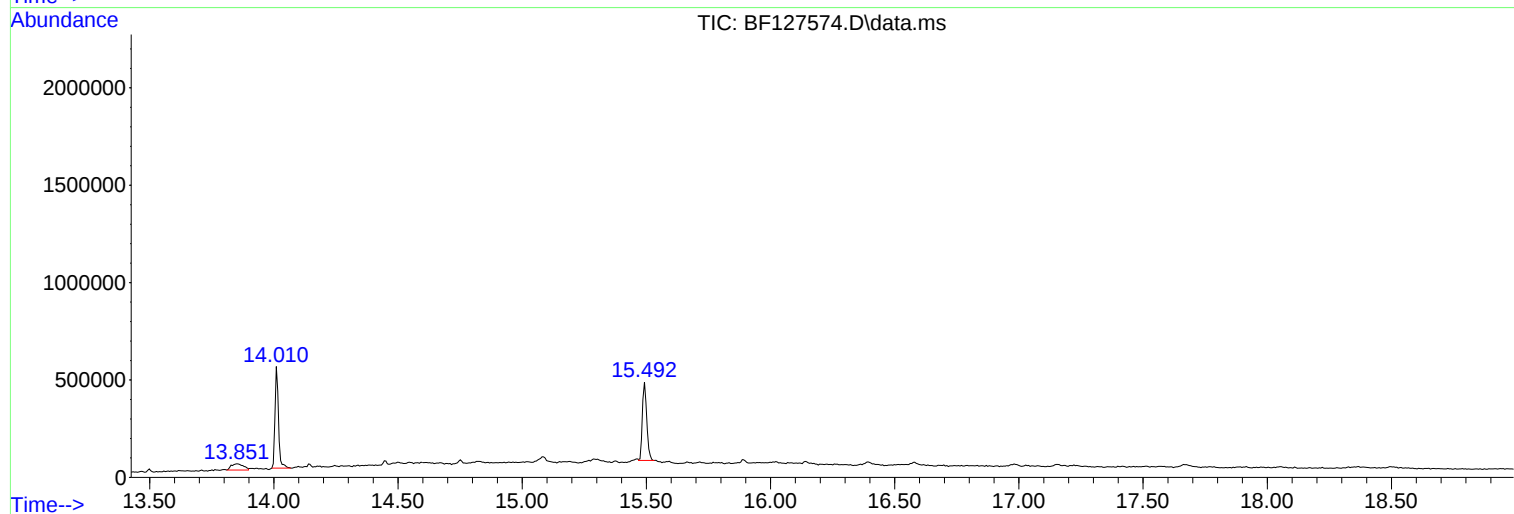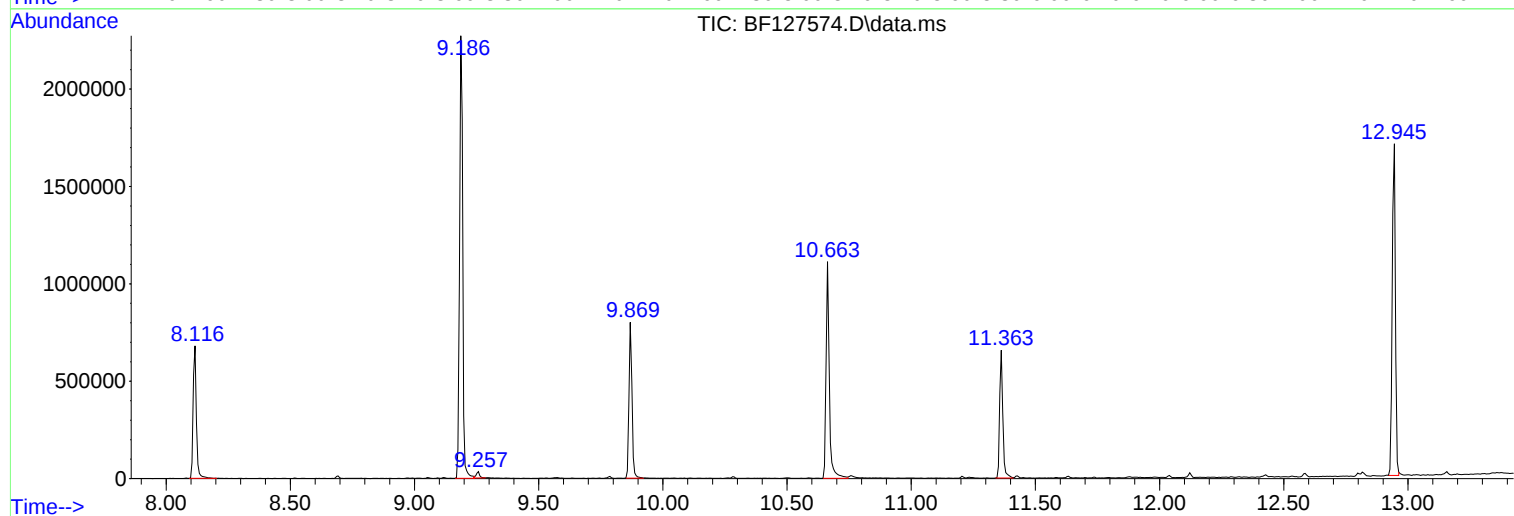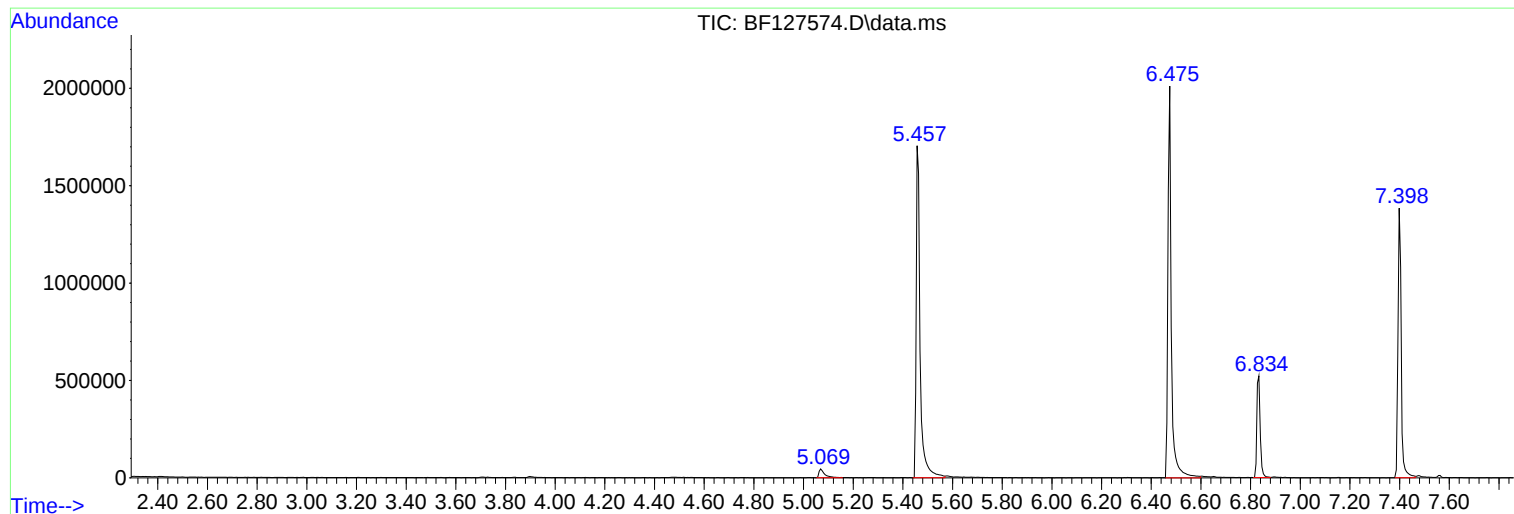

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032922\
Data File : BF127574.D
Acq On : 29 Mar 2022 19:21
Operator : CG\JU
Sample : N2157-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.069	2.88 ng	69833	1,4-Dichlorobenzene-d4	6.834

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	3-Octanol	130	C8H18O	000589-98-0	36		
3	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33		
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	27		
5	Propane, 2-ethoxy-2-methyl-	102	C6H14O	000637-92-3	23		

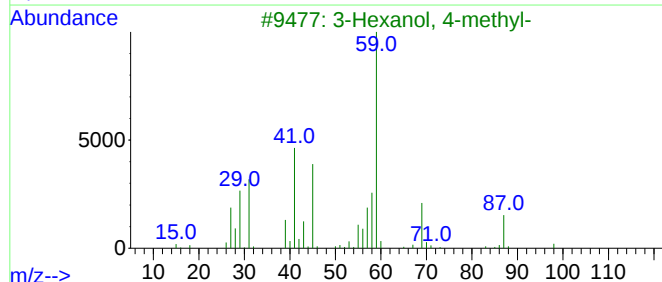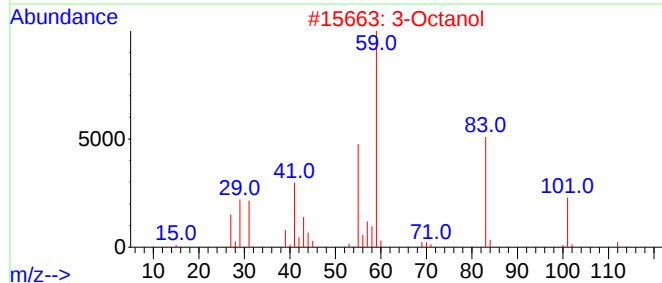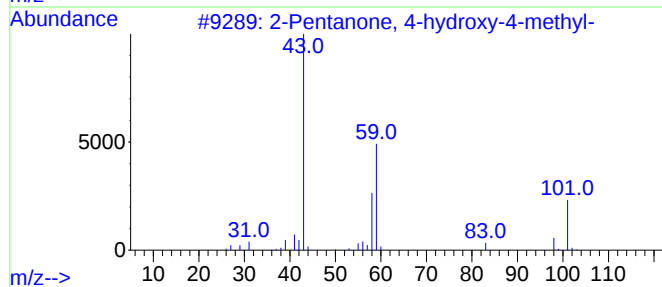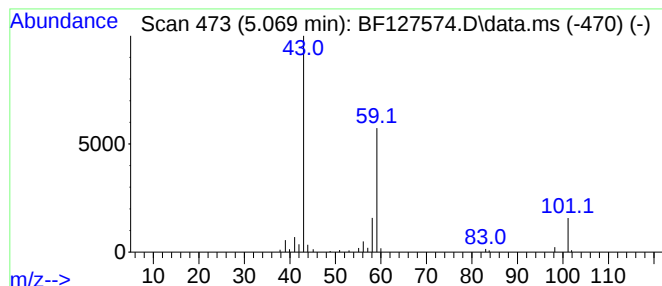

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032922\
Data File : BF127574.D
Acq On : 29 Mar 2022 19:21
Operator : CG\JU
Sample : N2157-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Trichloroacetic acid, hexad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.851	4.45 ng	110878	Chrysene-d12	14.010

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	87
2			Behenic alcohol	326	C22H46O	000661-19-8	87
3			Heptadecyl trifluoroacetate	352	C19H35F3O2	1010351-87-0	86
4			Bromoacetic acid, octadecyl ester	390	C20H39BrO2	018992-03-5	83
5			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	80

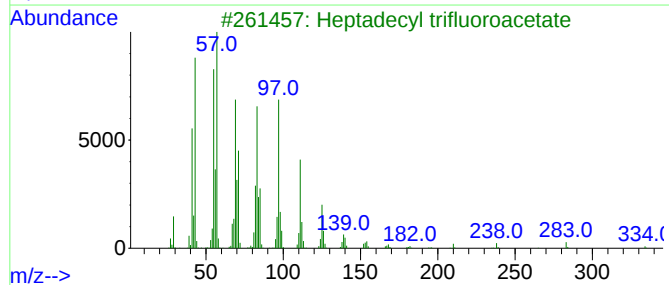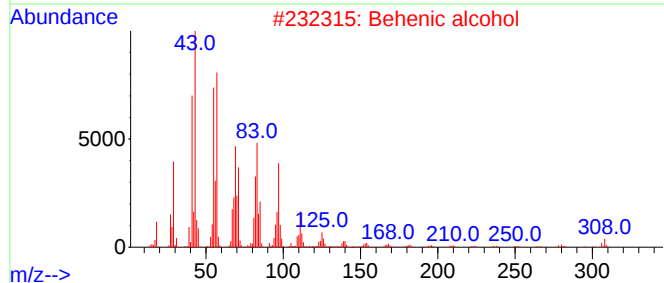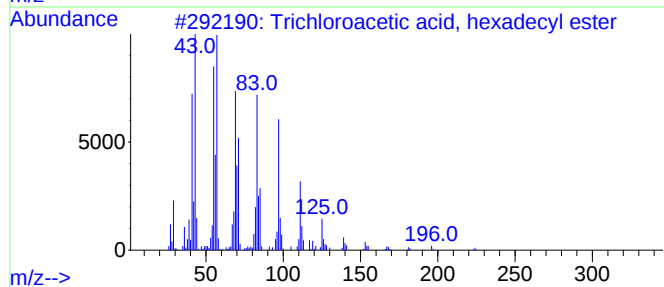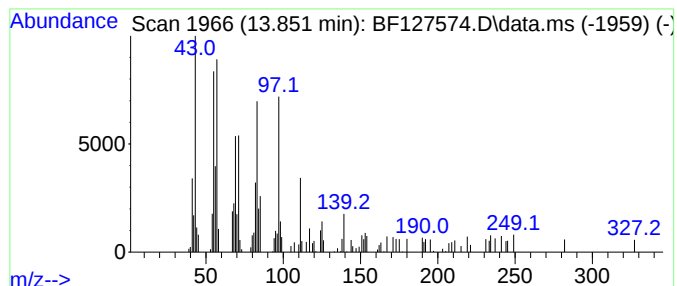

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032922\
Data File : BF127574.D
Acq On : 29 Mar 2022 19:21
Operator : CG\JU
Sample : N2157-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.069	2.9	ng	69833	1	6.834	484650	20.0
Trichloroacetic...	13.851	4.5	ng	110878	5	14.010	498408	20.0