


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033015\
 Data File : BF078100.D
 Acq On : 31 Mar 2015 1:14
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 28 05:37:34 2015

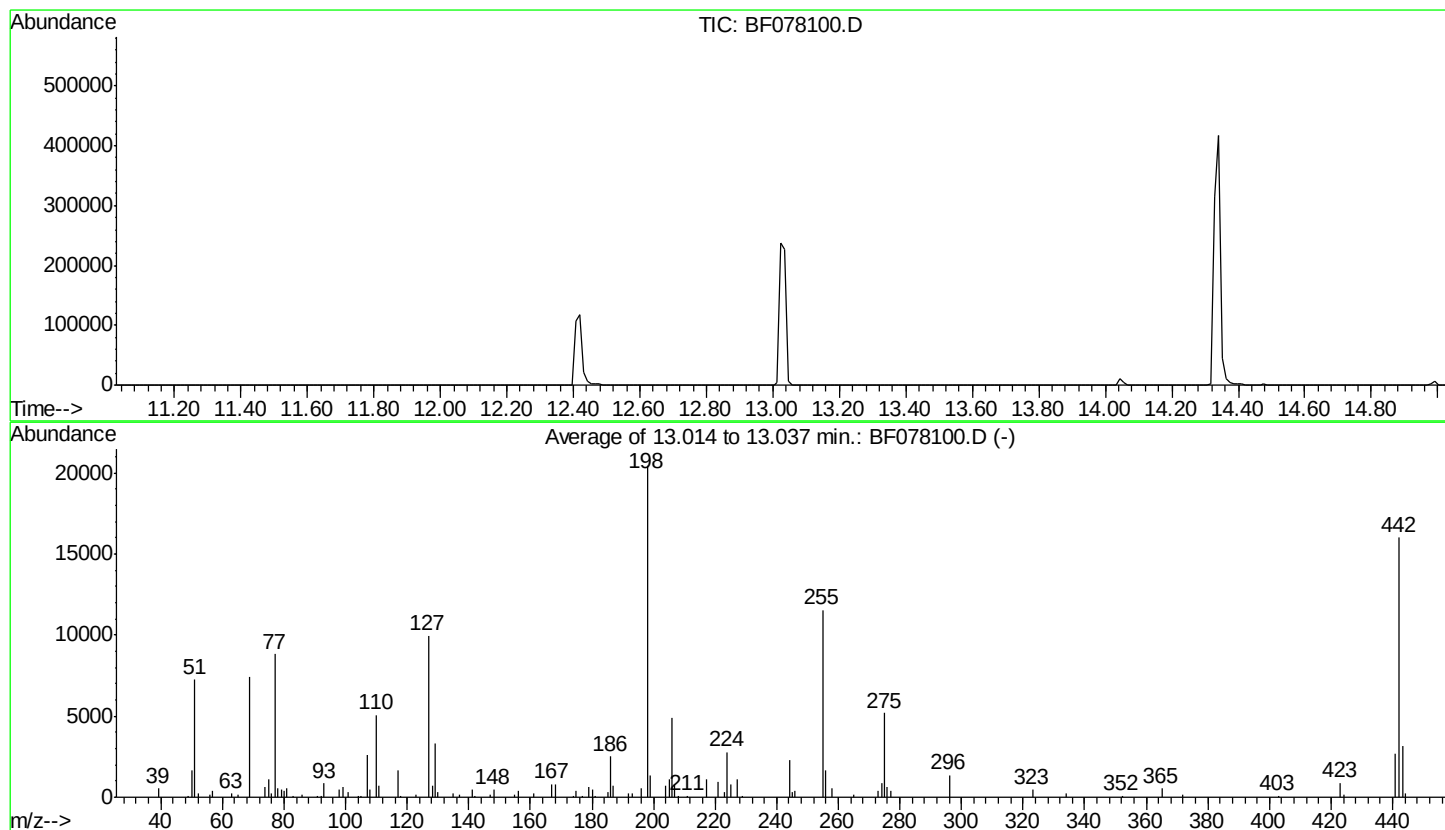

AutoFind: Scans 1061, 1062, 1063; Background Corrected with Scan 1058

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	7259	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.4	7451	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	9978	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20460	PASS
199	198	5	9	6.5	1335	PASS
275	198	10	60	25.4	5197	PASS
365	198	1	100	2.6	532	PASS
441	442	0.01	24	16.7	2676	PASS
442	198	50	100	78.3	16020	PASS
443	442	15	24	19.6	3139	PASS