


Data Path : Z:\HPCHEM1\BNA_F\Data\BF033015\
Data File : BF078080.D
Acq On : 30 Mar 2015 11:51
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 28 05:37:34 2015

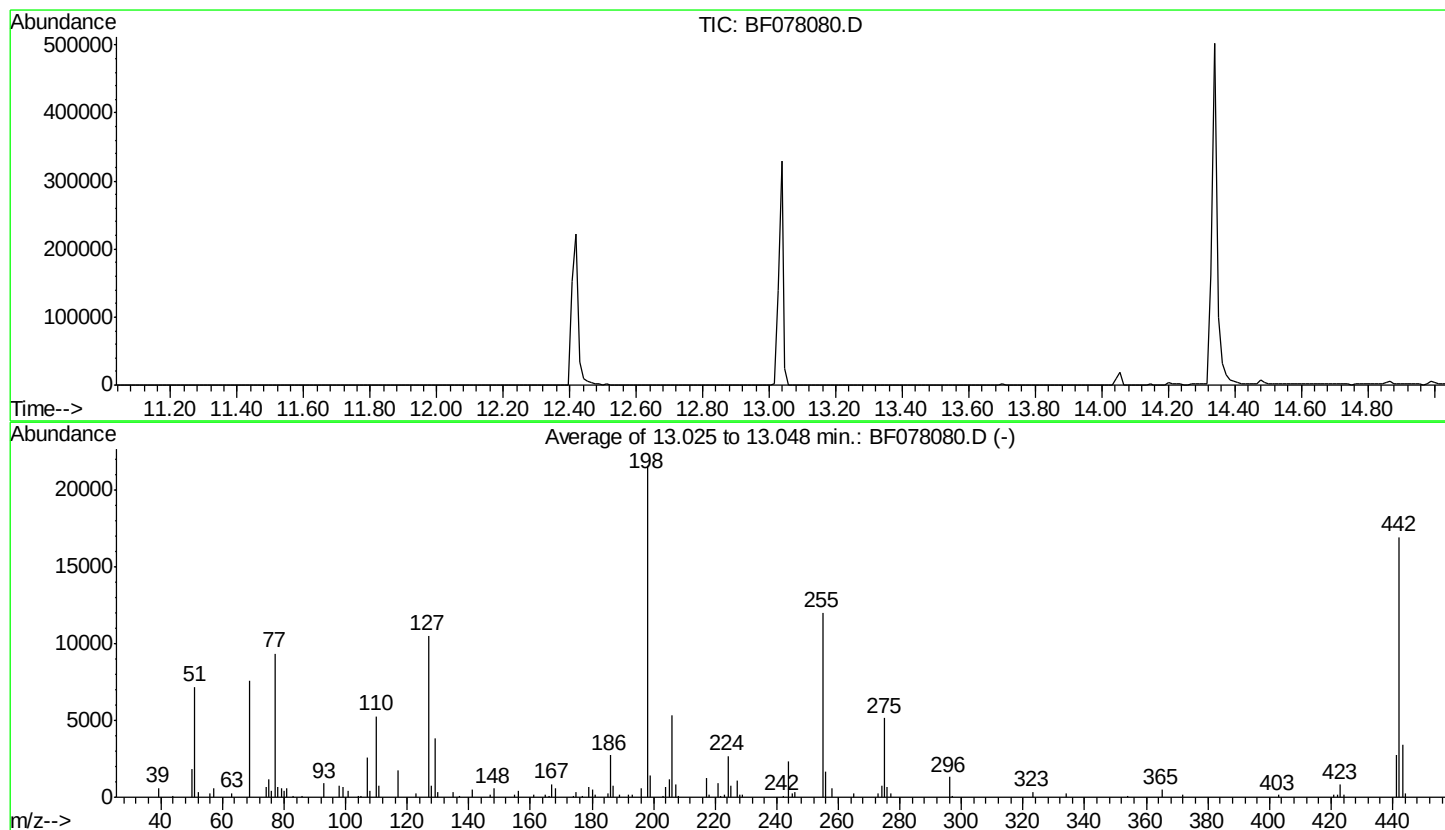

AutoFind: Scans 1062, 1063, 1064; Background Corrected with Scan 1059

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	7193	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.9	7549	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	10545	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21600	PASS
199	198	5	9	6.4	1379	PASS
275	198	10	60	23.9	5169	PASS
365	198	1	100	2.2	477	PASS
441	442	0.01	24	16.2	2741	PASS
442	198	50	100	78.4	16933	PASS
443	442	15	24	20.2	3419	PASS