

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
 Data File : BF085900.D
 Acq On : 30 Mar 2016 21:46
 Operator : UM/SJ
 Sample : H2023-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B-6

Quant Time: Mar 30 23:48:19 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 30 12:31:18 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.80	152	108172	20.00	ng	0.00
21) Naphthalene-d8	8.08	136	450793	20.00	ng	-0.01
38) Acenaphthene-d10	9.84	164	192765	20.00	ng	0.00
63) Phenanthrene-d10	11.32	188	322778	20.00	ng	-0.01
75) Chrysene-d12	13.96	240	225411	20.00	ng	-0.01
86) Perylene-d12	15.37	264	226067	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	828114	127.50	ng	0.00
7) Phenol-d6	6.44	99	1135108	137.45	ng	-0.01
23) Nitrobenzene-d5	7.36	82	685799	85.67	ng	-0.01
41) 2,4,6-Tribromophenol	10.63	330	245289	133.93	ng	0.00
44) 2-Fluorobiphenyl	9.17	172	1187097	102.89	ng	0.00
78) Terphenyl-d14	12.91	244	774936	70.70	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.36	70	88137	17.82	ng	# 79
25) Isophorone	7.36	82	637083	41.31	ng	# 68
37) 2-Methylnaphthalene	8.80	142	226	Below Cal		# 15
49) Dimethylphthalate	9.56	163	223041	15.25	ng	99
56) 2,4-Dinitrotoluene	9.84	165	24785	6.19	ng	# 37
66) 4-Bromophenyl-phenylether	10.63	248	16432	4.98	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
Data File : BF085900.D
Acq On : 30 Mar 2016 21:46
Operator : UM/SJ
Sample : H2023-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
B-6

Quant Time: Mar 30 23:48:19 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 30 12:31:18 2016
Response via : Initial Calibration

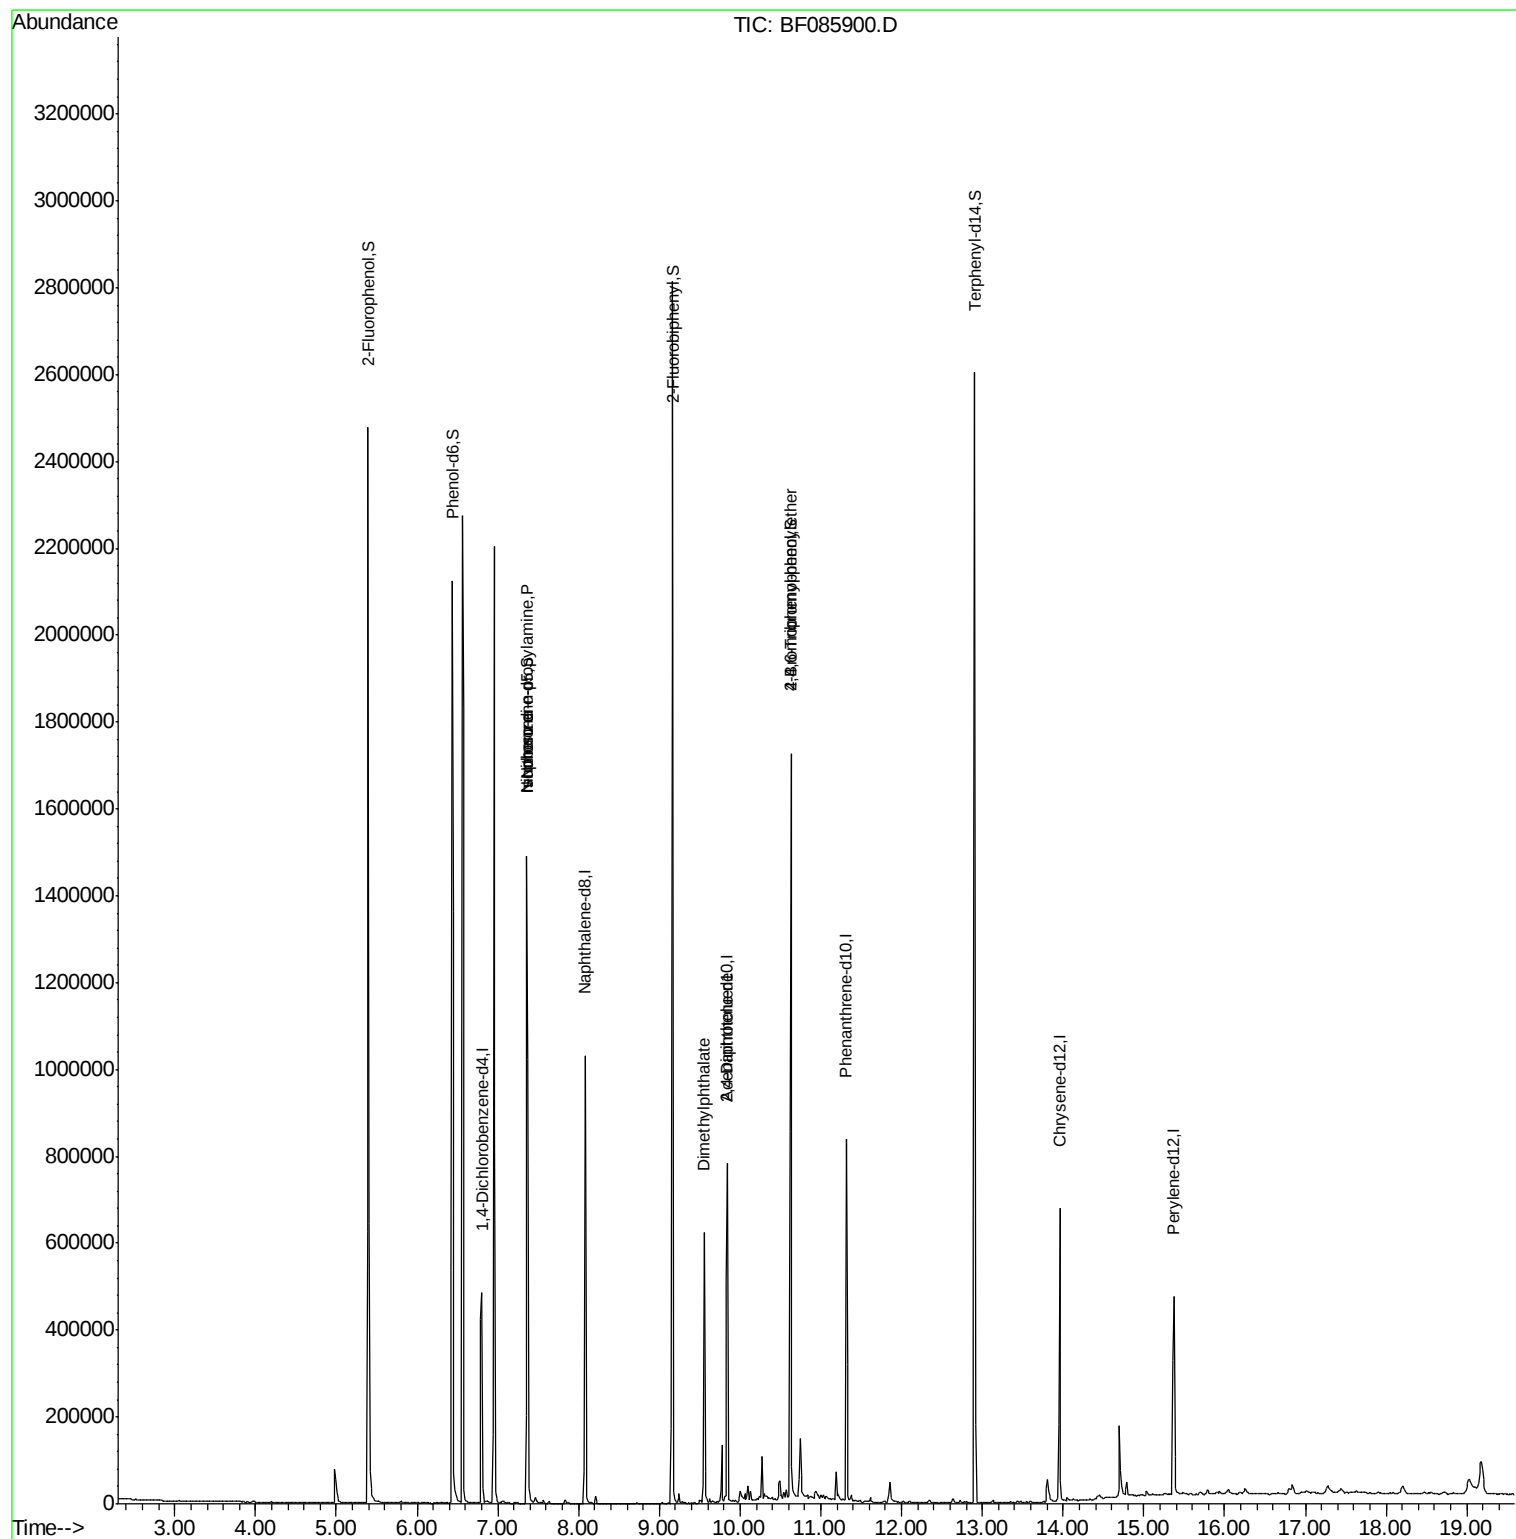

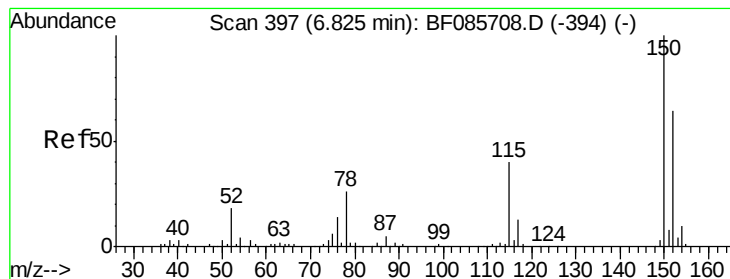


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.80 min Scan# 395
 Delta R.T. -0.00 min
 Lab File: BF085900.D
 Acq: 30 Mar 2016 21:46

Instrument :
 BNA_F
 ClientSampleId :
 B-6

Tgt Ion:152 Resp: 108172
 Ion Ratio Lower Upper
 152 100
 150 154.0 124.2 186.2
 115 53.9 47.0 70.6

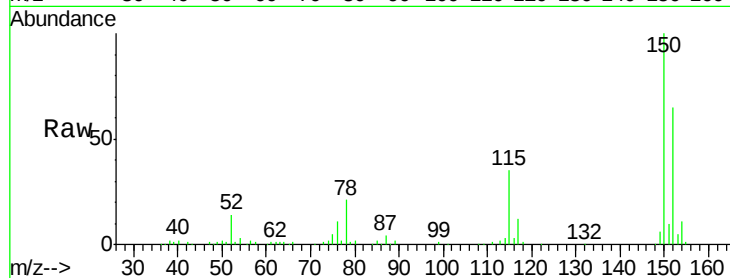


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

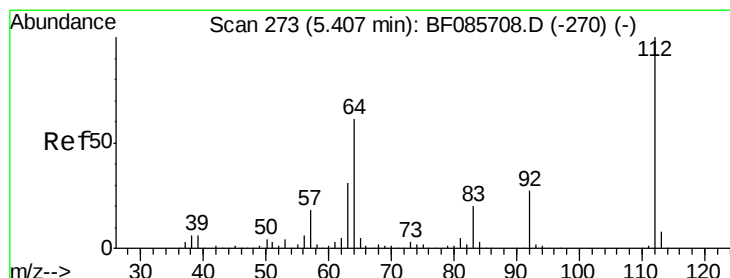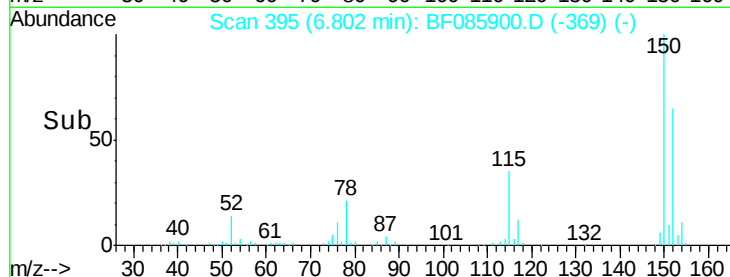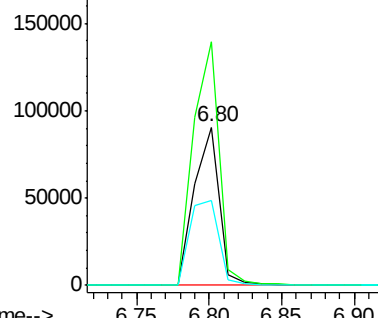



#5


2-Fluorophenol
 Concen: 127.50 ng
 RT: 5.40 min Scan# 272
 Delta R.T. -0.00 min
 Lab File: BF085900.D
 Acq: 30 Mar 2016 21:46

Tgt Ion:112 Resp: 828114
 Ion Ratio Lower Upper
 112 100
 64 56.0 39.9 59.9
 63 28.7 20.2 30.2

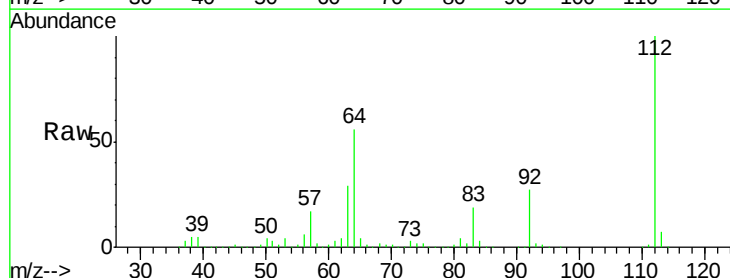

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

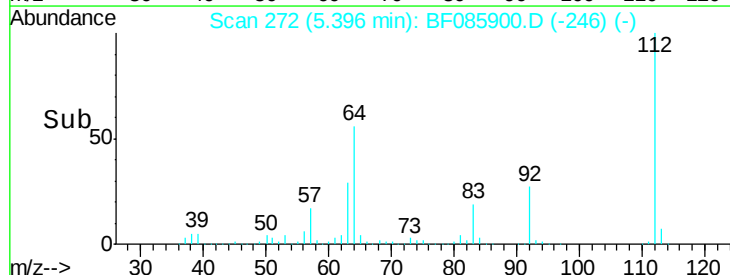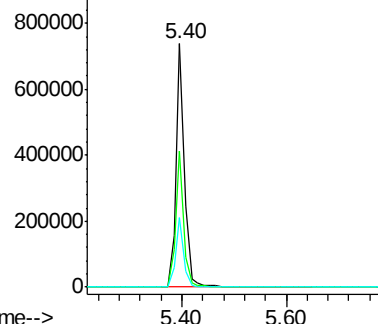

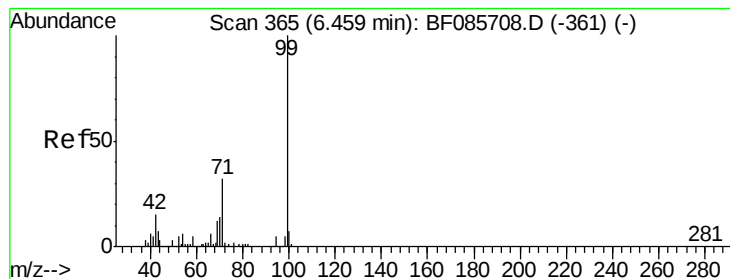

#7

Phenol-d6

Concen: 137.45 ng

RT: 6.44 min Scan# 363

Delta R.T. -0.01 min

Lab File: BF085900.D

Acq: 30 Mar 2016 21:46

Instrument :

BNA_F

ClientSampleId :

B-6


Tgt Ion: 99 Resp: 1135108

Ion Ratio Lower Upper

99 100

42 15.8 11.1 16.7




71 33.5 24.9 37.3

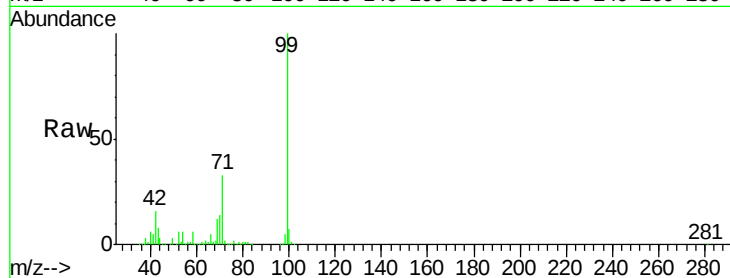

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

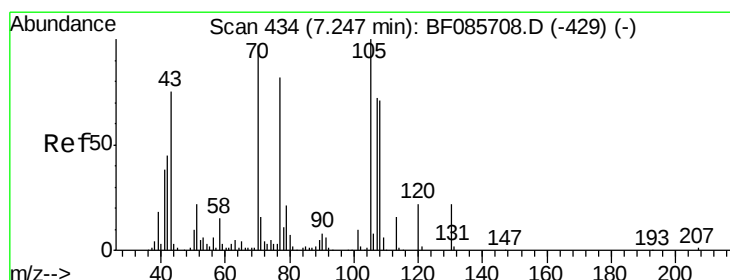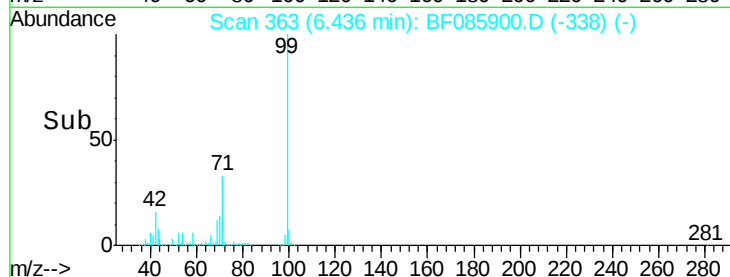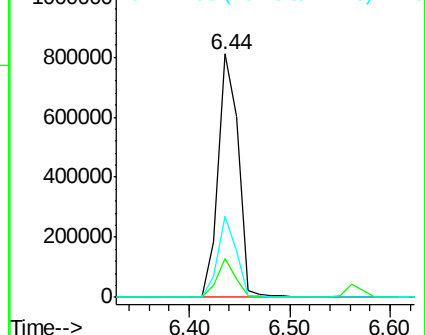

#19

n-Nitroso-di-n-propylamine

Concen: 17.82 ng

RT: 7.36 min Scan# 444

Delta R.T. 0.14 min

Lab File: BF085900.D

Acq: 30 Mar 2016 21:46

Tgt Ion: 70 Resp: 88137


Ion Ratio Lower Upper

70 100

42 42.6 37.1 55.7

101 0.0 8.6 12.8#

130 2.1 19.6 29.4#


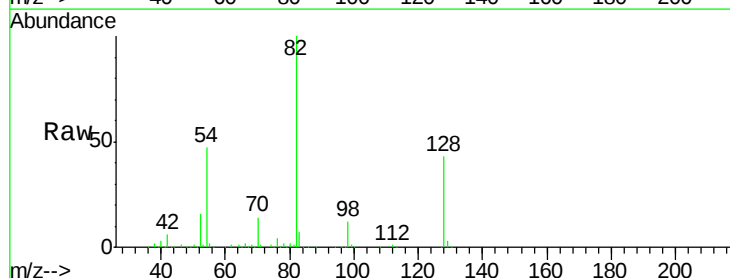



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

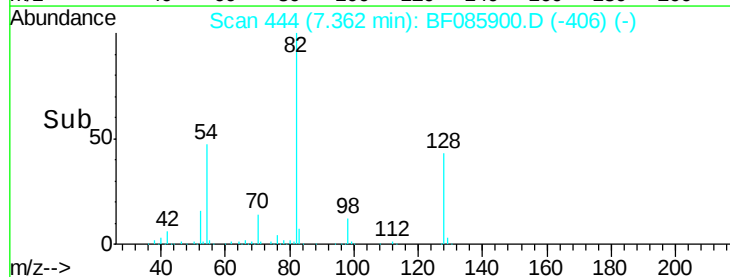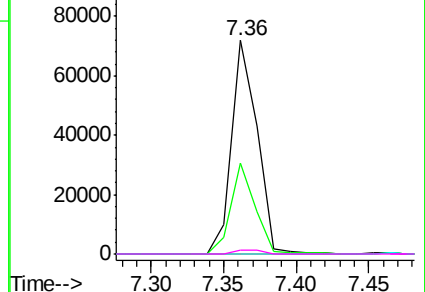


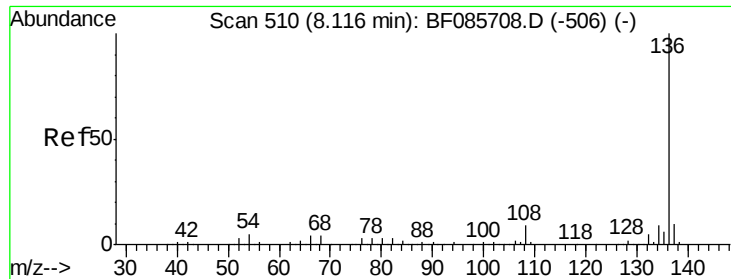




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.08 min Scan# 507
Delta R.T. -0.01 min
Lab File: BF085900.D
Acq: 30 Mar 2016 21:46

Instrument :
BNA_F
ClientSampleId :
B-6

Tgt Ion:	136	Resp:	450793
Ion	Ratio	Lower	Upper
136	100		
137	10.7	9.1	13.7
54	7.5	7.4	11.0
68	6.0	5.8	8.8




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

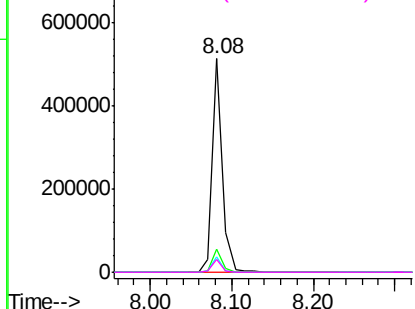
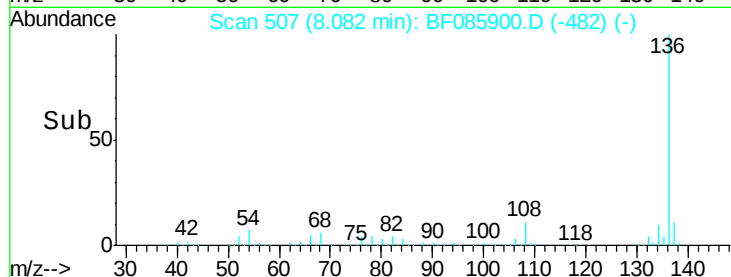



#23
Nitrobenzene-d5
Concen: 85.67 ng
RT: 7.36 min Scan# 444
Delta R.T. -0.01 min
Lab File: BF085900.D
Acq: 30 Mar 2016 21:46

Tgt Ion:	82	Resp:	685799
Ion	Ratio	Lower	Upper
82	100		
128	42.6	41.8	62.8
54	47.4	33.4	50.0



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

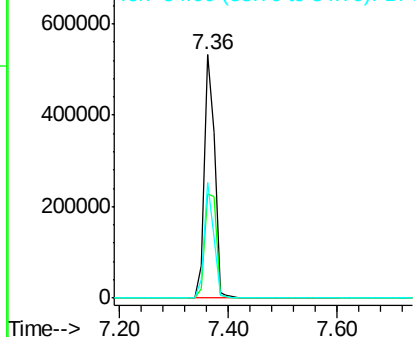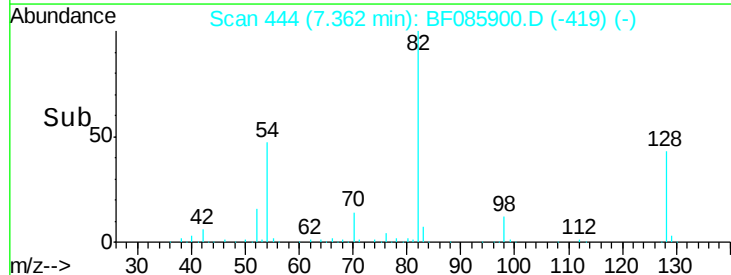

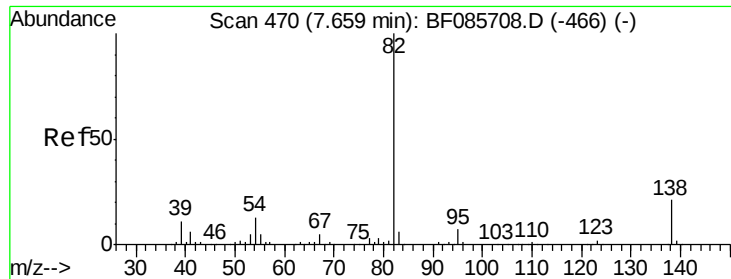

#25

Isophorone

Concen: 41.31 ng

RT: 7.36 min Scan# 444

Delta R.T. -0.27 min

Lab File: BF085900.D

Acq: 30 Mar 2016 21:46

Instrument :

BNA_F

ClientSampleId :

B-6


Tgt Ion: 82 Resp: 637083

Ion Ratio Lower Upper

82 100

95 0.0 5.4 8.2#




138 0.0 12.9 19.3#

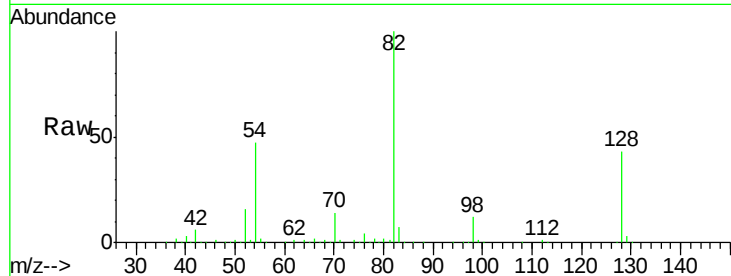

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 95.00 (94.70 to 95.70): BF0

Ion 138.00 (137.70 to 138.70): E

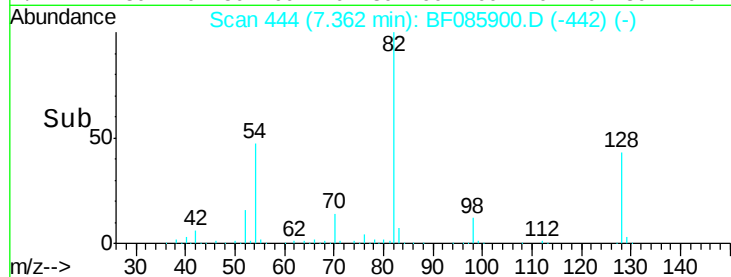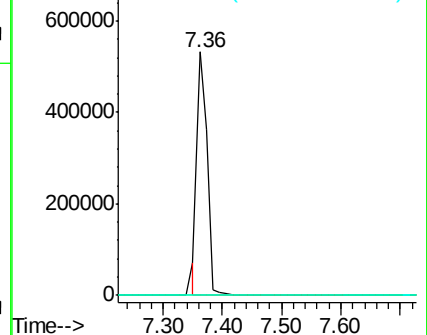

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.84 min Scan# 661

Delta R.T. -0.00 min

Lab File: BF085900.D

Acq: 30 Mar 2016 21:46


Tgt Ion: 164 Resp: 192765

Ion Ratio Lower Upper

164 100

162 104.2 82.1 123.1



160 48.9 37.4 56.2




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

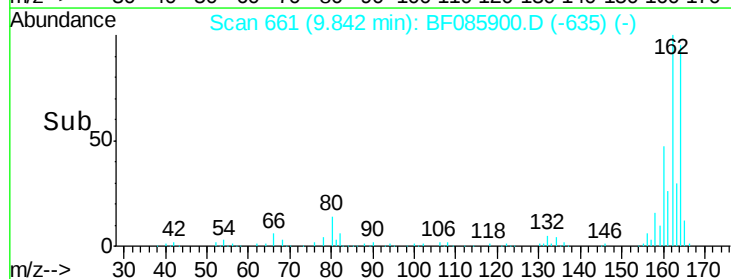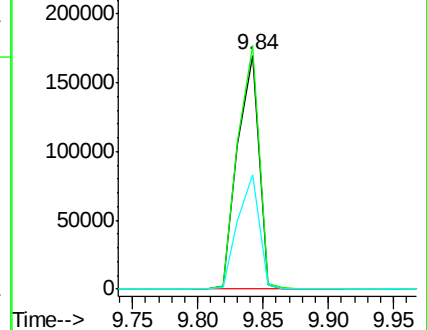


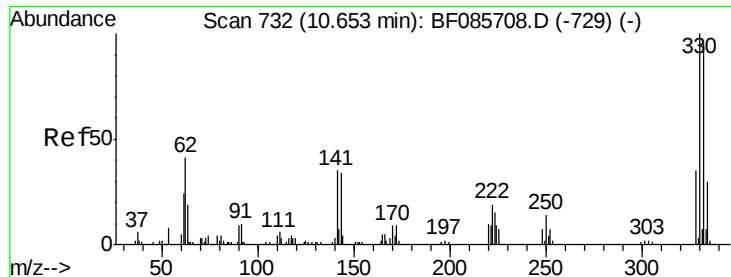




#41
 2,4,6-Tribromophenol
 Concen: 133.93 ng
 RT: 10.63 min Scan# 730
 Delta R.T. -0.00 min
 Lab File: BF085900.D
 Acq: 30 Mar 2016 21:46

Instrument :
 BNA_F
 ClientSampleId :
 B-6

Tgt Ion:330 Resp: 245289
 Ion Ratio Lower Upper
 330 100
 332 95.6 78.2 117.2
 141 36.0 31.5 47.3

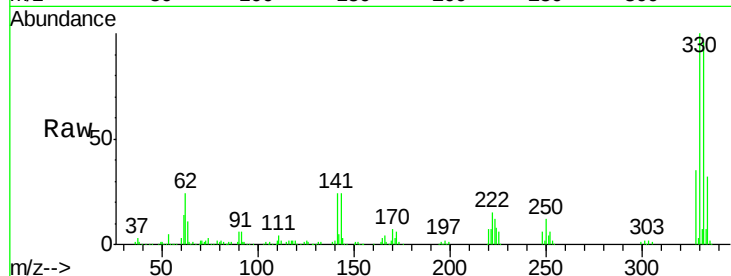


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

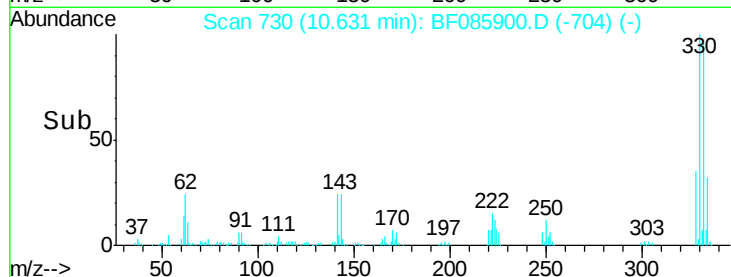
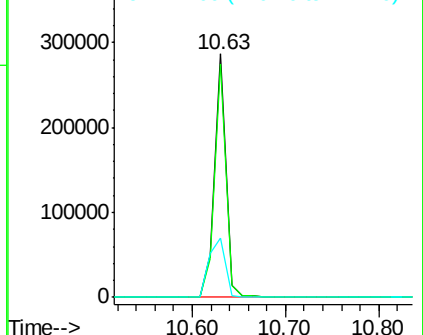



#44
 2-Fluorobiphenyl
 Concen: 102.89 ng
 RT: 9.17 min Scan# 602
 Delta R.T. -0.00 min
 Lab File: BF085900.D
 Acq: 30 Mar 2016 21:46

Tgt Ion:172 Resp: 1187097
 Ion Ratio Lower Upper
 172 100
 171 36.4 29.4 44.2
 170 24.6 19.8 29.6



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

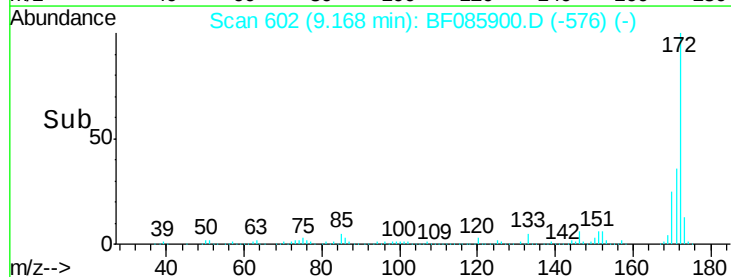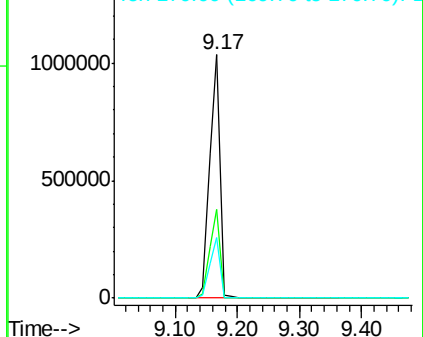

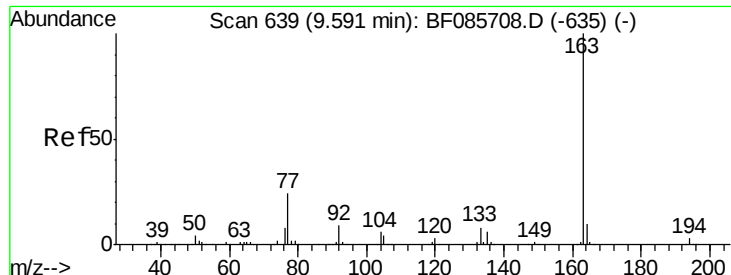

#49

Dimethylphthalate

Concen: 15.25 ng

RT: 9.56 min Scan# 636

Delta R.T. -0.01 min

Lab File: BF085900.D

Acq: 30 Mar 2016 21:46

Instrument :

BNA_F

ClientSampleId :

B-6


Tgt Ion:163 Resp: 223041

Ion Ratio Lower Upper

163 100

194 3.3 2.9 4.3




164 10.3 8.3 12.5

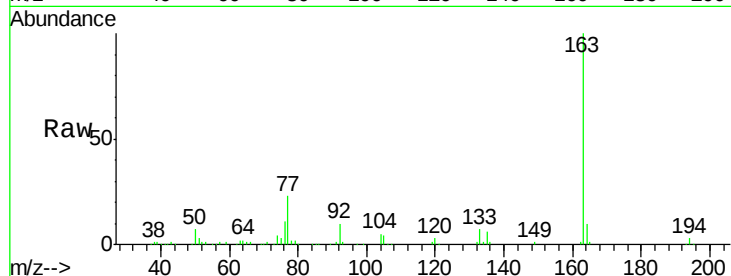

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

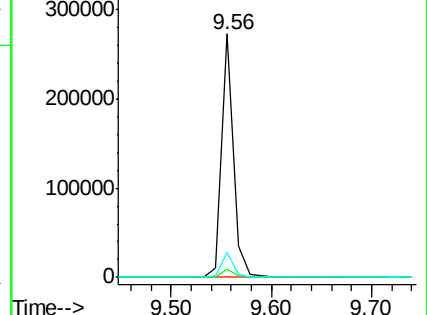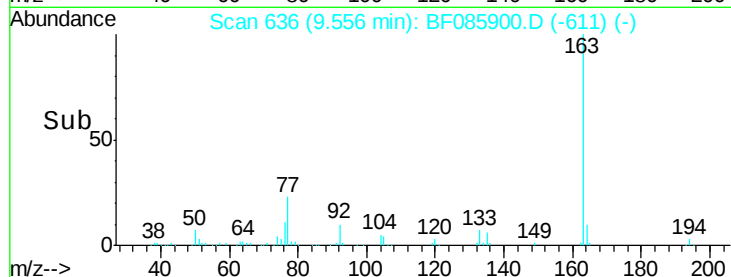

#56

2,4-Dinitrotoluene

Concen: 6.19 ng

RT: 9.84 min Scan# 661

Delta R.T. -0.19 min

Lab File: BF085900.D

Acq: 30 Mar 2016 21:46

Tgt Ion:165 Resp: 24785


Ion Ratio Lower Upper

165 100

63 1.5 24.9 37.3#

89 2.0 41.0 61.6#

182 0.0 2.1 3.1#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

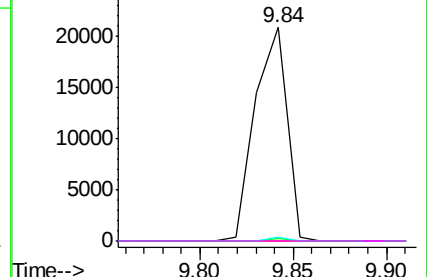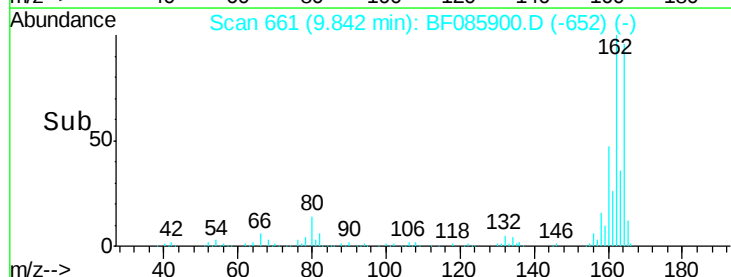


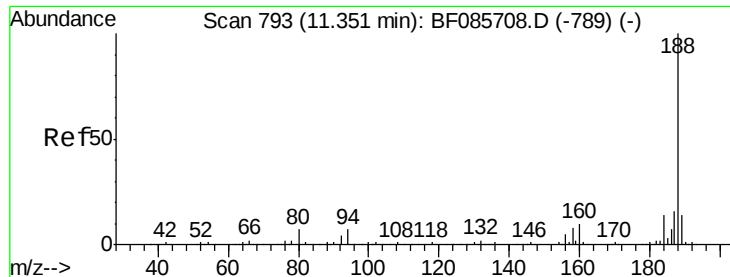




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.32 min Scan# 790
Delta R.T. -0.01 min
Lab File: BF085900.D
Acq: 30 Mar 2016 21:46

Instrument :
BNA_F
ClientSampleId :
B-6

Tgt Ion:188 Resp: 322778
Ion Ratio Lower Upper
188 100
94 12.2 5.4 8.0#
80 13.4 5.5 8.3#

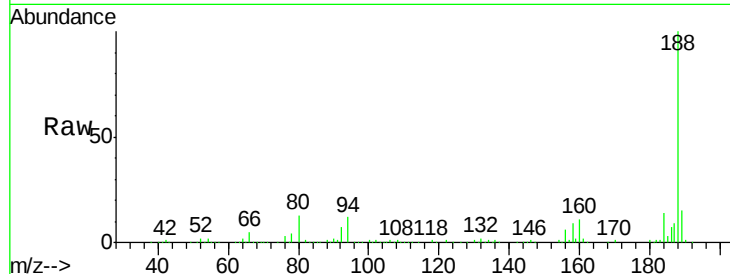


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

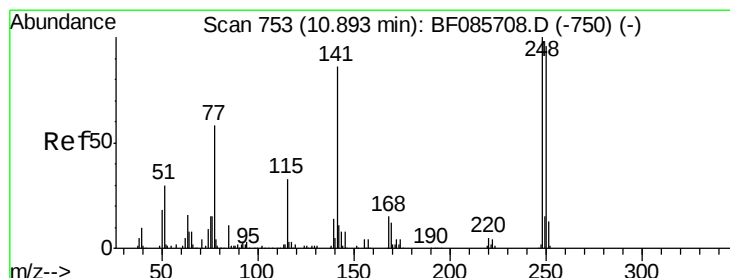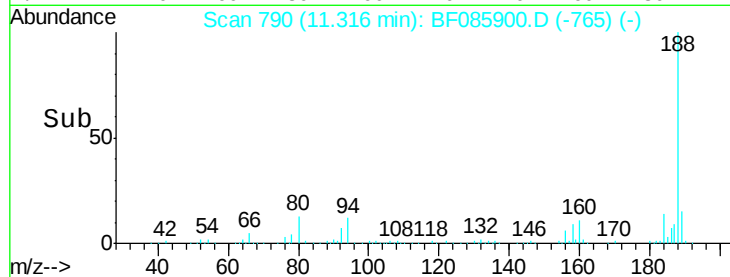
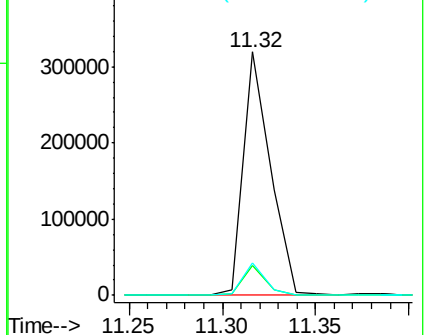



#66
4-Bromophenyl-phenylether
Concen: 4.98 ng
RT: 10.63 min Scan# 730
Delta R.T. -0.24 min
Lab File: BF085900.D
Acq: 30 Mar 2016 21:46

Tgt Ion:248 Resp: 16432
Ion Ratio Lower Upper
248 100
250 194.2 77.4 116.0#
141 391.7 63.6 95.4#

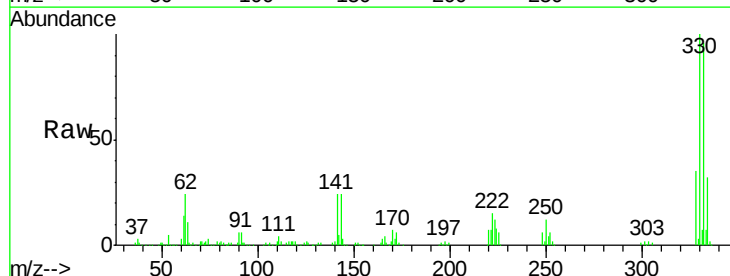

Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

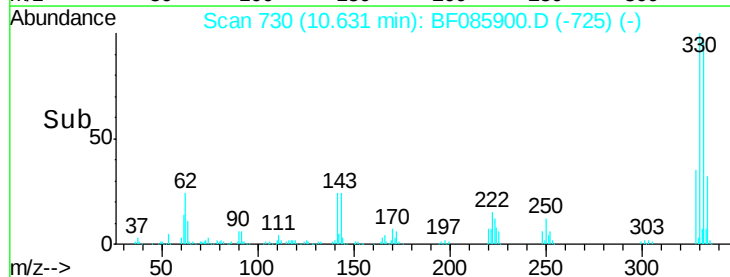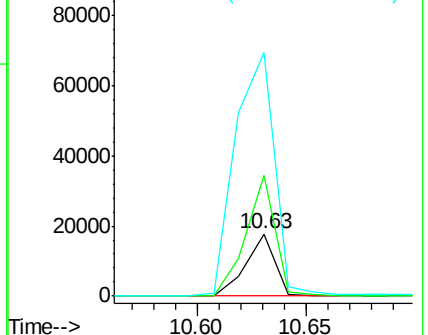

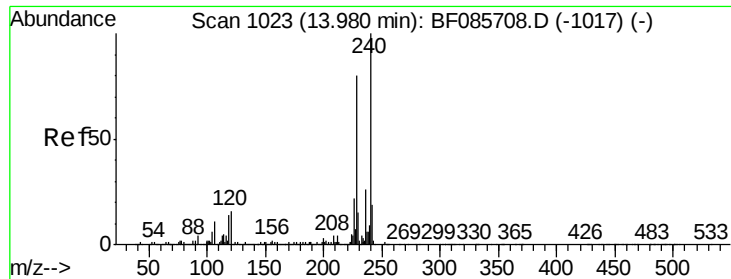

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.96 min Scan# 1021

Delta R.T. -0.01 min

Lab File: BF085900.D

Acq: 30 Mar 2016 21:46

Instrument :

BNA_F

ClientSampleId :

B-6


Tgt Ion:240 Resp: 225411

Ion Ratio Lower Upper

240 100

120 10.8 13.8 20.8#




236 26.7 20.6 30.8

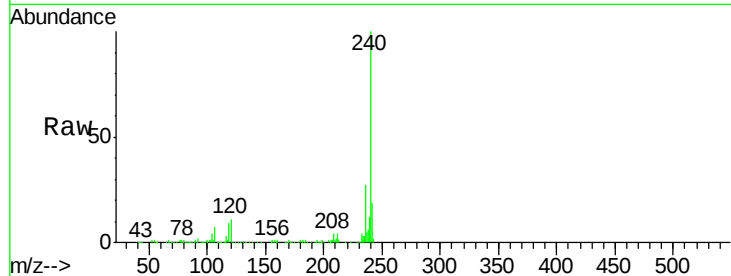

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

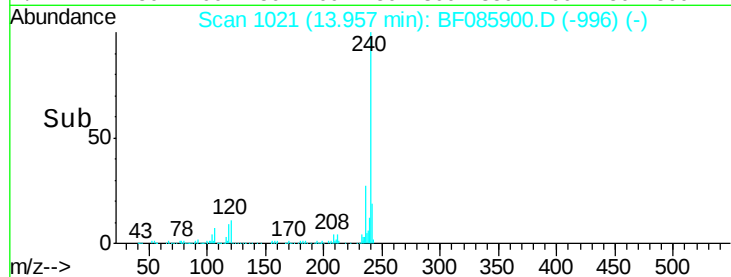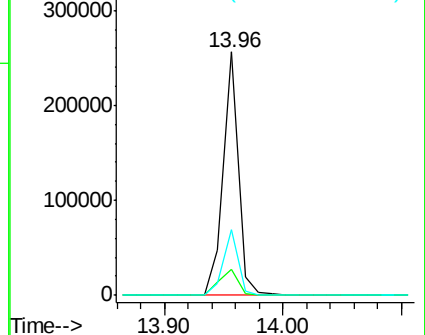

#78

Terphenyl-d14

Concen: 70.70 ng

RT: 12.91 min Scan# 929

Delta R.T. -0.00 min

Lab File: BF085900.D

Acq: 30 Mar 2016 21:46


Tgt Ion:244 Resp: 774936

Ion Ratio Lower Upper

244 100

212 7.2 6.1 9.1



122 12.3 10.2 15.4




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

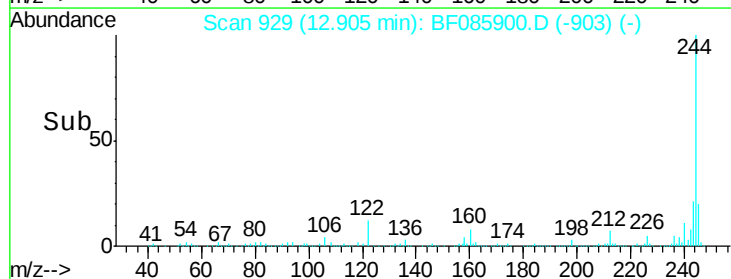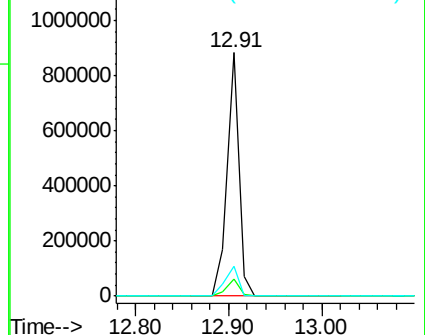


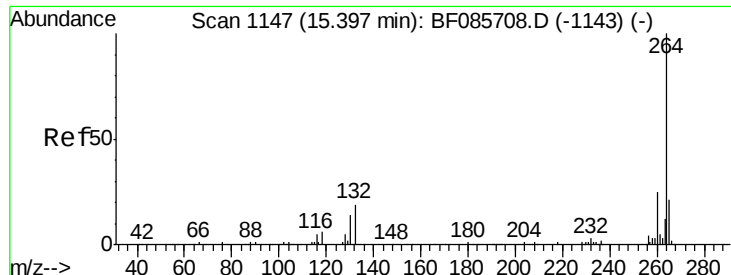

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.37 min Scan# 1145
Delta R.T. -0.00 min
Lab File: BF085900.D
Acq: 30 Mar 2016 21:46

Instrument :
BNA_F
ClientSampleId :
B-6

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.0	19.4	29.2
265	21.3	17.2	25.8

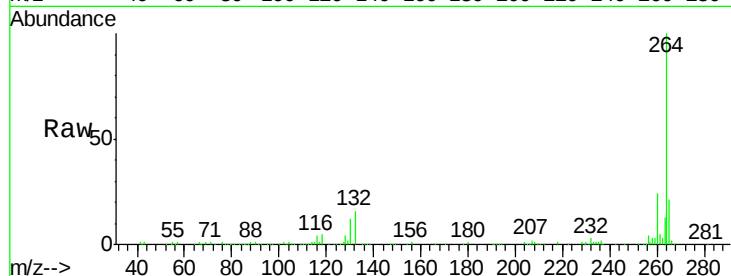

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

