
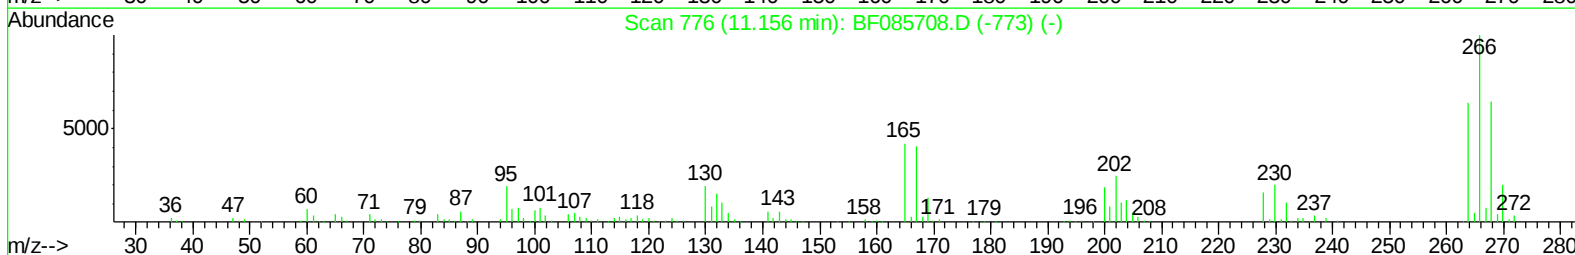
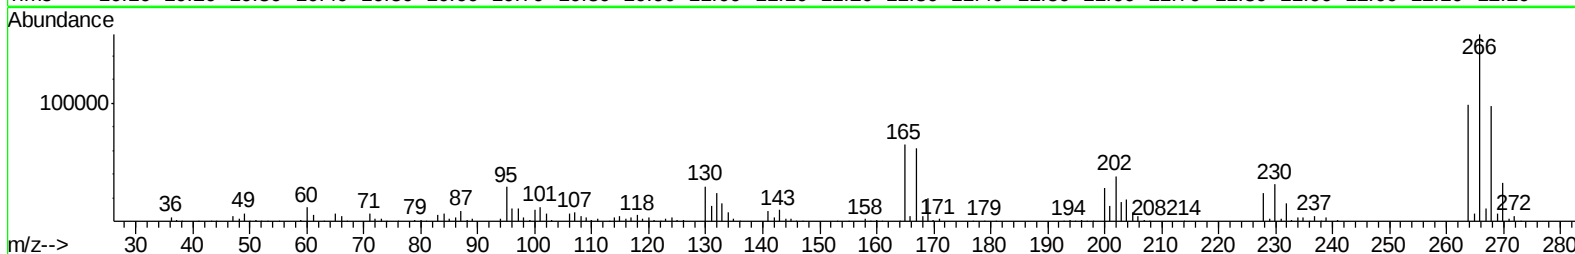


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
Data File : BF085877.D
Acq On : 30 Mar 2016 10:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 04:06:01 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 30 12:31:18 2016
Response via : Initial Calibration

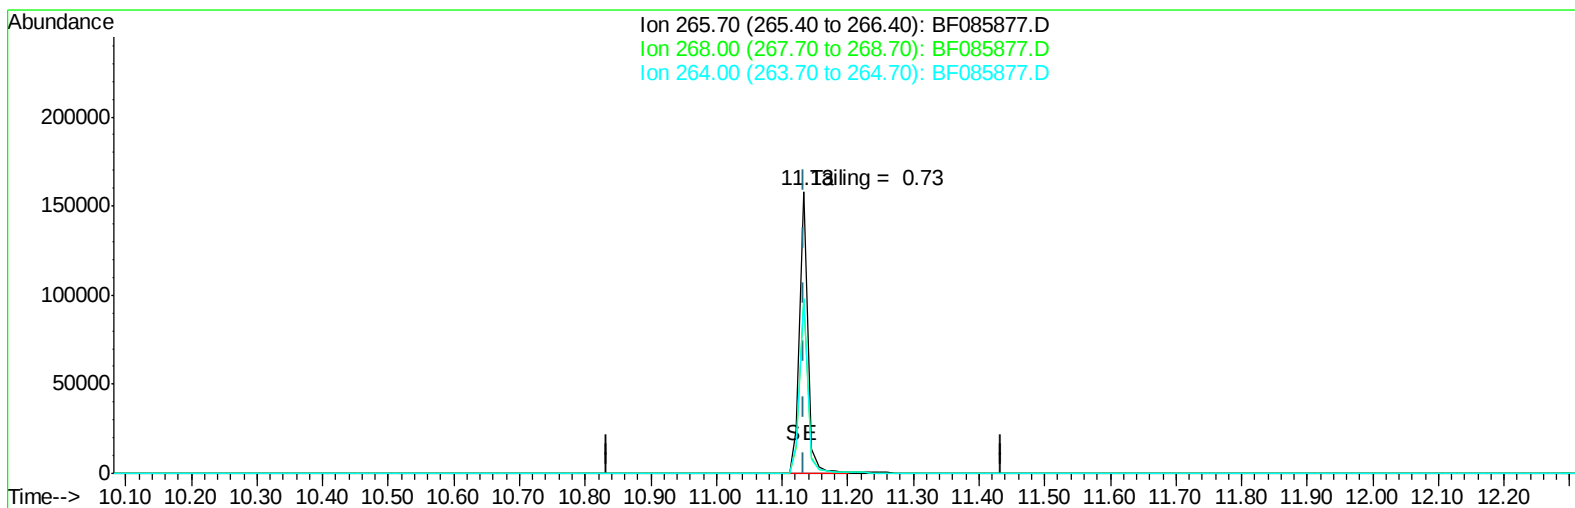

TIC: BF085877.D

(69) Pentachlorophenol (C)




11.134min (-0.000) 0.00ng

response 142530

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	61.89
264.00	63.30	62.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
Data File : BF085877.D
Acq On : 30 Mar 2016 10:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 04:06:01 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 30 12:31:18 2016
Response via : Initial Calibration

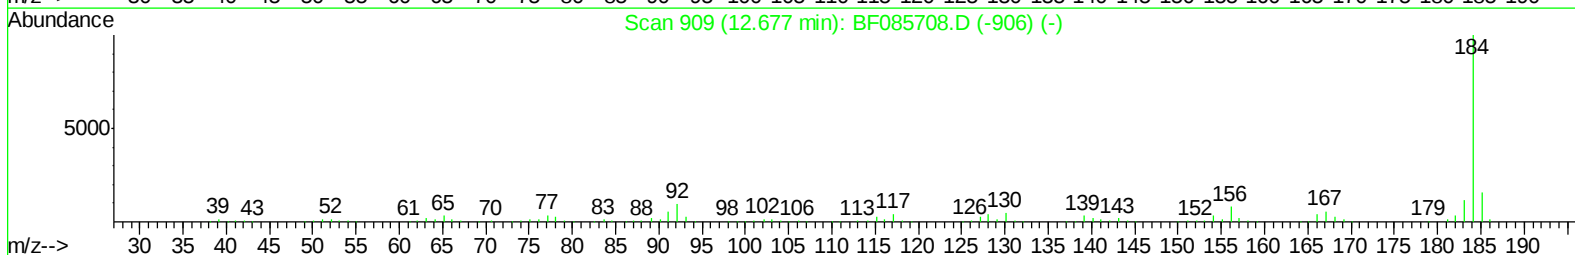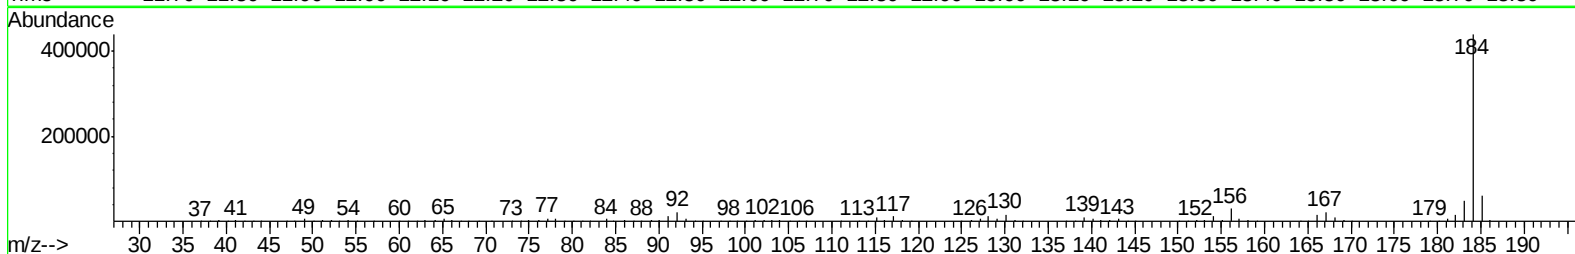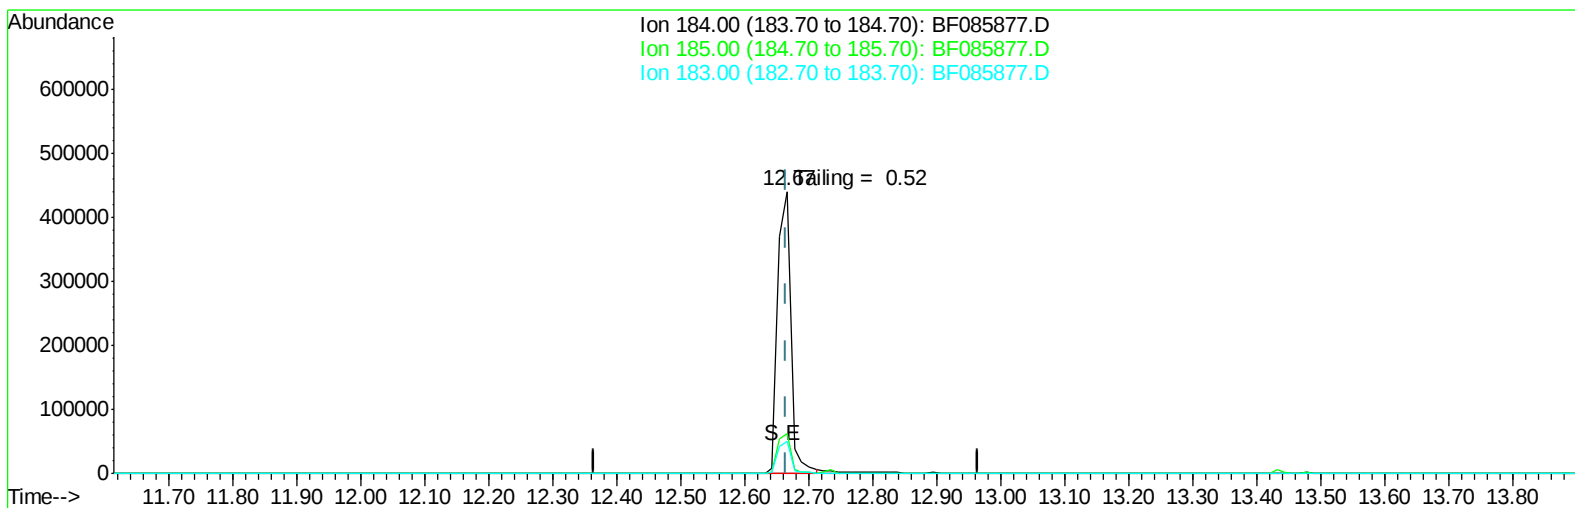

TIC: BF085877.D

(76) Benzidine

12.665min (0.000) 27718.56ng

response 630614

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	13.97
183.00	11.80	11.39
0.00	0.00	0.00