
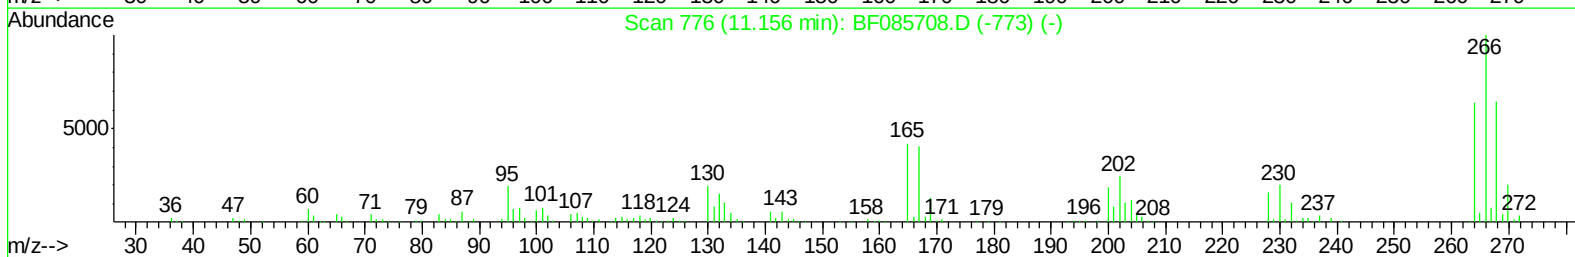
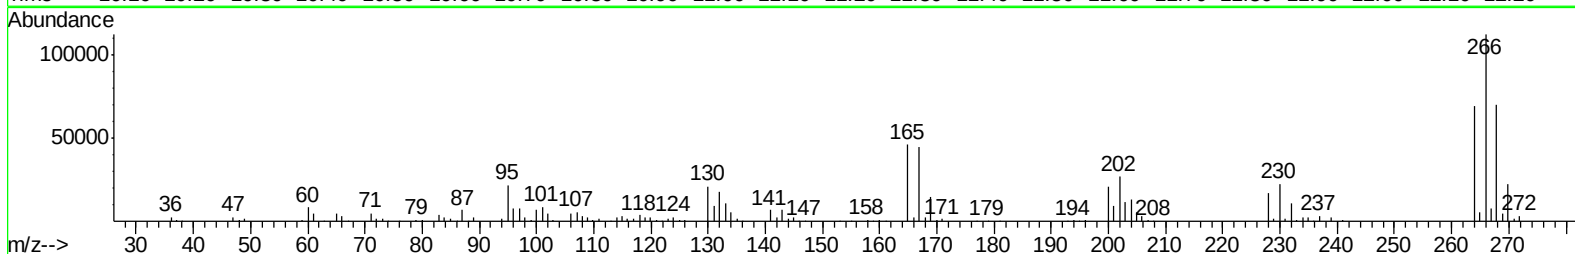


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
Data File : BF085902.D
Acq On : 31 Mar 2016 00:40
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 04:07:33 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 30 12:31:18 2016
Response via : Initial Calibration

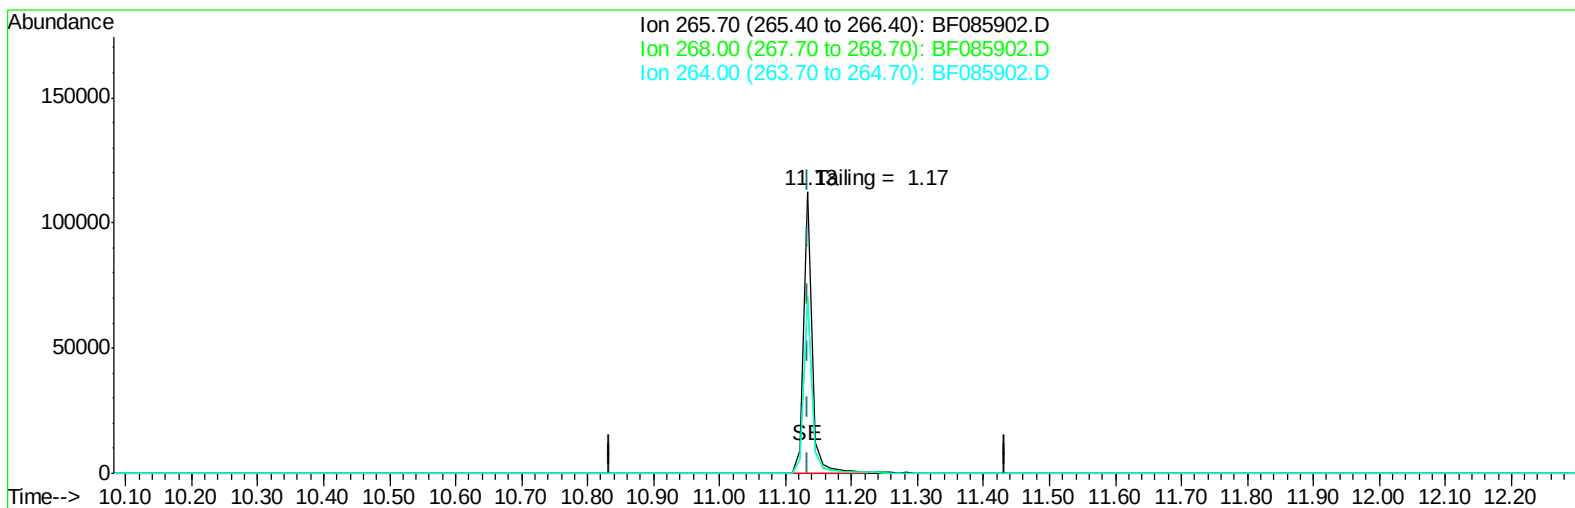

TIC: BF085902.D

(69) Pentachlorophenol (C)




11.133min (-0.000) 33073.73ng

response 99718

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.74
264.00	63.30	61.55
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
Data File : BF085902.D
Acq On : 31 Mar 2016 00:40
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 04:07:33 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 30 12:31:18 2016
Response via : Initial Calibration

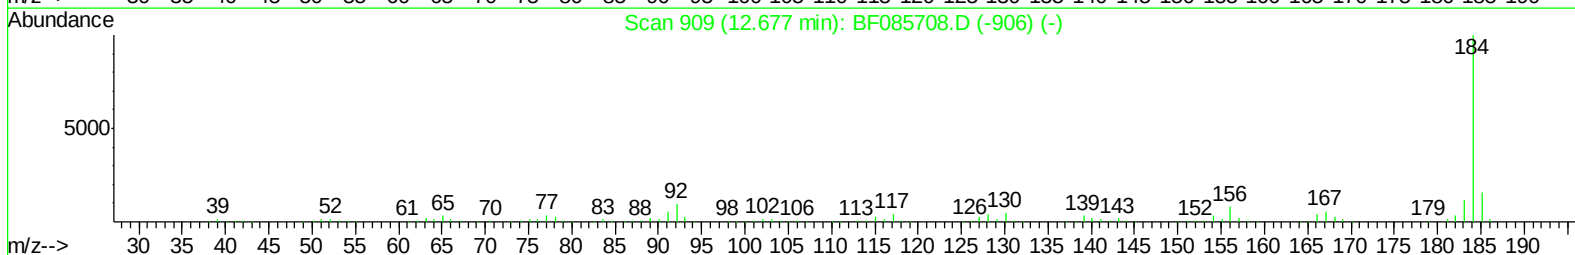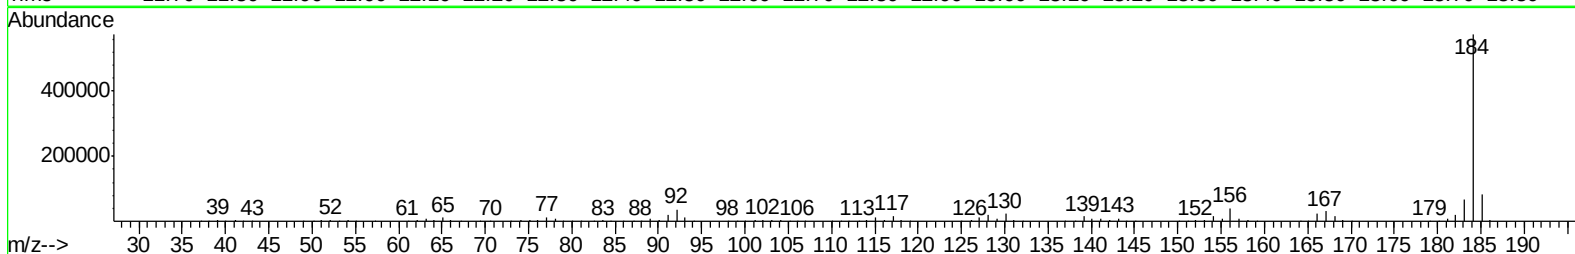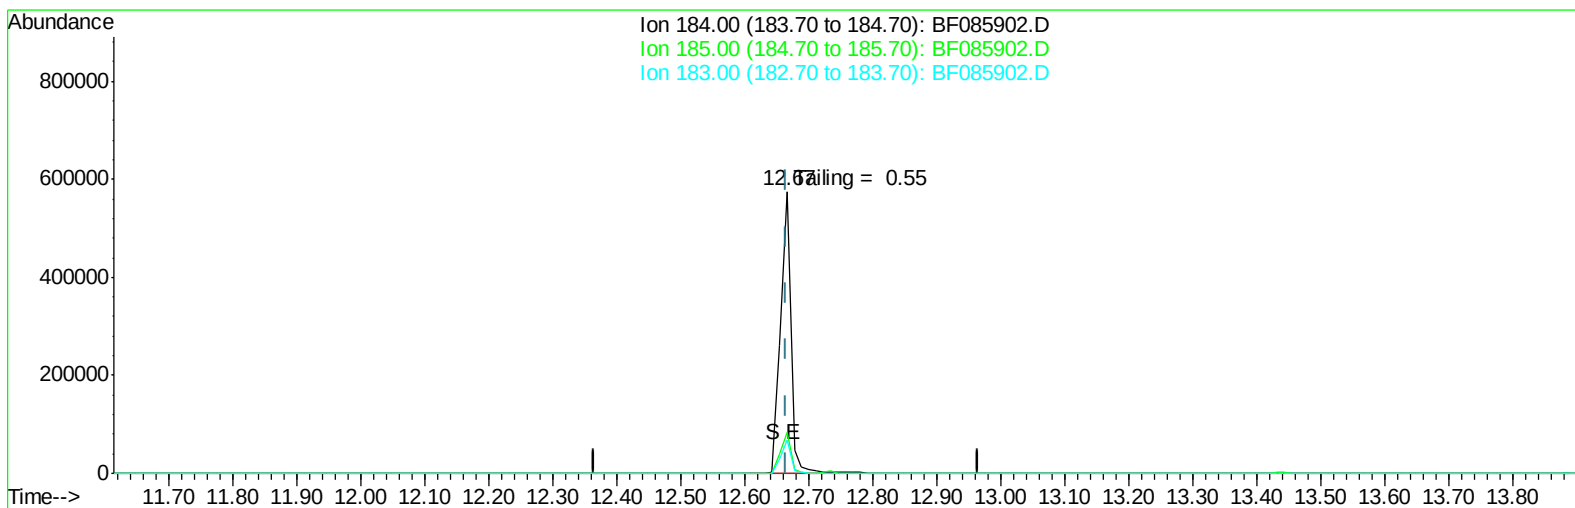

TIC: BF085902.D

(76) Benzidine

12.665min (-0.000) 16054.05ng

response 638321

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.37
183.00	11.80	11.62
0.00	0.00	0.00