

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
 Data File : BF085891.D
 Acq On : 30 Mar 2016 17:31
 Operator : UM/SJ
 Sample : H2017-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-COMP

Quant Time: Mar 31 03:40:40 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 30 12:31:18 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.80	152	104440	20.00	ng	0.00
21) Naphthalene-d8	8.08	136	444516	20.00	ng	-0.01
38) Acenaphthene-d10	9.84	164	192291	20.00	ng	0.00
63) Phenanthrene-d10	11.32	188	365496	20.00	ng	-0.01
75) Chrysene-d12	13.96	240	252355	20.00	ng	-0.01
86) Perylene-d12	15.37	264	211243	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	801621	127.83	ng	0.00
7) Phenol-d6	6.44	99	1143107	143.37	ng	-0.01
23) Nitrobenzene-d5	7.36	82	653237	82.76	ng	-0.01
41) 2,4,6-Tribromophenol	10.63	330	274334	150.16	ng	0.00
44) 2-Fluorobiphenyl	9.17	172	1153557	100.23	ng	0.00
78) Terphenyl-d14	12.91	244	874641	71.28	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.56	163	209069	14.33	ng	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
Data File : BF085891.D
Acq On : 30 Mar 2016 17:31
Operator : UM/SJ
Sample : H2017-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-COMP

Quant Time: Mar 31 03:40:40 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 30 12:31:18 2016
Response via : Initial Calibration

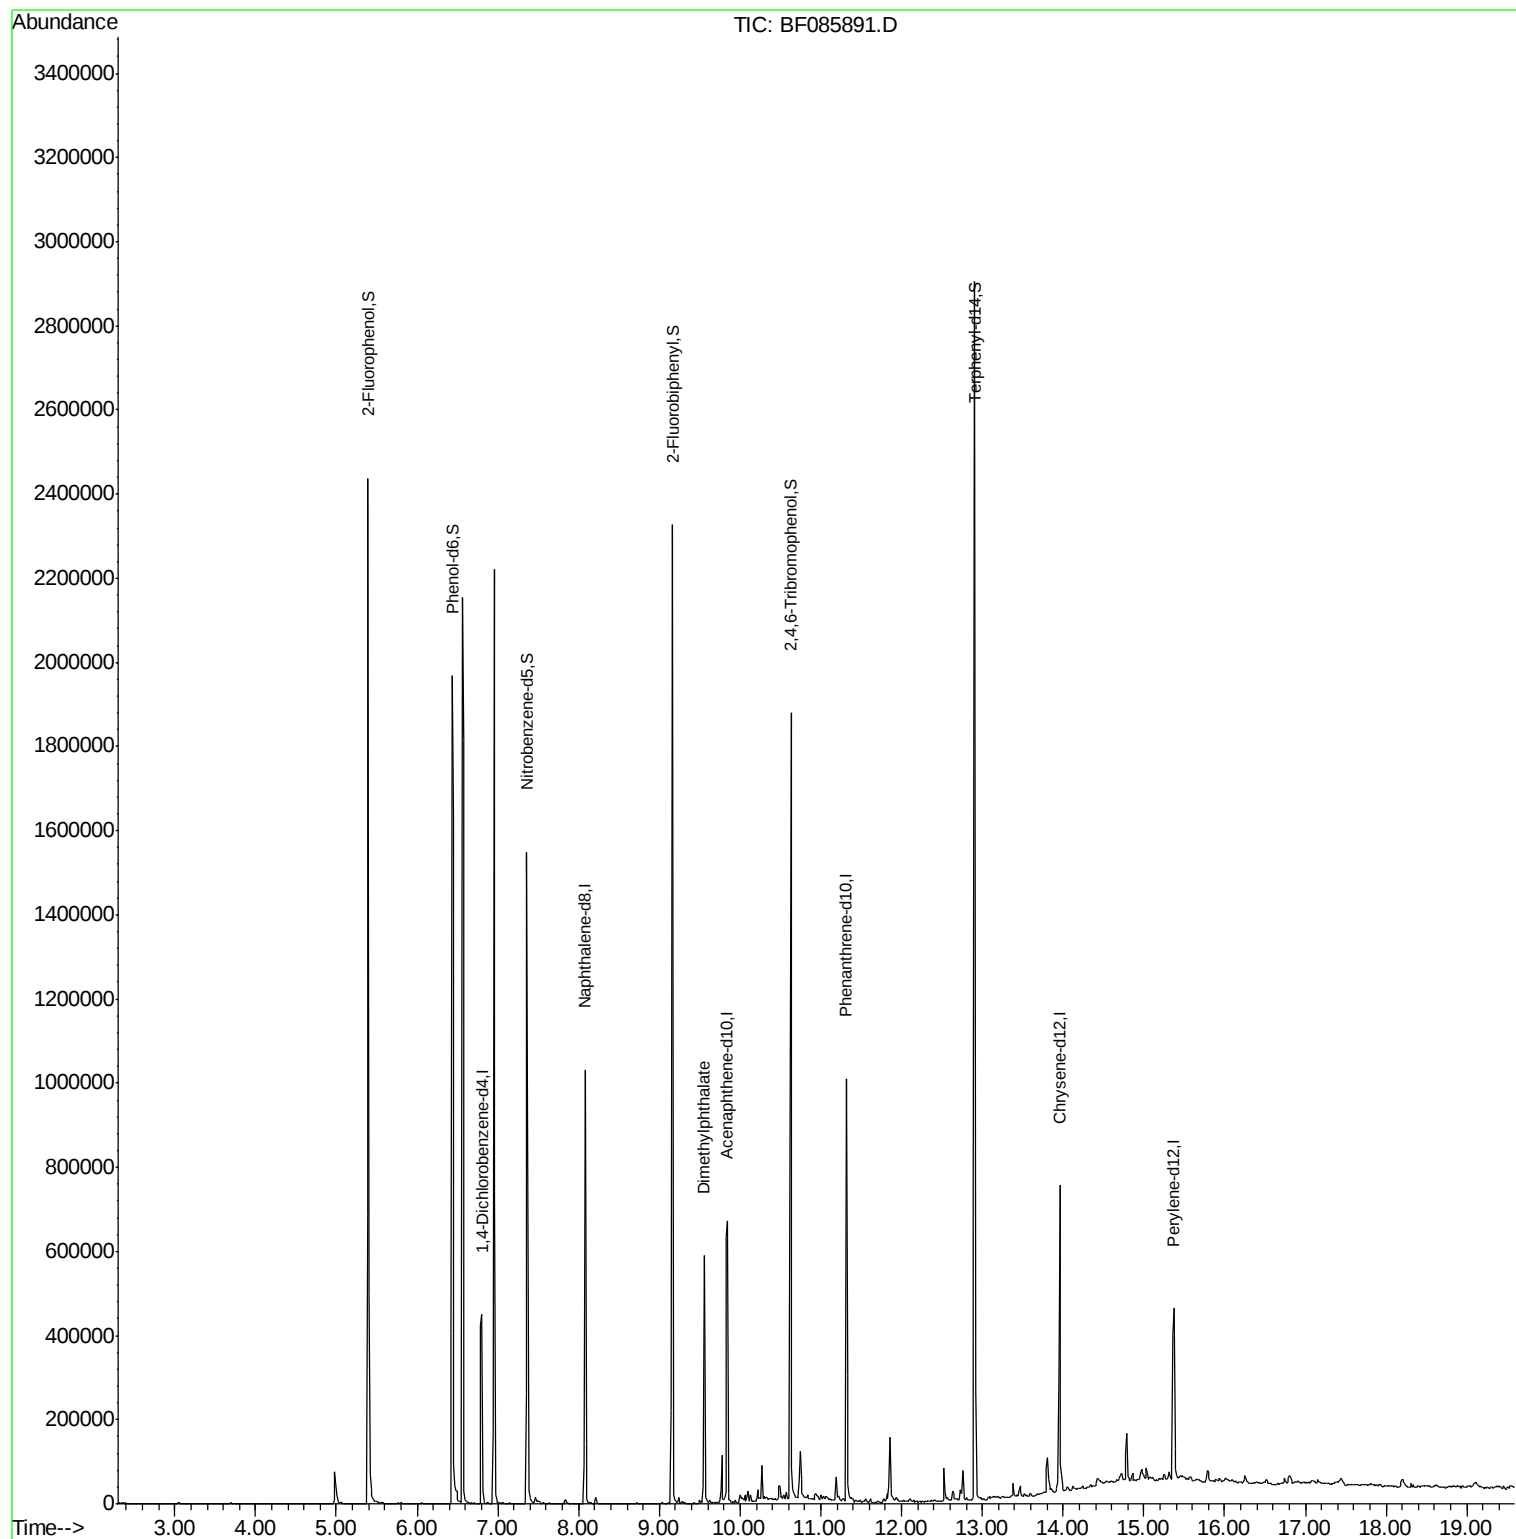



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.80 min Scan# 395

Delta R.T. -0.00 min

Lab File: BF085891.D

Acq: 30 Mar 2016 17:31

Instrument :

BNA_F

ClientSampleId :

SB-COMP


Tgt Ion:152 Resp: 104440

Ion Ratio Lower Upper

152 100

150 154.1 124.2 186.2




115 53.2 47.0 70.6

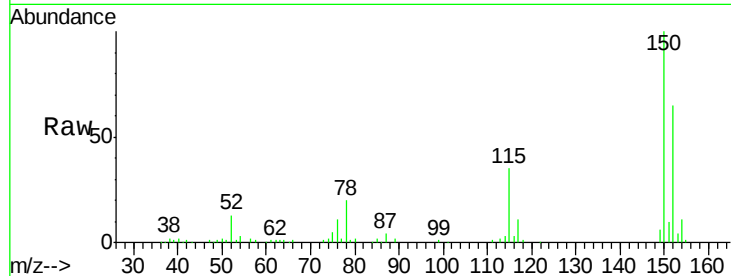

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

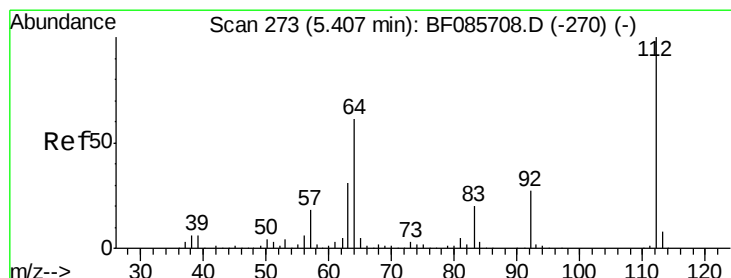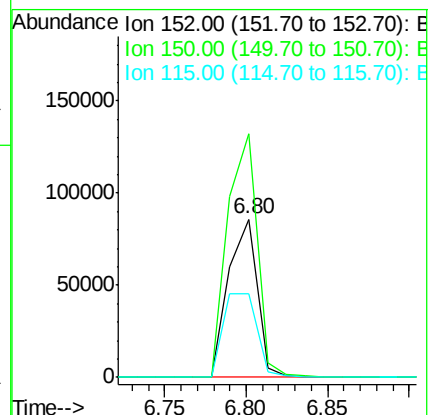

#5

2-Fluorophenol

Concen: 127.83 ng

RT: 5.40 min Scan# 272

Delta R.T. -0.00 min

Lab File: BF085891.D

Acq: 30 Mar 2016 17:31


Tgt Ion:112 Resp: 801621

Ion Ratio Lower Upper

112 100

64 54.5 39.9 59.9



63 28.0 20.2 30.2



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

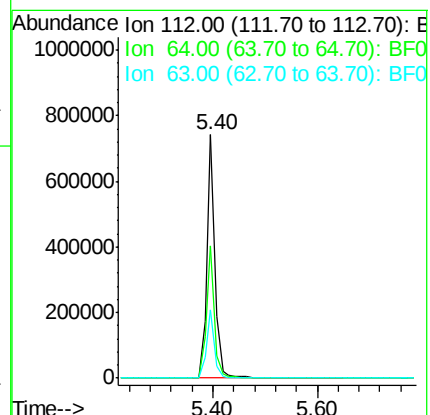



#7

Phenol-d6

Concen: 143.37 ng

RT: 6.44 min Scan# 363

Delta R.T. -0.01 min

Lab File: BF085891.D

Acq: 30 Mar 2016 17:31

Instrument :

BNA_F

ClientSampleId :

SB-COMP





Tgt Ion: 99 Resp: 1143107

Ion Ratio Lower Upper

99 100

42 15.6 11.1 16.7

71 32.8 24.9 37.3

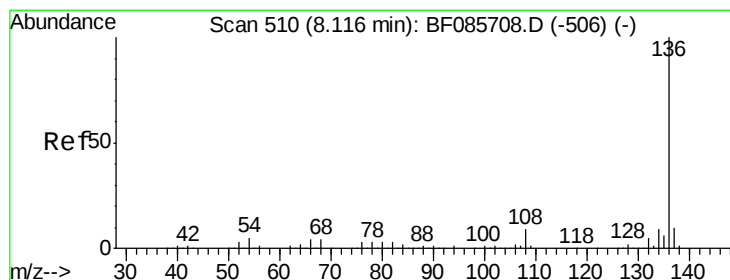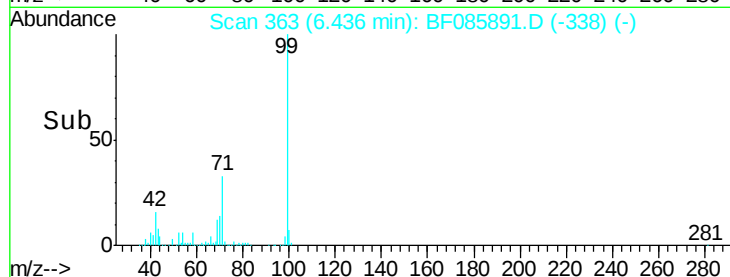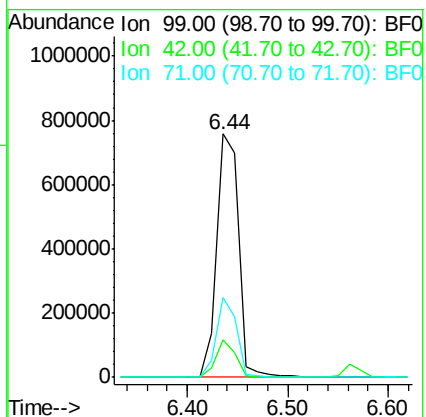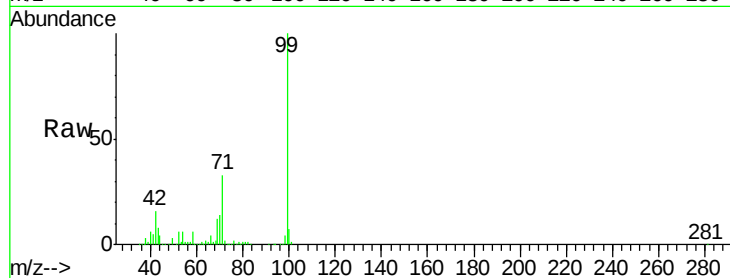

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.08 min Scan# 507

Delta R.T. -0.01 min

Lab File: BF085891.D

Acq: 30 Mar 2016 17:31

Tgt Ion: 136 Resp: 444516




Ion Ratio Lower Upper

136 100

137 11.1 9.1 13.7

54 7.4 7.4 11.0

68 6.2 5.8 8.8

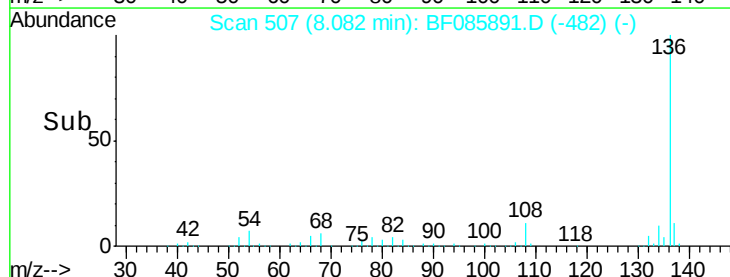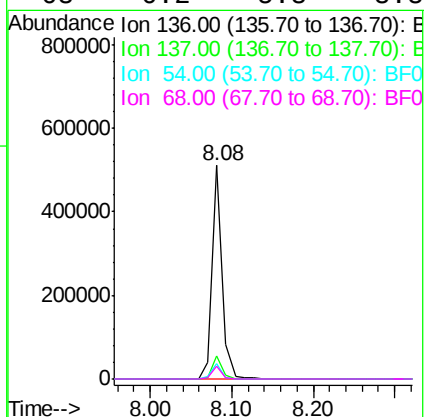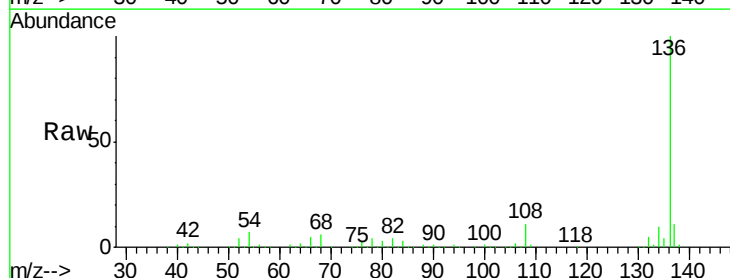







#23
 Nitrobenzene-d5
 Concen: 82.76 ng
 RT: 7.36 min Scan# 444
 Delta R.T. -0.01 min
 Lab File: BF085891.D
 Acq: 30 Mar 2016 17:31

Instrument :
 BNA_F
 ClientSampleId :
 SB-COMP

Tgt Ion: 82 Resp: 653237
 Ion Ratio Lower Upper
 82 100
 128 42.7 41.8 62.8
 54 47.1 33.4 50.0

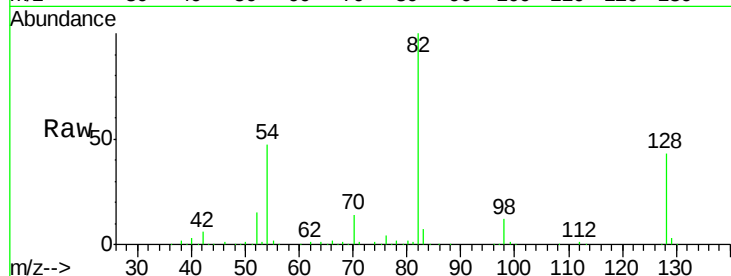


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0


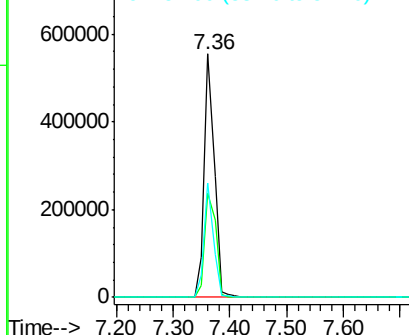



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.84 min Scan# 661
 Delta R.T. -0.00 min
 Lab File: BF085891.D
 Acq: 30 Mar 2016 17:31

Tgt Ion: 164 Resp: 192291
 Ion Ratio Lower Upper
 164 100
 162 105.4 82.1 123.1
 160 50.0 37.4 56.2



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

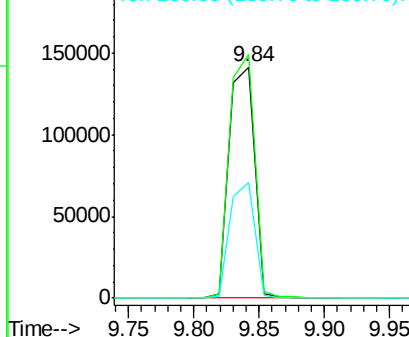


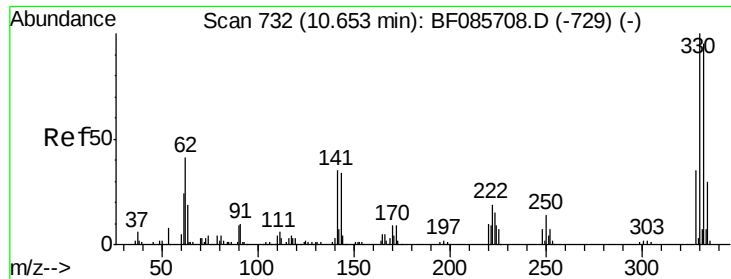




#41
 2,4,6-Tribromophenol
 Concen: 150.16 ng
 RT: 10.63 min Scan# 730
 Delta R.T. -0.00 min
 Lab File: BF085891.D
 Acq: 30 Mar 2016 17:31

Instrument :
 BNA_F
 ClientSampleId :
 SB-COMP

Tgt Ion:330 Resp: 274334
 Ion Ratio Lower Upper
 330 100
 332 96.4 78.2 117.2
 141 34.3 31.5 47.3




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

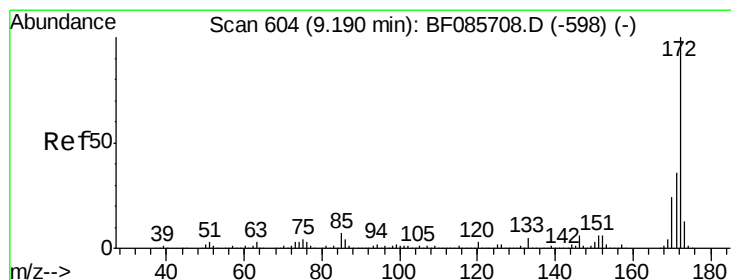
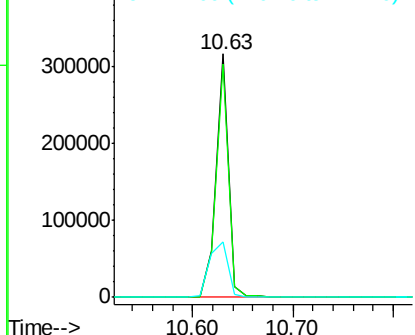



#44
 2-Fluorobiphenyl
 Concen: 100.23 ng
 RT: 9.17 min Scan# 602
 Delta R.T. -0.00 min
 Lab File: BF085891.D
 Acq: 30 Mar 2016 17:31

Tgt Ion:172 Resp: 1153557
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.4 44.2
 170 24.2 19.8 29.6

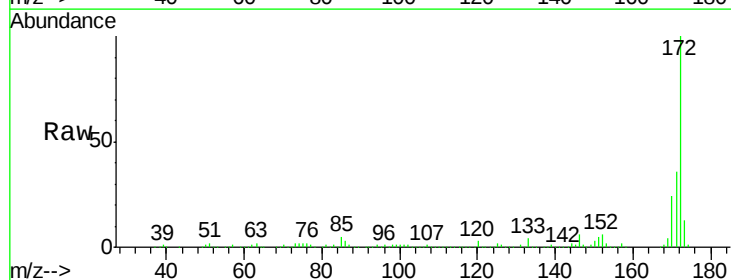

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

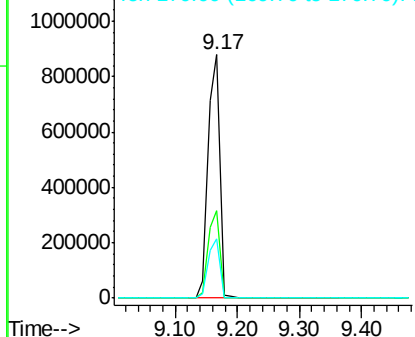

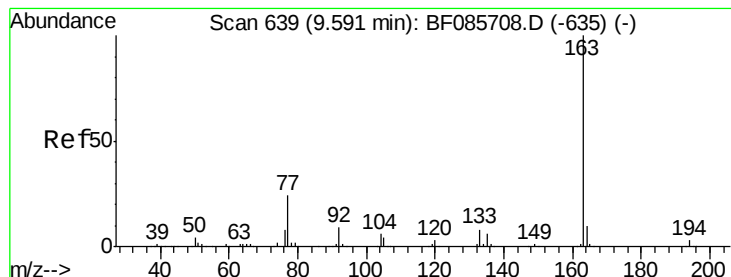

#49

Dimethylphthalate

Concen: 14.33 ng

RT: 9.56 min Scan# 636

Delta R.T. -0.01 min

Lab File: BF085891.D

Acq: 30 Mar 2016 17:31

Instrument :

BNA_F

ClientSampleId :

SB-COMP


Tgt Ion:163 Resp: 209069

Ion Ratio Lower Upper

163 100

194 3.1 2.9 4.3




164 10.4 8.3 12.5



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

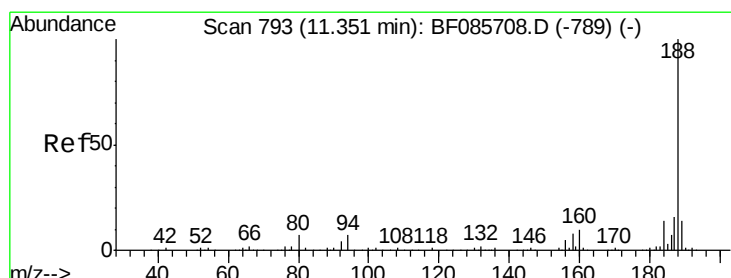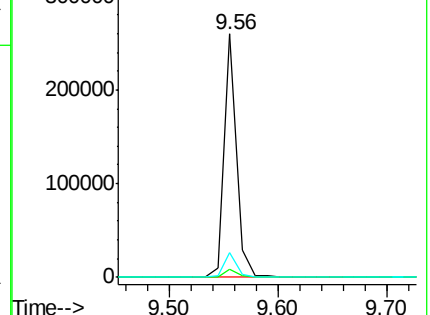

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.32 min Scan# 790

Delta R.T. -0.01 min

Lab File: BF085891.D

Acq: 30 Mar 2016 17:31


Tgt Ion:188 Resp: 365496

Ion Ratio Lower Upper

188 100

94 12.0 5.4 8.0#



80 12.9 5.5 8.3#




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0



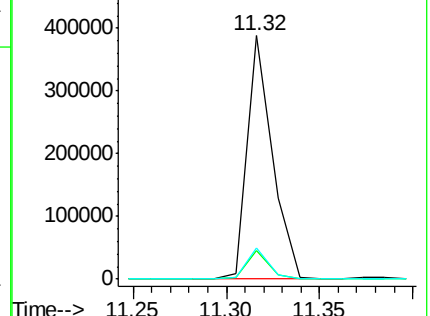
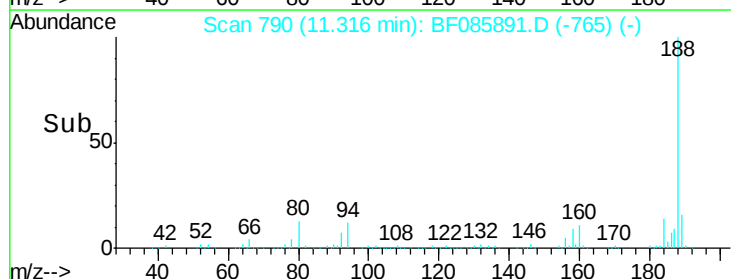


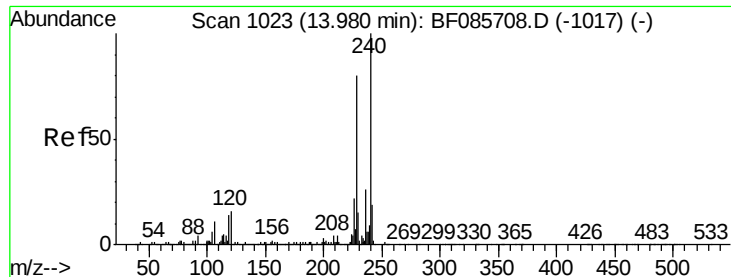

#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.96 min Scan# 1021
Delta R.T. -0.01 min
Lab File: BF085891.D
Acq: 30 Mar 2016 17:31




Instrument :
BNA_F
ClientSampleId :
SB-COMP


Tgt Ion:240 Resp: 252355
Ion Ratio Lower Upper
240 100
120 9.9 13.8 20.8#
236 26.6 20.6 30.8

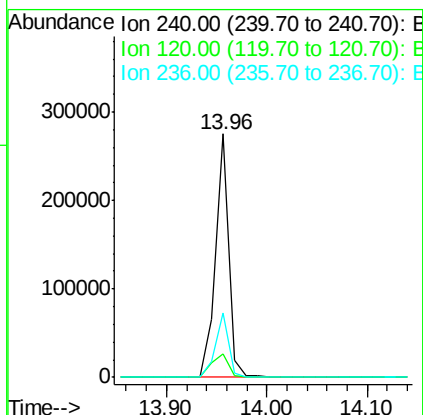

#78
Terphenyl-d14
Concen: 71.28 ng
RT: 12.91 min Scan# 929
Delta R.T. -0.00 min
Lab File: BF085891.D
Acq: 30 Mar 2016 17:31

Tgt Ion:244 Resp: 874641
Ion Ratio Lower Upper
244 100
212 7.4 6.1 9.1
122 12.1 10.2 15.4

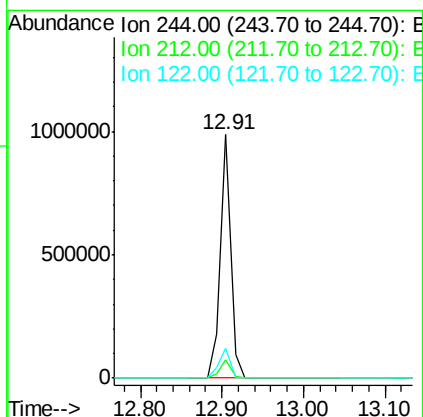


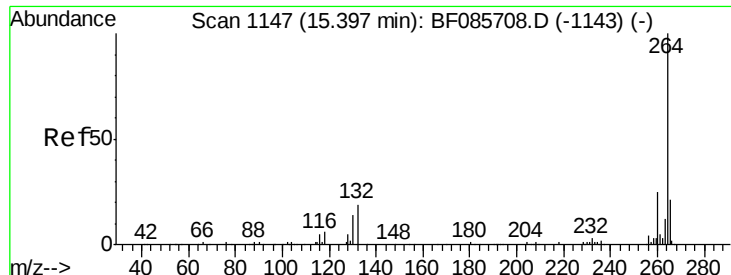

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.37 min Scan# 1145
Delta R.T. -0.00 min
Lab File: BF085891.D
Acq: 30 Mar 2016 17:31

Instrument :
BNA_F
ClientSampleId :
SB-COMP

Tgt Ion: 264 Resp: 211243
Ion Ratio Lower Upper
264 100
260 24.0 19.4 29.2
265 21.5 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

