

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
 Data File : BF085919.D
 Acq On : 31 Mar 2016 8:38
 Operator : UM/SJ
 Sample : H2010-02
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AMBOY-SB28COMP0.5-15.0

Quant Time: Mar 31 16:33:19 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 30 12:31:18 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.80	152	96694	20.00	ng	0.00
21) Naphthalene-d8	8.08	136	393324	20.00	ng	-0.01
38) Acenaphthene-d10	9.83	164	157181	20.00	ng	-0.01
63) Phenanthrene-d10	11.32	188	268269	20.00	ng	-0.01
75) Chrysene-d12	13.96	240	195580	20.00	ng	-0.01
86) Perylene-d12	15.37	264	193339	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	831984	143.30	ng	0.00
7) Phenol-d6	6.44	99	946008	128.15	ng	-0.01
23) Nitrobenzene-d5	7.36	82	579878	83.02	ng	-0.01
41) 2,4,6-Tribromophenol	10.63	330	217977	145.96	ng	0.00
44) 2-Fluorobiphenyl	9.17	172	1002658	106.58	ng	0.00
78) Terphenyl-d14	12.90	244	694294	73.01	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.56	163	167139	14.02	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
Data File : BF085919.D
Acq On : 31 Mar 2016 8:38
Operator : UM/SJ
Sample : H2010-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AMBOY-SB28COMP0.5-15.0

Quant Time: Mar 31 16:33:19 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 30 12:31:18 2016
Response via : Initial Calibration

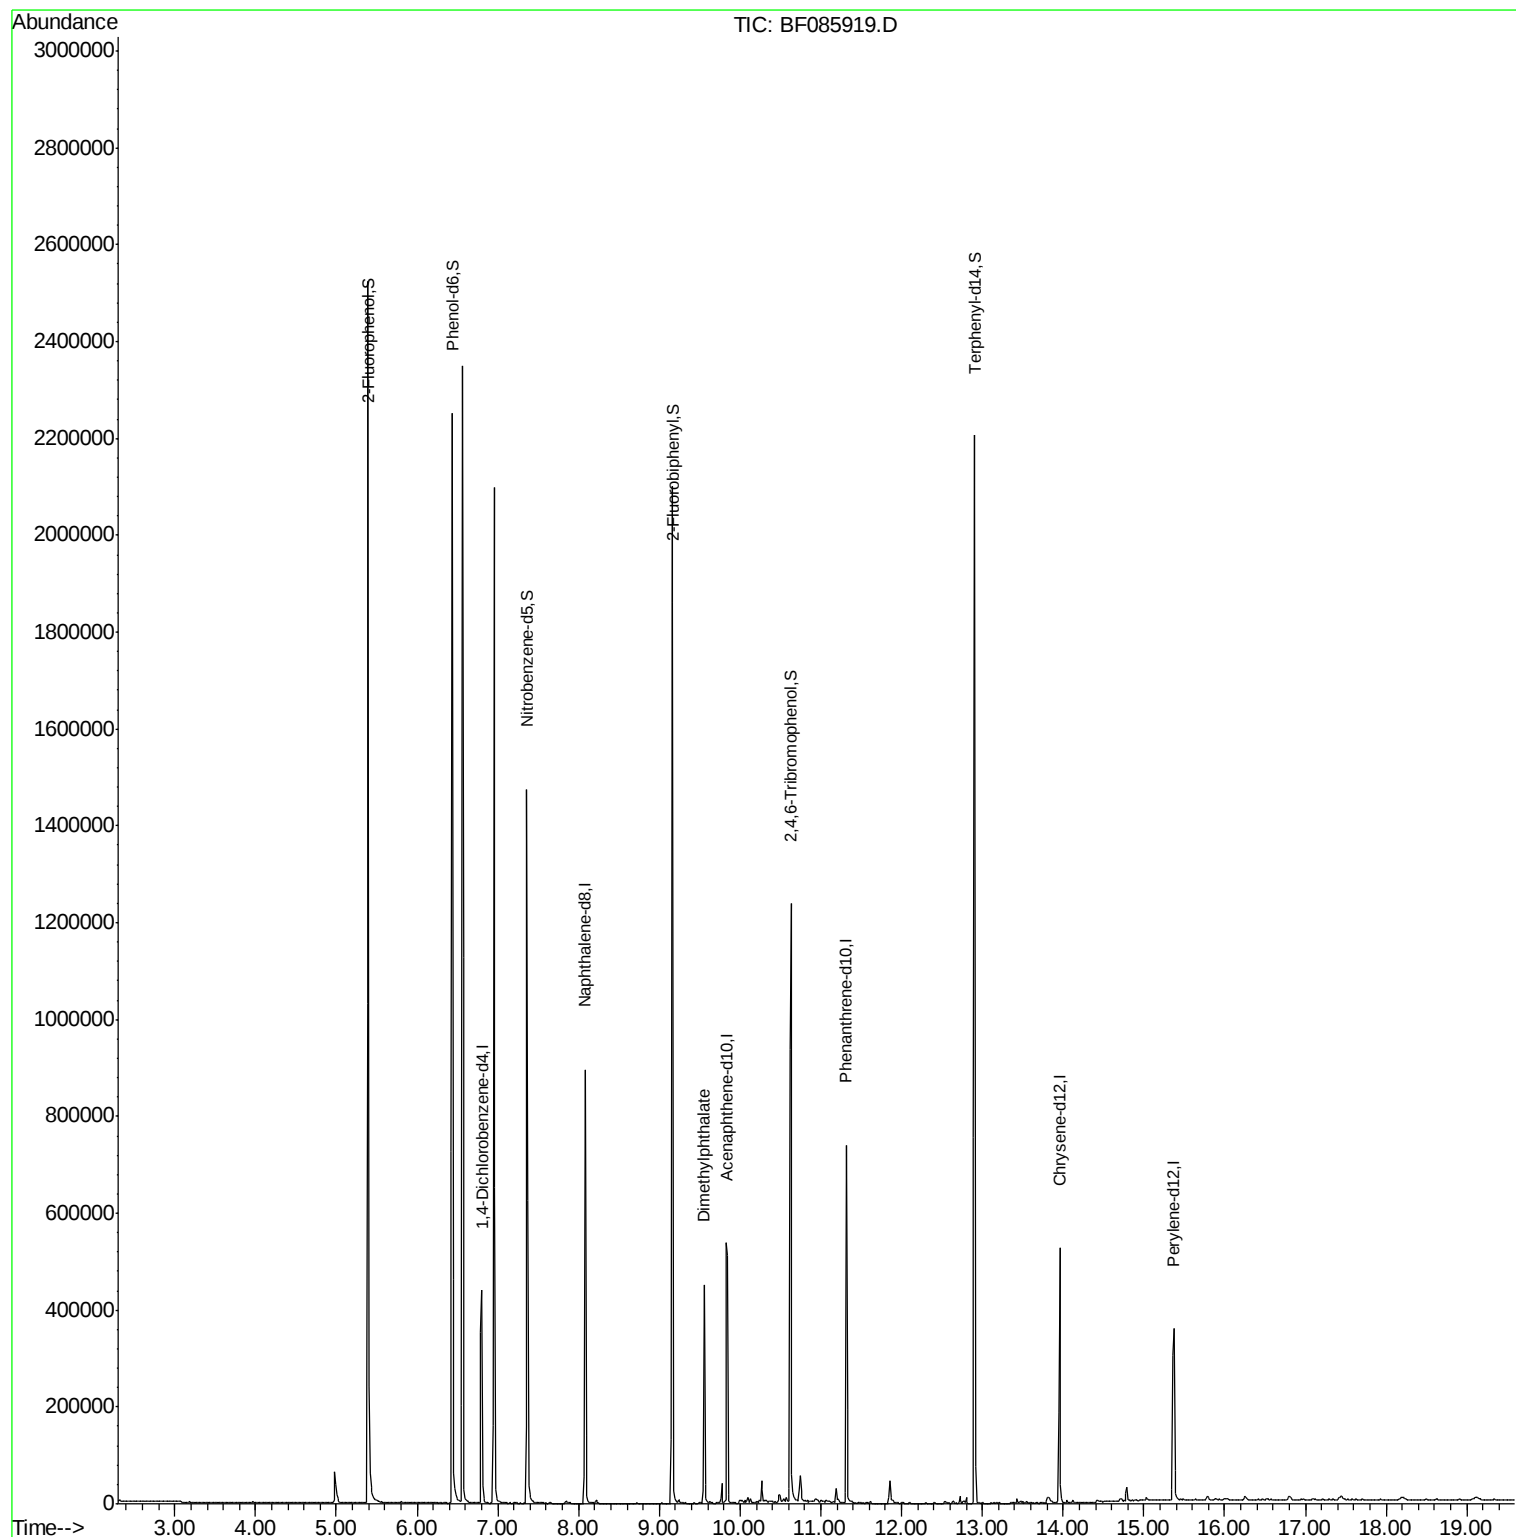

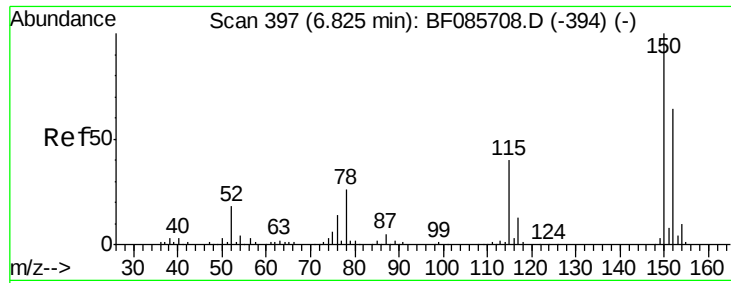

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.80 min Scan# 395

Delta R.T. -0.00 min

Lab File: BF085919.D

Acq: 31 Mar 2016 8:38

Instrument :

BNA_F

ClientSampleId :

AMBOY-SB28COMP0.5-15.0


Tgt Ion:152 Resp: 96694

Ion Ratio Lower Upper

152 100

150 158.3 124.2 186.2




115 54.0 47.0 70.6

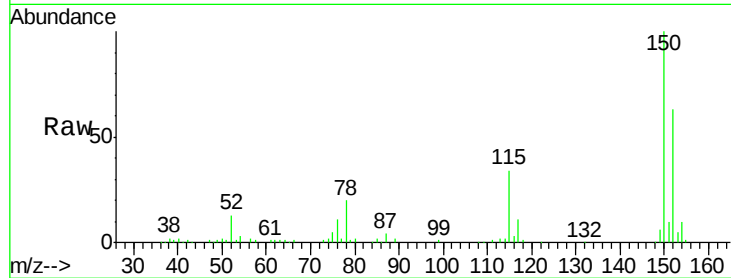

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

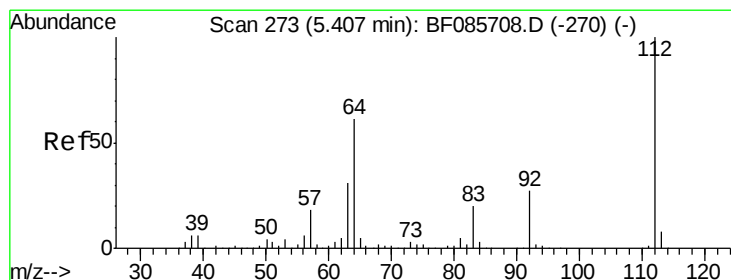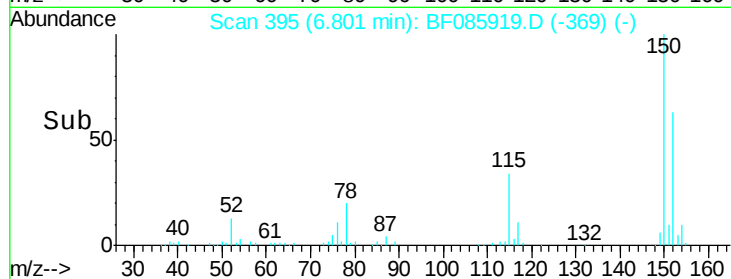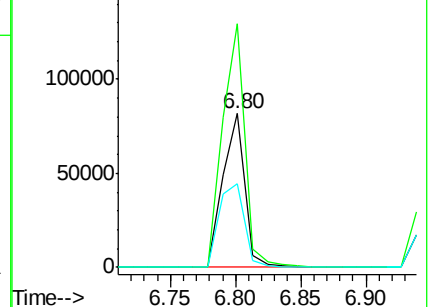

#5

2-Fluorophenol

Concen: 143.30 ng

RT: 5.40 min Scan# 272

Delta R.T. -0.00 min

Lab File: BF085919.D

Acq: 31 Mar 2016 8:38


Tgt Ion:112 Resp: 831984

Ion Ratio Lower Upper

112 100

64 53.8 39.9 59.9



63 27.3 20.2 30.2

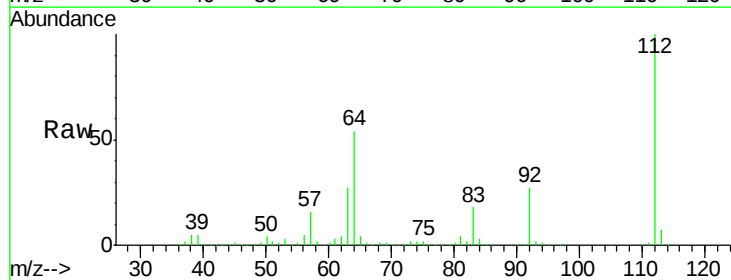

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

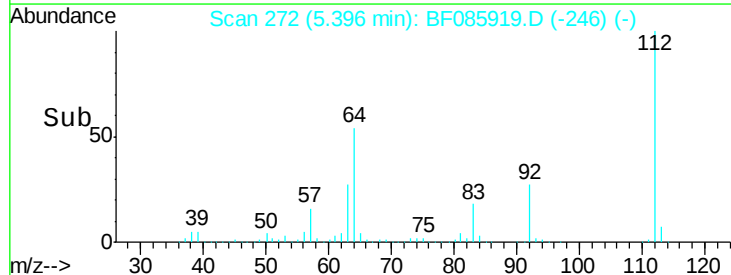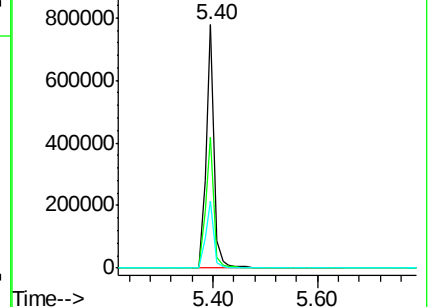



#7

Phenol-d6

Concen: 128.15 ng

RT: 6.44 min Scan# 363

Delta R.T. -0.01 min

Lab File: BF085919.D

Acq: 31 Mar 2016 8:38

Instrument :

BNA_F

ClientSampleId :

AMBOY-SB28COMP0.5-15.0


Tgt Ion: 99 Resp: 946008

Ion Ratio Lower Upper

99 100

42 15.4 11.1 16.7




71 33.0 24.9 37.3

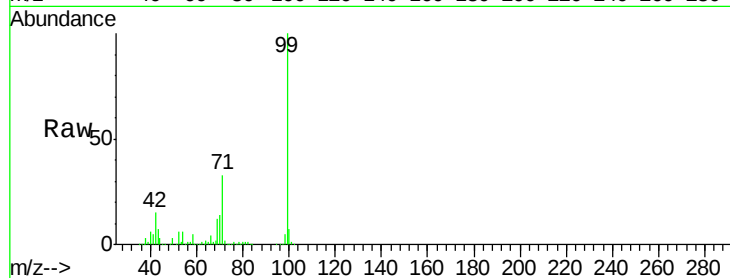

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

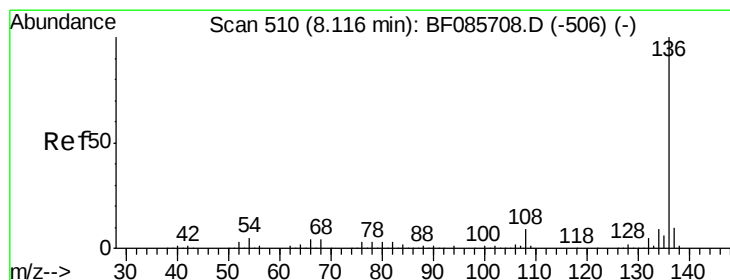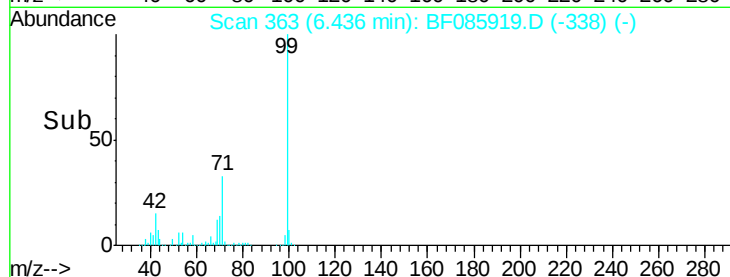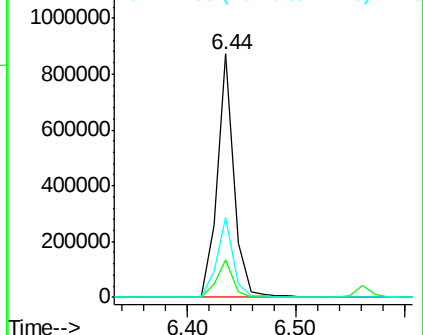

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.08 min Scan# 507

Delta R.T. -0.01 min

Lab File: BF085919.D

Acq: 31 Mar 2016 8:38

Tgt Ion: 136 Resp: 393324


Ion Ratio Lower Upper

136 100

137 11.1 9.1 13.7

54 7.1 7.4 11.0#

68 5.9 5.8 8.8


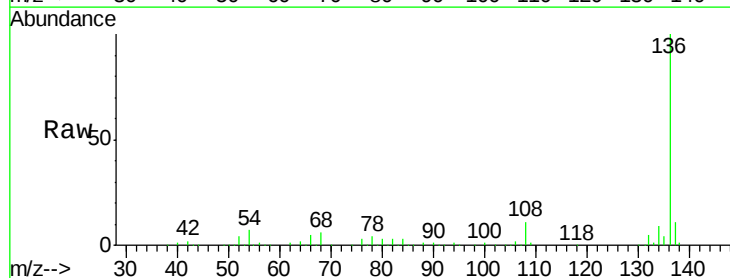


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

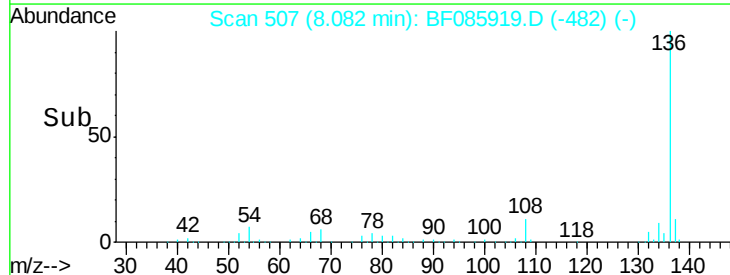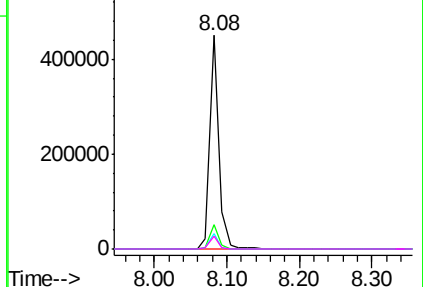







#23
 Nitrobenzene-d5
 Concen: 83.02 ng
 RT: 7.36 min Scan# 444
 Delta R.T. -0.01 min
 Lab File: BF085919.D
 Acq: 31 Mar 2016 8:38

Instrument :
 BNA_F
 ClientSampleId :
 AMBOY-SB28COMP0.5-15.0

Tgt Ion: 82 Resp: 579878
 Ion Ratio Lower Upper
 82 100
 128 42.2 41.8 62.8
 54 47.0 33.4 50.0

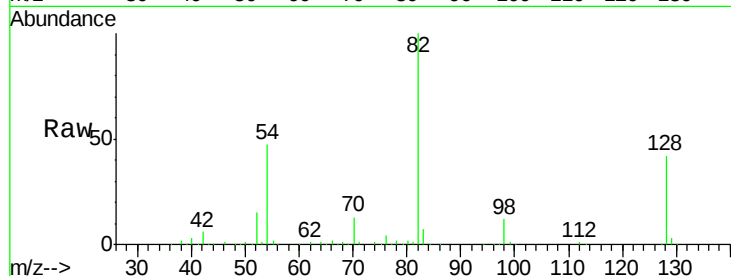


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

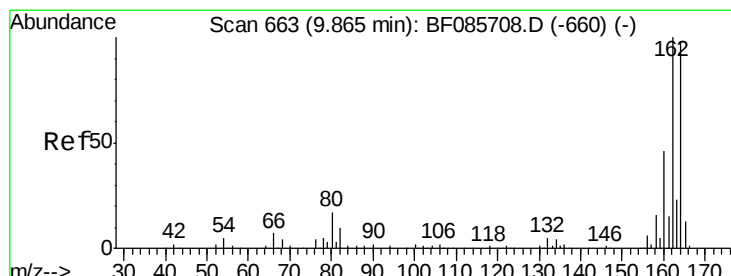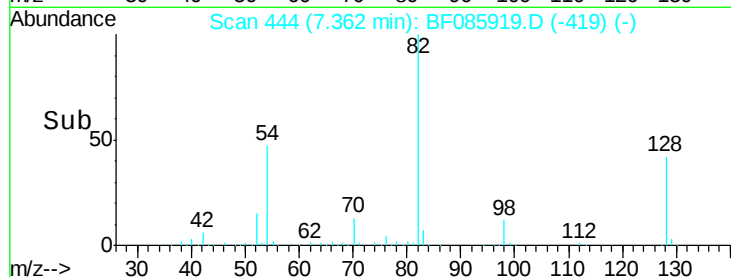
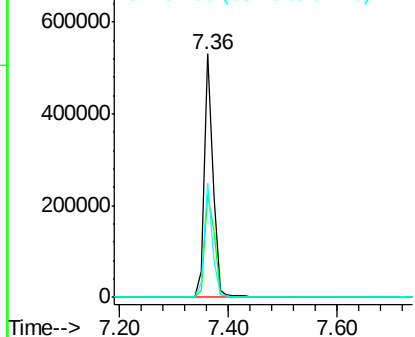



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.83 min Scan# 660
 Delta R.T. -0.01 min
 Lab File: BF085919.D
 Acq: 31 Mar 2016 8:38

Tgt Ion: 164 Resp: 157181
 Ion Ratio Lower Upper
 164 100
 162 100.9 82.1 123.1
 160 45.8 37.4 56.2

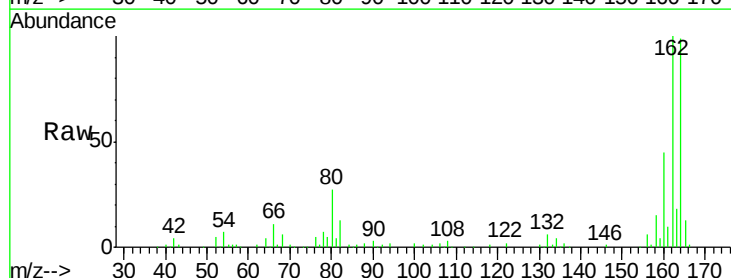

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

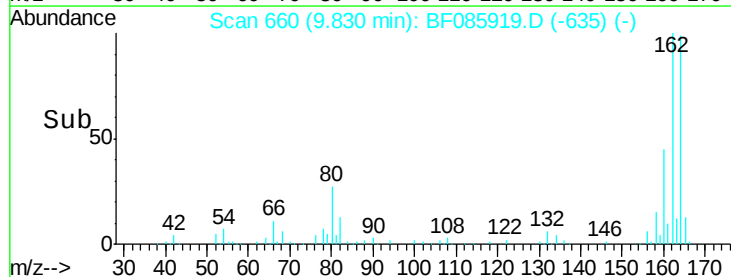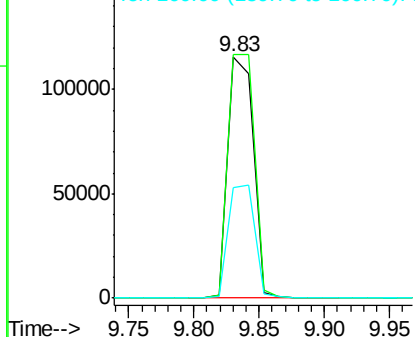


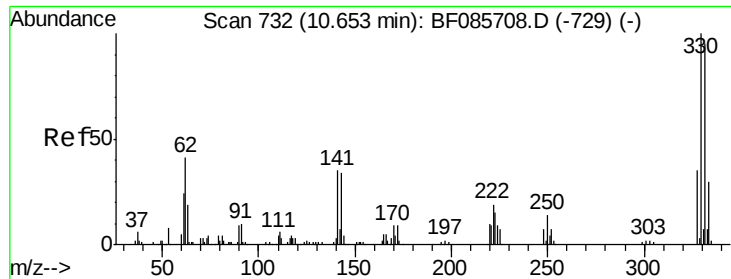




#41
 2,4,6-Tribromophenol
 Concen: 145.96 ng
 RT: 10.63 min Scan# 730
 Delta R.T. -0.00 min
 Lab File: BF085919.D
 Acq: 31 Mar 2016 8:38

Instrument :
 BNA_F
 ClientSampleId :
 AMBOY-SB28COMP0.5-15.0

Tgt Ion:330 Resp: 217977
 Ion Ratio Lower Upper
 330 100
 332 95.3 78.2 117.2
 141 33.2 31.5 47.3

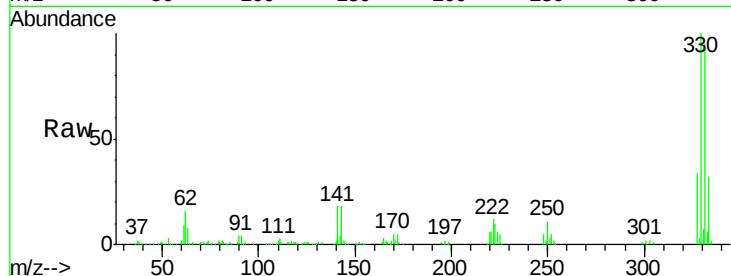


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

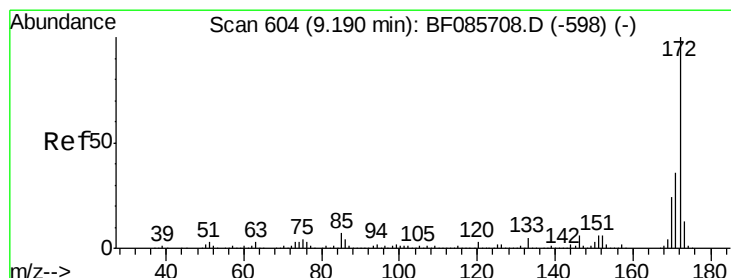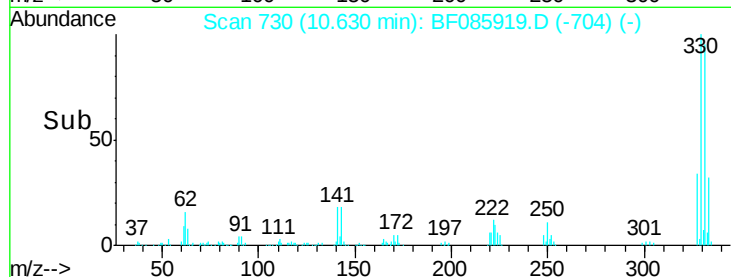
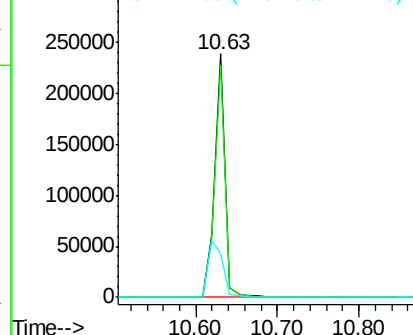



#44
 2-Fluorobiphenyl
 Concen: 106.58 ng
 RT: 9.17 min Scan# 602
 Delta R.T. -0.00 min
 Lab File: BF085919.D
 Acq: 31 Mar 2016 8:38

Tgt Ion:172 Resp: 1002658
 Ion Ratio Lower Upper
 172 100
 171 35.3 29.4 44.2
 170 23.9 19.8 29.6

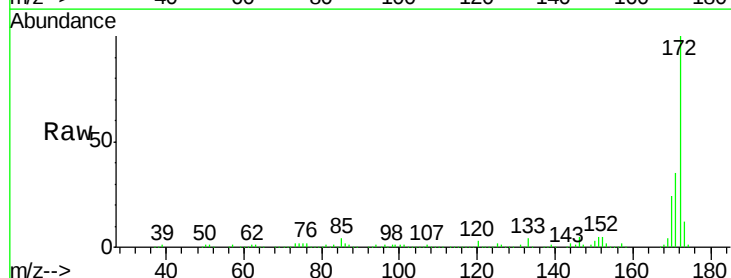

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

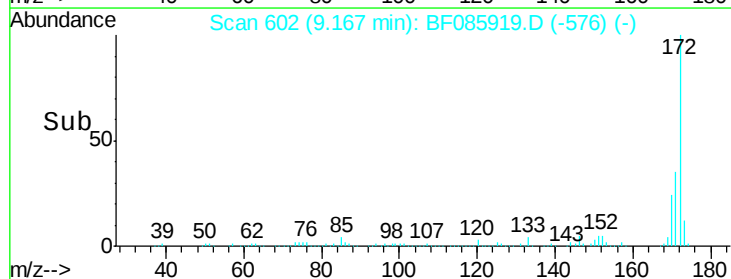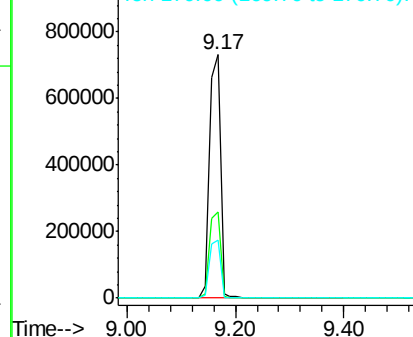

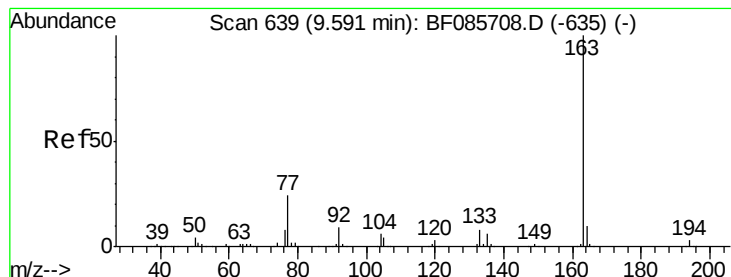

#49

Dimethylphthalate

Concen: 14.02 ng

RT: 9.56 min Scan# 636

Delta R.T. -0.01 min

Lab File: BF085919.D

Acq: 31 Mar 2016 8:38

Instrument :

BNA_F

ClientSampleId :

AMBOY-SB28COMP0.5-15.0


Tgt Ion:163 Resp: 167139

Ion Ratio Lower Upper

163 100

194 3.3 2.9 4.3




164 9.6 8.3 12.5

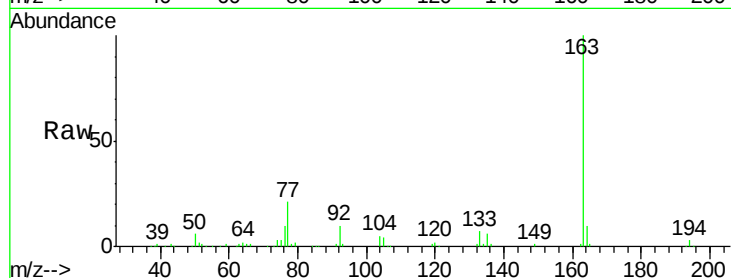

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

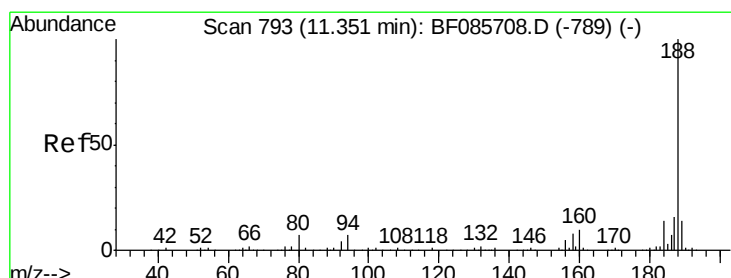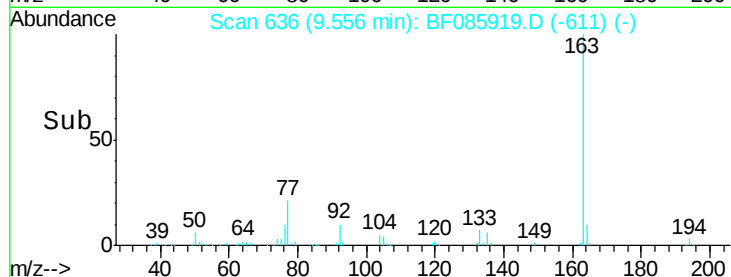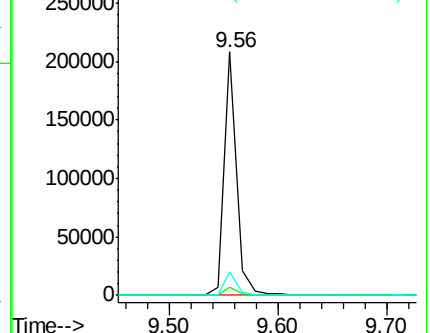

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.32 min Scan# 790

Delta R.T. -0.01 min

Lab File: BF085919.D

Acq: 31 Mar 2016 8:38


Tgt Ion:188 Resp: 268269

Ion Ratio Lower Upper

188 100

94 11.5 5.4 8.0#



80 11.9 5.5 8.3#

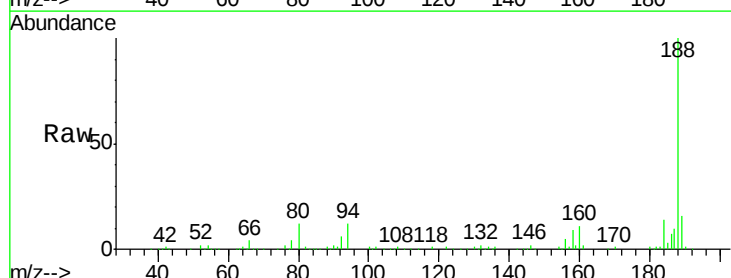


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

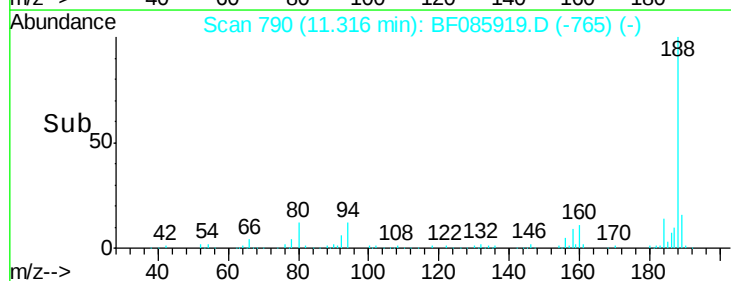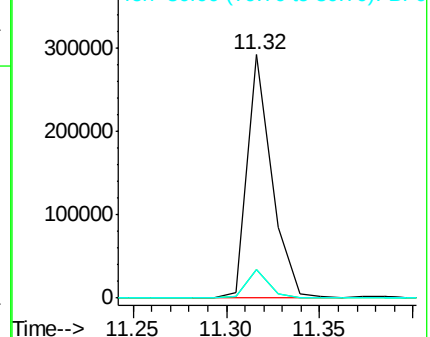

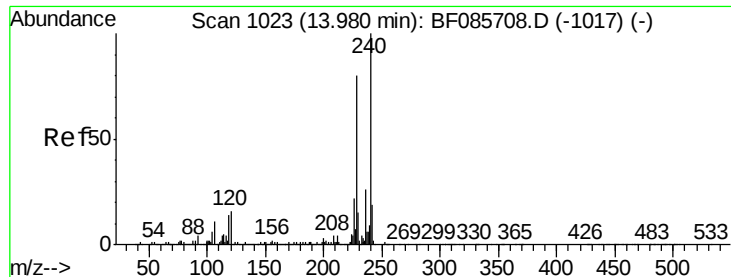

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.96 min Scan# 1021

Delta R.T. -0.01 min

Lab File: BF085919.D

Acq: 31 Mar 2016 8:38

Instrument :

BNA_F

ClientSampleId :

AMBOY-SB28COMP0.5-15.0


Tgt Ion:240 Resp: 195580

Ion Ratio Lower Upper

240 100

120 9.4 13.8 20.8#




236 26.1 20.6 30.8

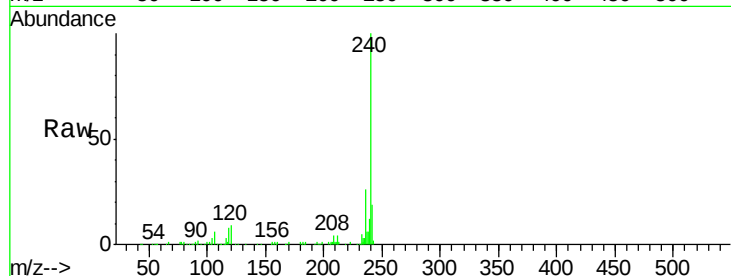

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

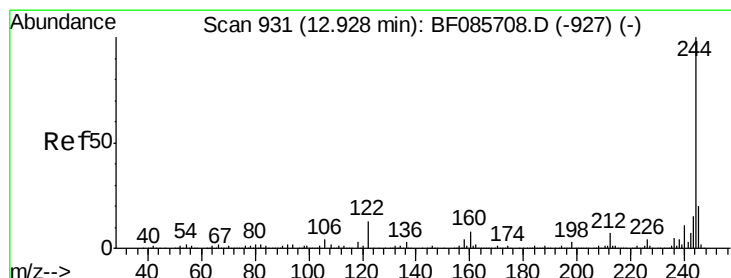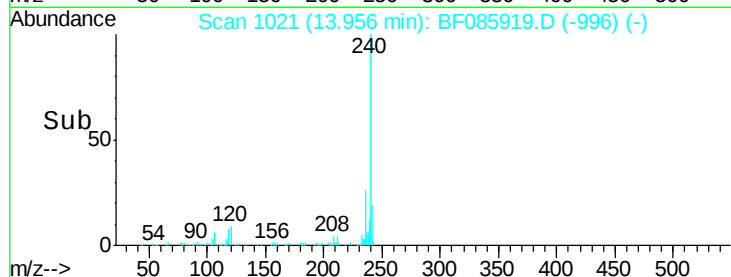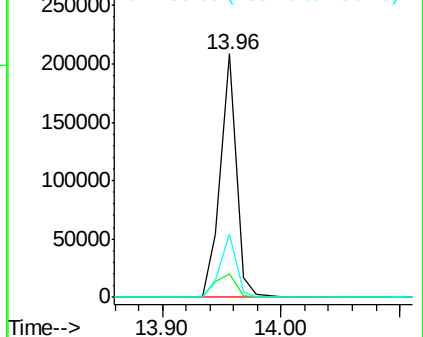

#78

Terphenyl-d14

Concen: 73.01 ng

RT: 12.90 min Scan# 929

Delta R.T. -0.00 min

Lab File: BF085919.D

Acq: 31 Mar 2016 8:38


Tgt Ion:244 Resp: 694294

Ion Ratio Lower Upper

244 100

212 7.3 6.1 9.1



122 10.8 10.2 15.4



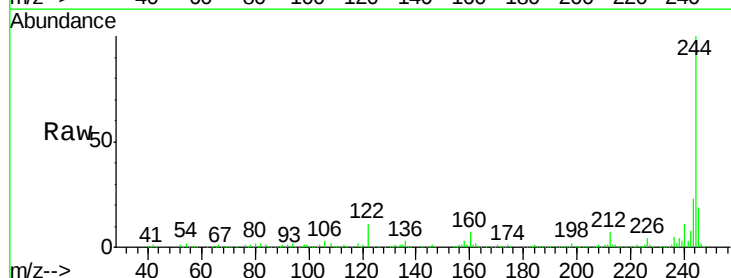


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

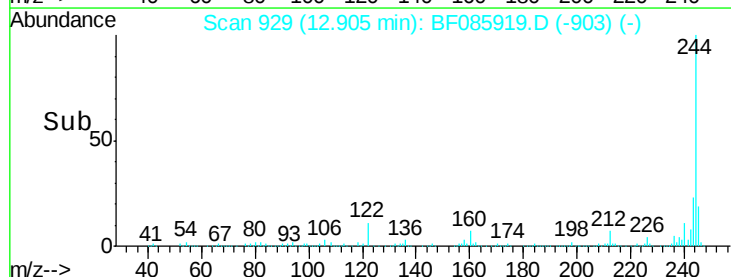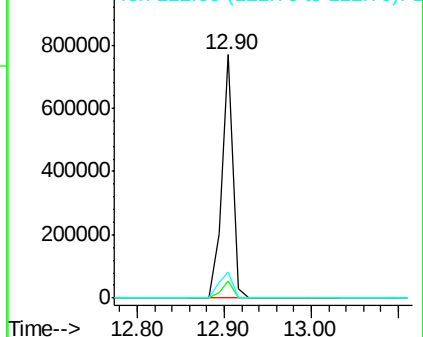

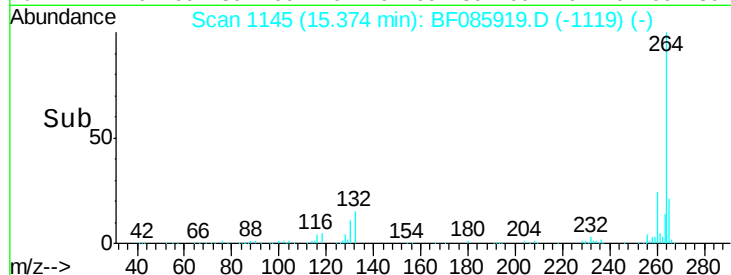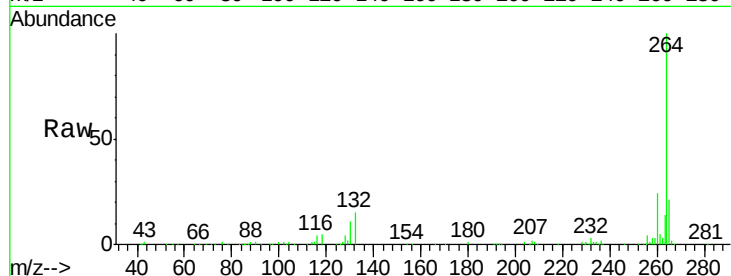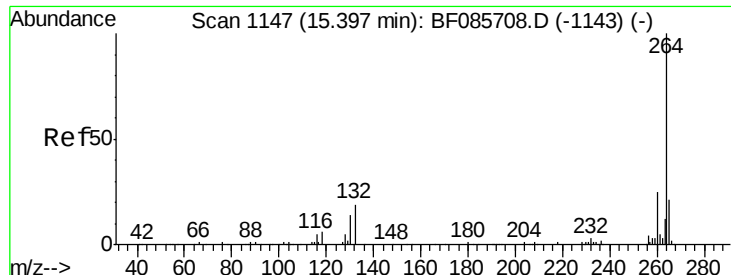

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.37 min Scan# 1145

Delta R.T. -0.00 min

Lab File: BF085919.D

Acq: 31 Mar 2016 8:38

Instrument :

BNA_F

ClientSampleId :

AMBOY-SB28COMP0.5-15.0

Tgt Ion:264 Resp: 193339

Ion Ratio Lower Upper

264 100

260 23.9 19.4 29.2

265 21.1 17.2 25.8

