

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
 Data File : BF085880.D
 Acq On : 30 Mar 2016 11:56
 Operator : UM/SJ
 Sample : H1739-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PT-BN-WP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.076	64	69	72	rBV	486695	1350901	17.90%	1.256%
2	5.396	269	272	275	rBV	2425029	2504094	33.18%	2.329%
3	6.447	360	364	366	rBV	2335502	2902991	38.47%	2.700%
4	6.539	369	372	373	rVV	1798489	1815155	24.05%	1.688%
5	6.573	373	375	377	rVB	2369829	2921194	38.71%	2.717%
6	6.745	387	390	392	rBV	3649235	3929402	52.07%	3.655%
7	6.802	392	395	397	rVV	584408	637073	8.44%	0.593%
8	6.950	406	408	411	rVB	2057076	2160996	28.63%	2.010%
9	7.305	437	439	442	rBV	1780137	2386513	31.62%	2.220%
10	7.373	442	445	449	rBV2	1603369	3584981	47.50%	3.334%
11	7.625	464	467	470	rBV	2616157	4011815	53.16%	3.731%
12	8.025	500	502	505	rBV	1364303	1356577	17.97%	1.262%
13	8.105	505	509	512	rVB	1235128	1911425	25.33%	1.778%
14	8.802	567	570	572	rBV	2752392	2761913	36.60%	2.569%
15	9.168	599	602	604	rBV	3309167	3595094	47.64%	3.344%
16	9.293	610	613	615	rBV	4139447	4767621	63.17%	4.434%
17	9.568	633	637	640	rBV	2767977	4598844	60.94%	4.277%
18	9.648	640	644	646	rVB	2293574	3072031	40.70%	2.857%
19	9.842	658	661	662	rBV	973743	1010608	13.39%	0.940%
20	9.876	662	664	667	rVB	3721079	4088046	54.17%	3.802%
21	10.036	676	678	681	rBV	1224859	1098309	14.55%	1.022%
22	10.265	695	698	700	rBV	2451783	2679840	35.51%	2.492%
23	10.391	706	709	712	rVB2	4659293	6797125	90.06%	6.322%
24	10.631	727	730	732	rBV	2077734	1989280	26.36%	1.850%
25	10.871	748	751	753	rVB	641404	657612	8.71%	0.612%
26	10.939	754	757	759	rBV	1660245	1537912	20.38%	1.430%
27	11.362	788	794	795	rBV2	4642608	7547062	100.00%	7.019%
28	11.396	795	797	800	rVB	1412566	1672248	22.16%	1.555%
29	11.888	837	840	843	rVB	2917214	2839890	37.63%	2.641%
30	12.151	861	863	865	rBV	174192	182944	2.42%	0.170%
31	12.539	894	897	899	rBV	3441437	3419677	45.31%	3.181%
32	12.905	926	929	932	rBV	3196231	3211111	42.55%	2.987%
33	13.385	968	971	973	rBV	2427105	2491319	33.01%	2.317%
34	13.945	1017	1020	1023	rBV2	4483964	5450307	72.22%	5.069%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
Data File : BF085880.D
Acq On : 30 Mar 2016 11:56
Operator : UM/SJ
Sample : H1739-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PT-BN-WP

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	14.551	1070	1073	1076	rBV	3392733	4401223	58.32%	4.094%
36	14.985	1107	1111	1113	rBV	3176597	4256902	56.40%	3.959%
37	15.374	1142	1145	1150	rBV	524809	661328	8.76%	0.615%
38	16.746	1261	1265	1269	rBV	607305	1255752	16.64%	1.168%


Sum of corrected areas: 107517115

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
Data File : BF085880.D
Acq On : 30 Mar 2016 11:56
Operator : UM/SJ
Sample : H1739-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PT-BN-WP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

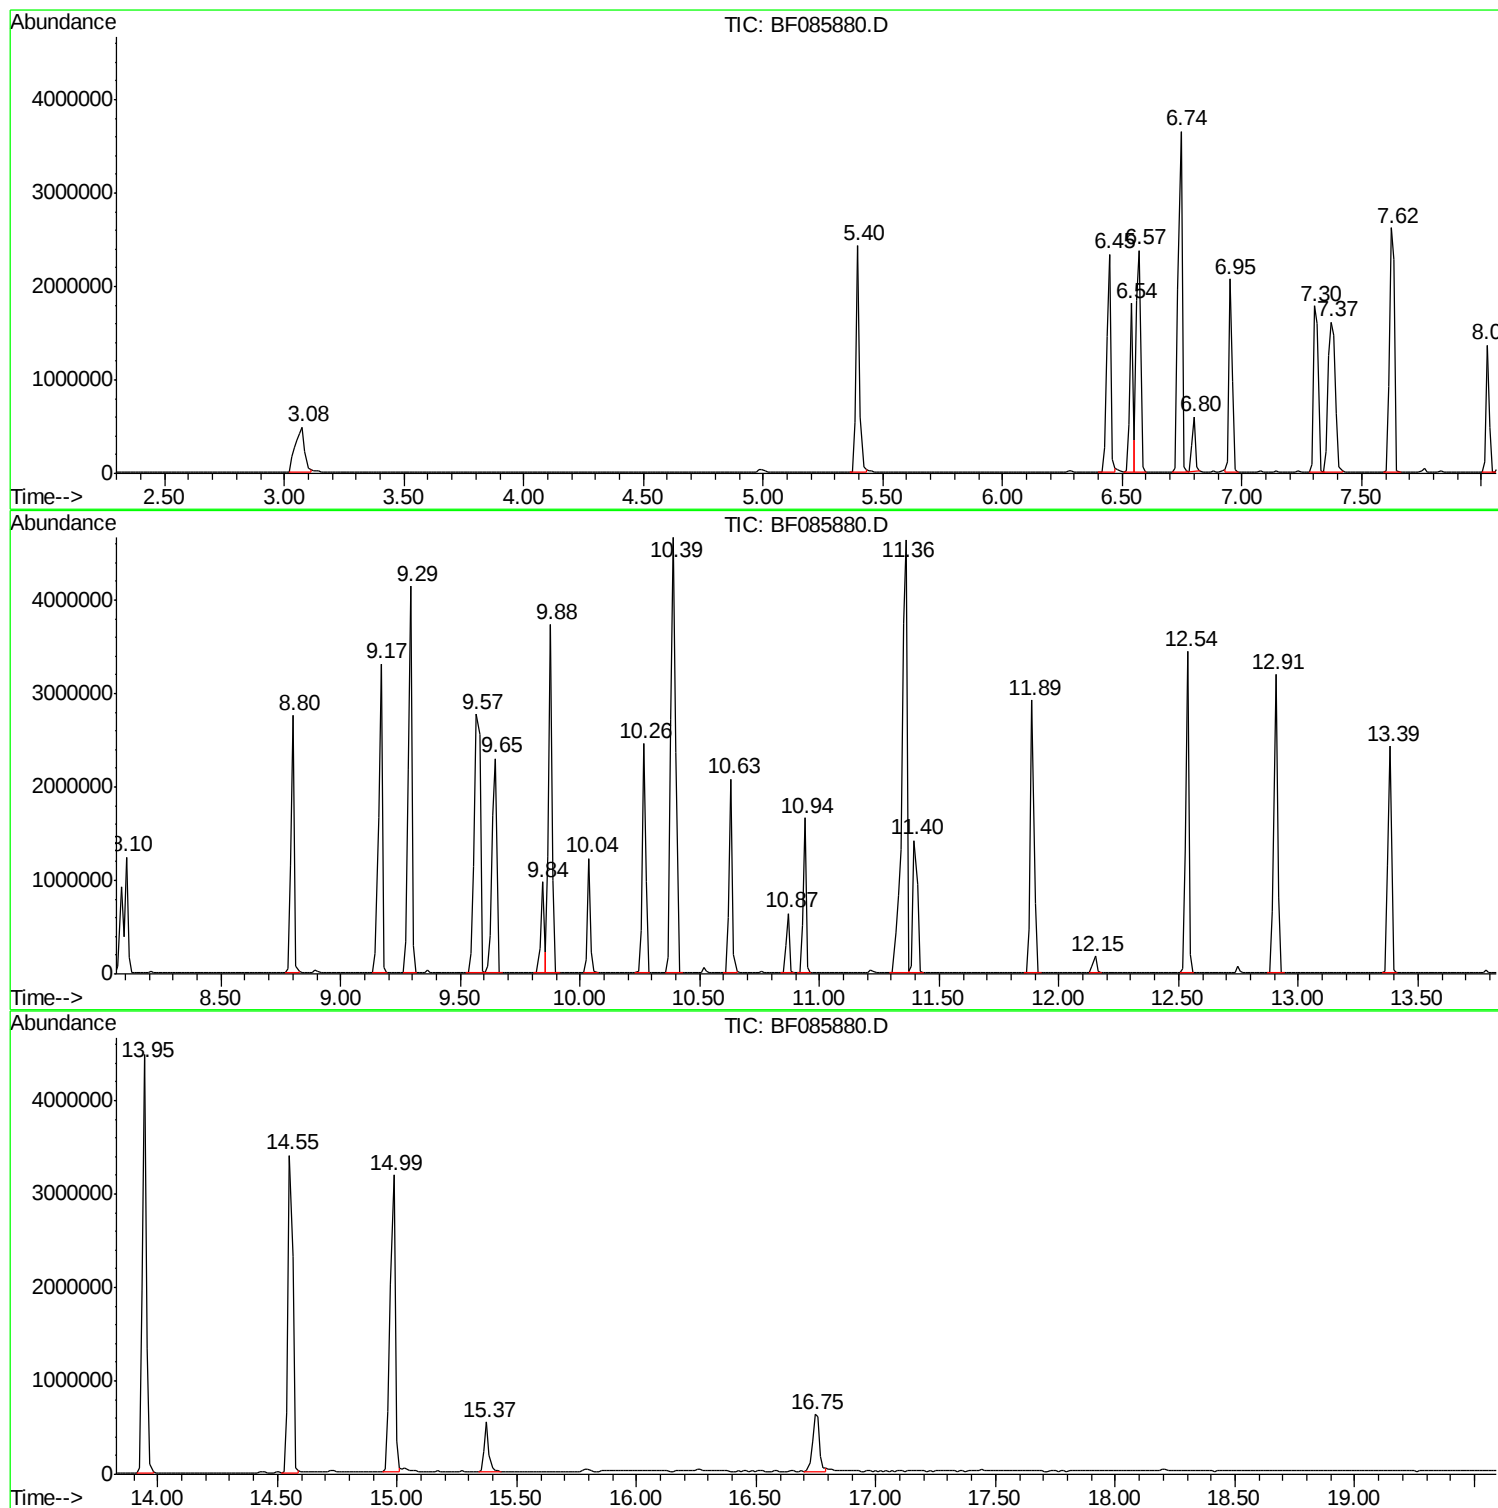

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
Data File : BF085880.D
Acq On : 30 Mar 2016 11:56
Operator : UM/SJ
Sample : H1739-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PT-BN-WP










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.95 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.95	67.84 ng	2161000	1,4-Dichlorobenzene-d4	6.80

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,4-Dichlorobenzene-D4	150	C6D4Cl2	003855-82-1	94
2			1,2-Dichlorobenzene-D4	150	C6D4Cl2	002199-69-1	94
3			9-Borabicyclo[3.3.1]nonane, 9-et...	150	C10H19B	052102-17-7	38
4			2-Chloro-4,6-difluoro-pyrimidine	150	C4HClF2N2	038953-30-9	38
5			2-Bromo-2'-nitroacetophenone	243	C8H6BrNO3	006851-99-6	12

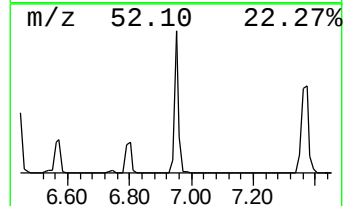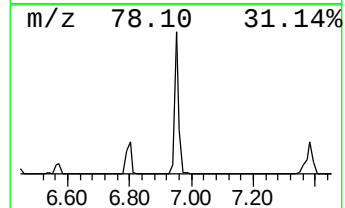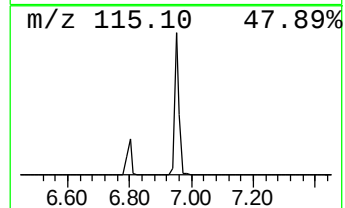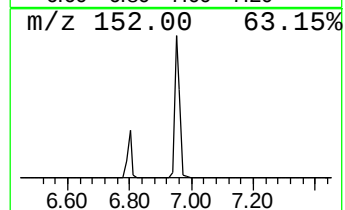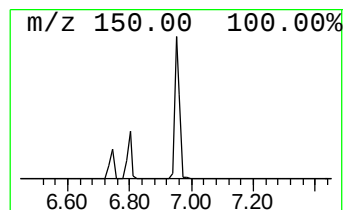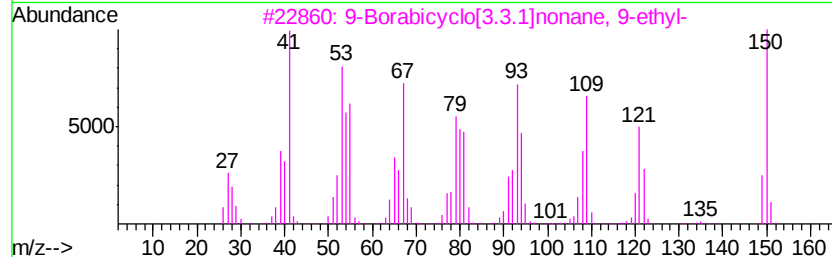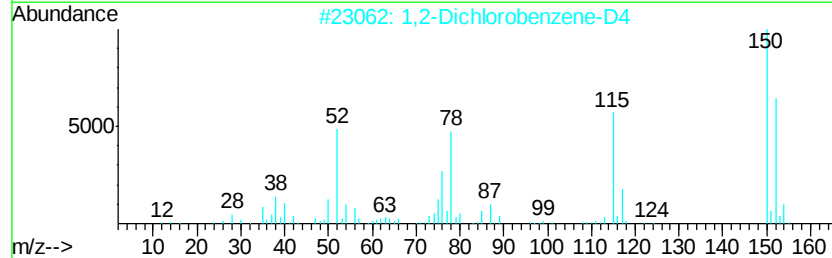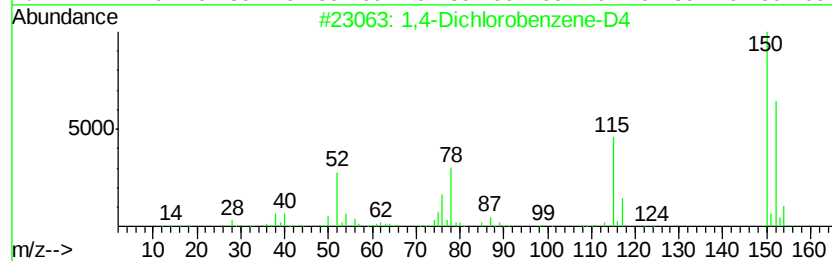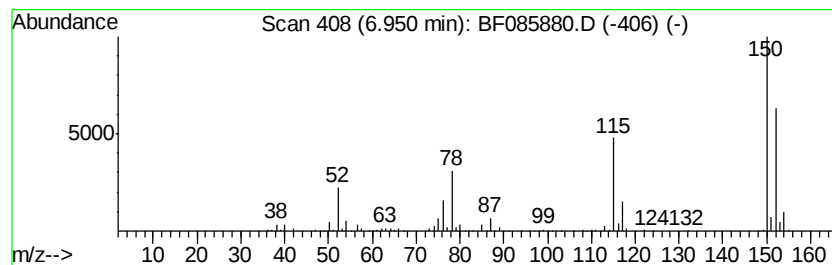

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
Data File : BF085880.D
Acq On : 30 Mar 2016 11:56
Operator : UM/SJ
Sample : H1739-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PT-BN-WP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.95	6.95	67.8	ng	2161000	1	6.80	637073	20.0