

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
 Data File : BF085914.D
 Acq On : 31 Mar 2016 6:17
 Operator : UM/SJ
 Sample : H2012-03
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 032416-P2EB-F-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.950	231	233	244	rBV	252724	355857	13.04%	2.114%
2	5.384	269	271	295	rVB	673122	862242	31.61%	5.121%
3	6.424	361	362	372	rBV	360809	548984	20.12%	3.261%
4	6.561	372	374	376	rBV	1688663	1446834	53.03%	8.593%
5	6.790	392	394	397	rBV	500620	653609	23.96%	3.882%
6	6.950	406	408	411	rBV	2124255	1889676	69.27%	11.224%
7	7.361	442	444	447	rBV	1461511	1446517	53.02%	8.592%
8	8.081	505	507	510	rBV	1042217	886250	32.49%	5.264%
9	9.156	599	601	604	rBV	2081227	2728086	100.00%	16.203%
10	9.556	634	636	638	rBV	114316	93015	3.41%	0.552%
11	9.842	658	661	663	rBV	628453	864704	31.70%	5.136%
12	10.265	694	698	700	rVB2	30888	47157	1.73%	0.280%
13	10.619	727	729	732	rBV2	683090	895516	32.83%	5.319%
14	10.745	737	740	746	rVB	48324	64321	2.36%	0.382%
15	11.316	788	790	793	rBV	818630	776416	28.46%	4.612%
16	12.905	926	929	931	rBV	2324194	2075404	76.08%	12.327%
17	13.956	1018	1021	1023	rBV	637680	604125	22.14%	3.588%
18	15.374	1142	1145	1150	rBV	454164	597775	21.91%	3.550%


Sum of corrected areas: 16836488

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
Data File : BF085914.D
Acq On : 31 Mar 2016 6:17
Operator : UM/SJ
Sample : H2012-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
032416-P2EB-F-U-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

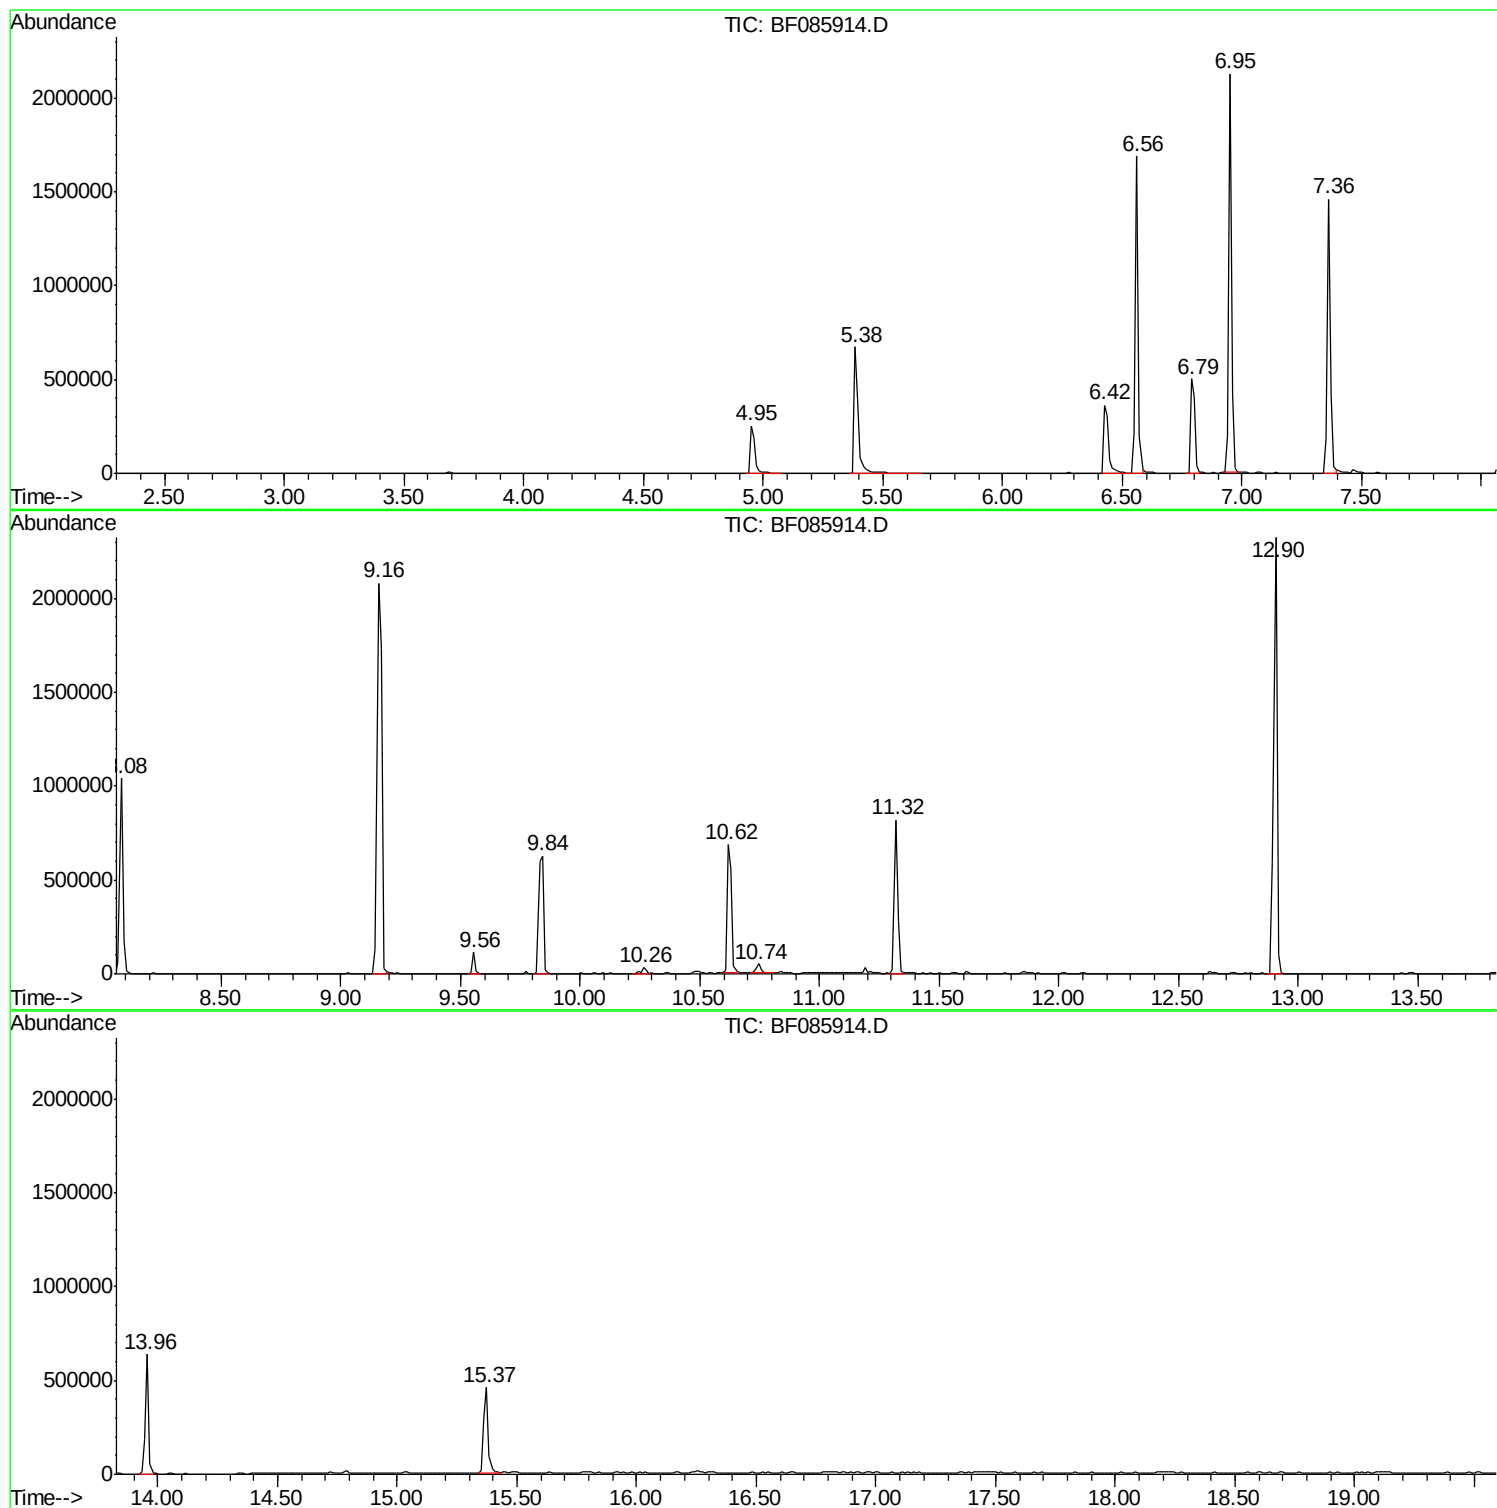

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
Data File : BF085914.D
Acq On : 31 Mar 2016 6:17
Operator : UM/SJ
Sample : H2012-03
Misc :
ALS Vial : 35 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
032416-P2EB-F-U-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.		
4.95	10.89 ng	355857	1,4-Dichlorobenzene-d4	6.80		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64	
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23	
3	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9	
4	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9	
5	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9	

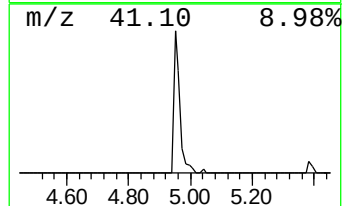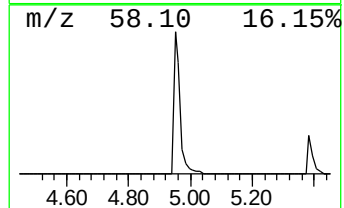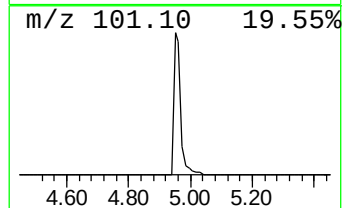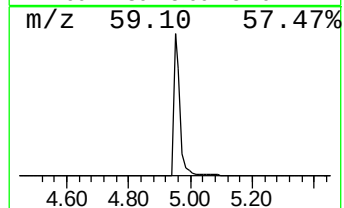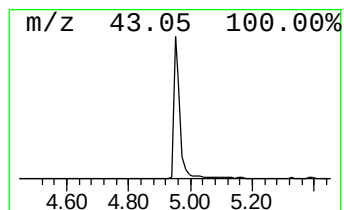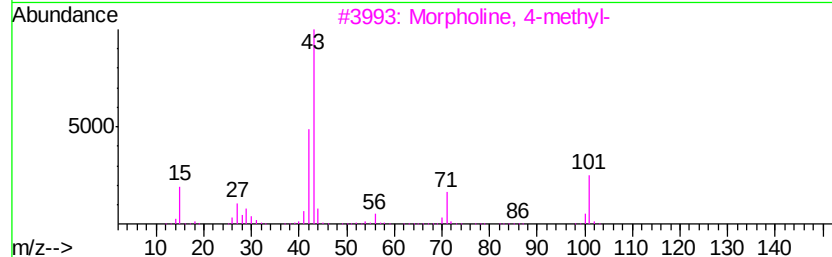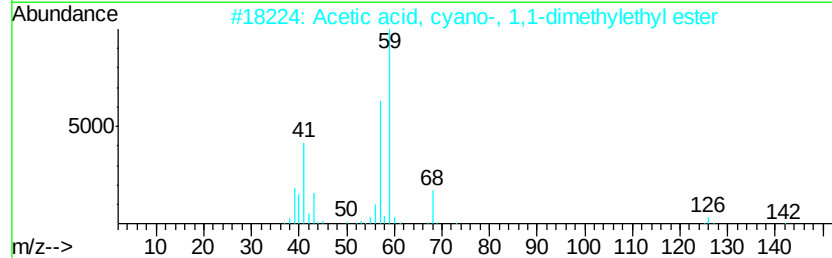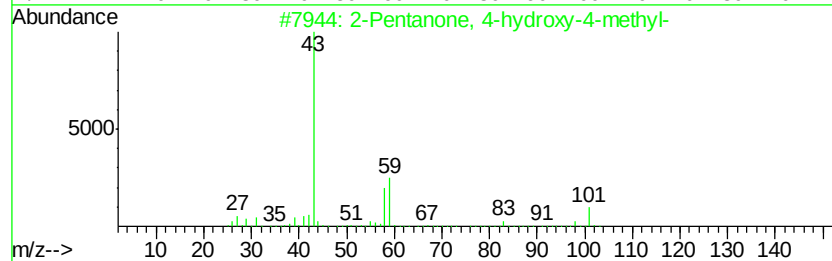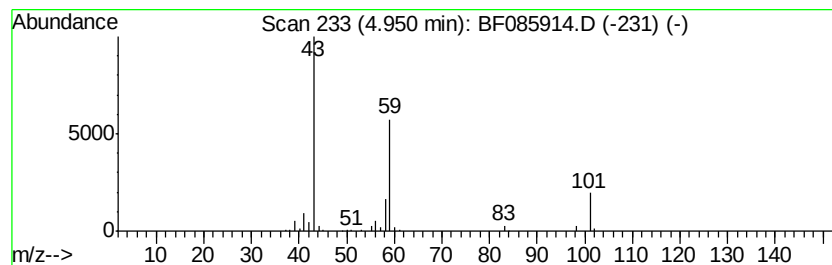

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033016\
Data File : BF085914.D
Acq On : 31 Mar 2016 6:17
Operator : UM/SJ
Sample : H2012-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
032416-P2EB-F-U-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.95	10.9	ng	355857	1	6.80	653609	20.0