


Data Path : Z:\HPCHEM1\BNA F\DATA\BF033016\
 Data File : BF085877.D
 Acq On : 30 Mar 2016 10:29
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 30 12:31:18 2016

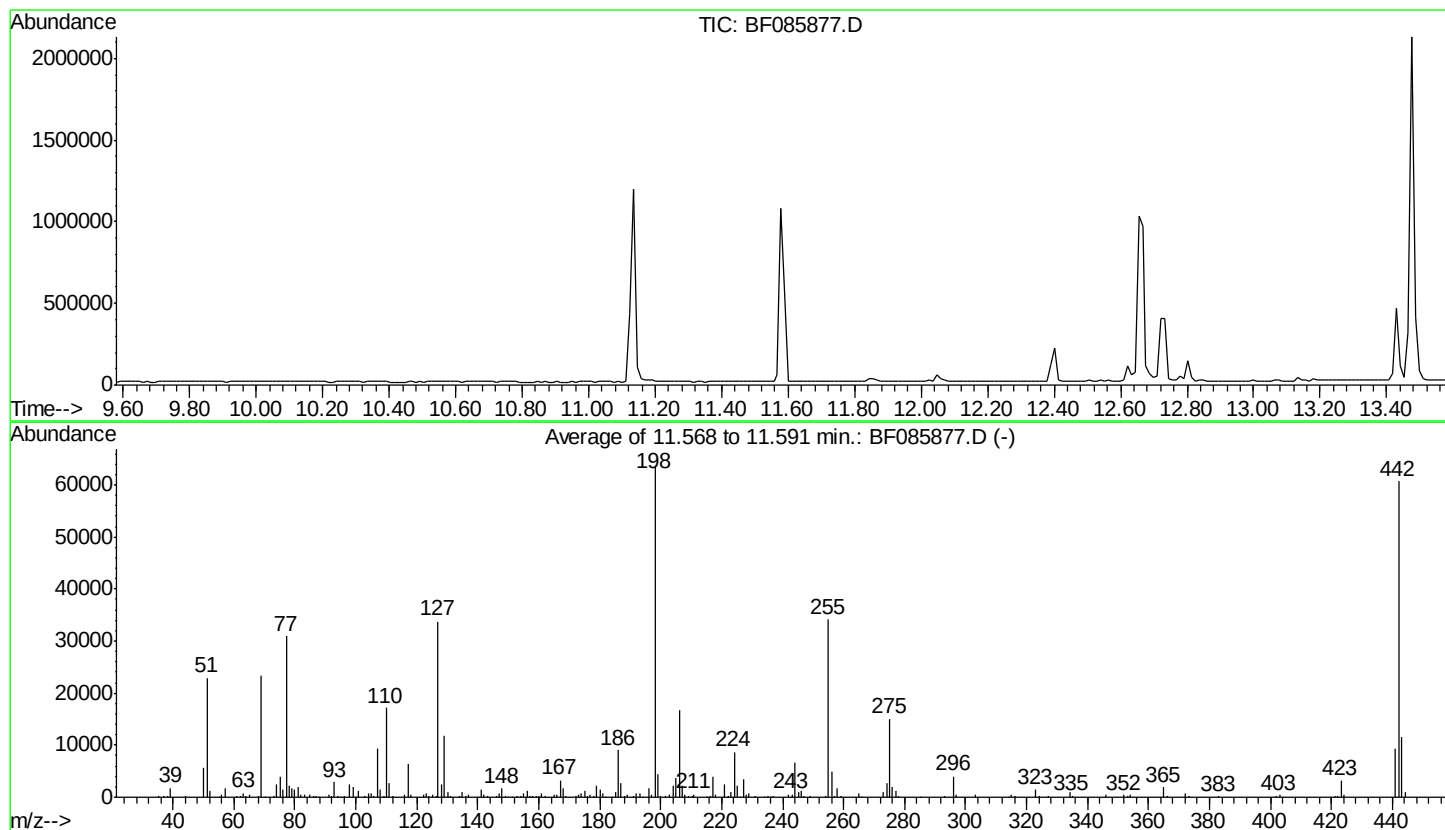

AutoFind: Scans 812, 813, 814; Background Corrected with Scan 809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	22885	PASS
68	69	0.00	2	1.4	336	PASS
69	198	0.00	100	36.6	23334	PASS
70	69	0.00	2	0.5	116	PASS
127	198	10	80	53.0	33768	PASS
197	198	0.00	2	0.8	500	PASS
198	198	100	100	100.0	63694	PASS
199	198	5	9	6.8	4321	PASS
275	198	10	60	23.7	15089	PASS
365	198	1	100	3.0	1934	PASS
441	442	0.01	24	15.5	9426	PASS
442	198	50	100	95.2	60658	PASS
443	442	15	24	19.2	11656	PASS