


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF033016\  
 Data File : BF085877.D  
 Acq On : 30 Mar 2016 10:29  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF032416.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Mar 30 12:31:18 2016

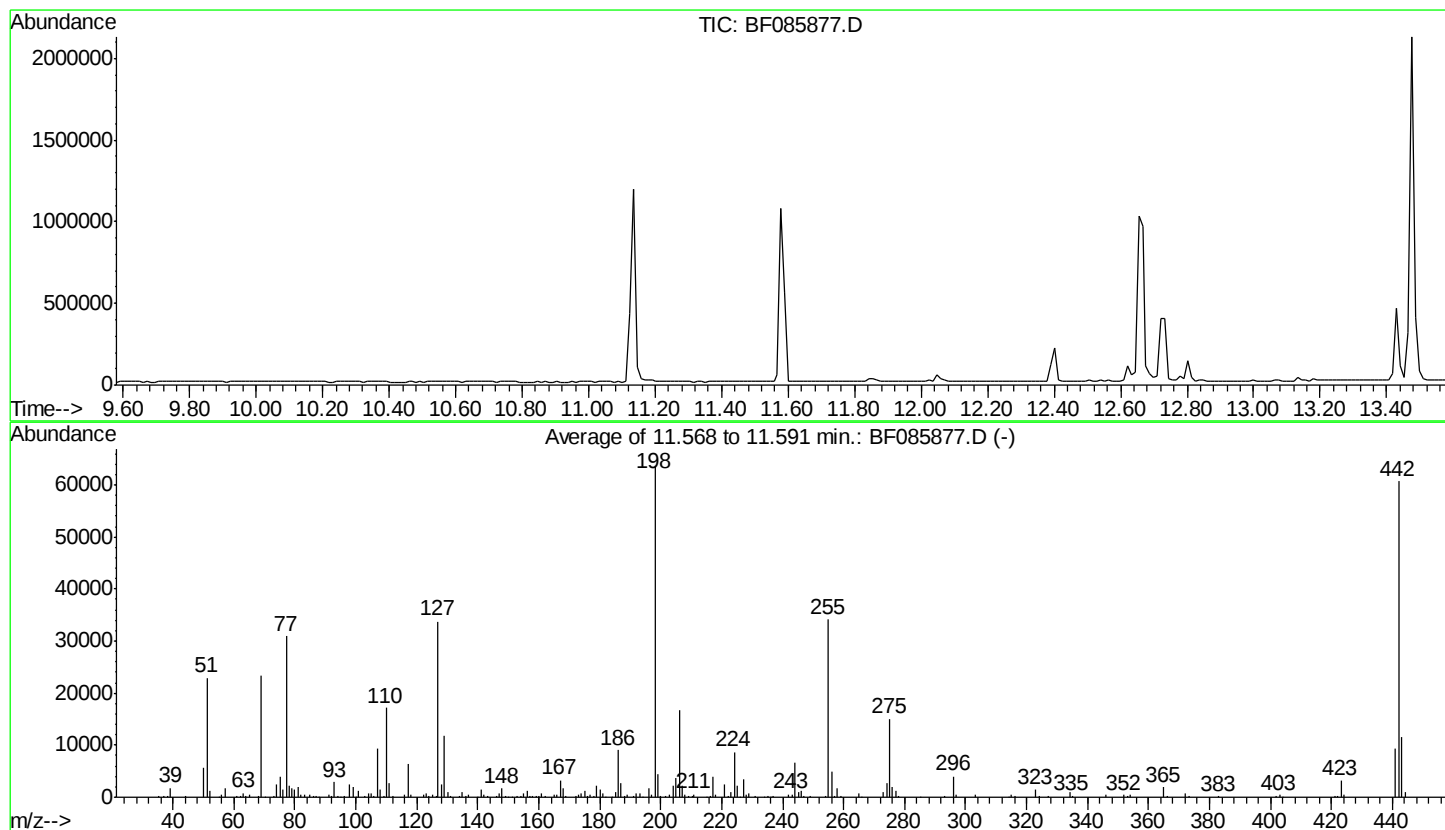

AutoFind: Scans 812, 813, 814; Background Corrected with Scan 809

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 35.9         | 22885      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.4          | 336        | PASS                |
| 69             | 198             | 0.00            | 100             | 36.6         | 23334      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 116        | PASS                |
| 127            | 198             | 10              | 80              | 53.0         | 33768      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.8          | 500        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 63694      | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 4321       | PASS                |
| 275            | 198             | 10              | 60              | 23.7         | 15089      | PASS                |
| 365            | 198             | 1               | 100             | 3.0          | 1934       | PASS                |
| 441            | 442             | 0.01            | 24              | 15.5         | 9426       | PASS                |
| 442            | 198             | 50              | 100             | 95.2         | 60658      | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 11656      | PASS                |