


Data Path : Z:\HPCHEM1\BNA_F\Data\BF033016\
 Data File : BF085902.D
 Acq On : 31 Mar 2016 00:40
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 30 12:31:18 2016

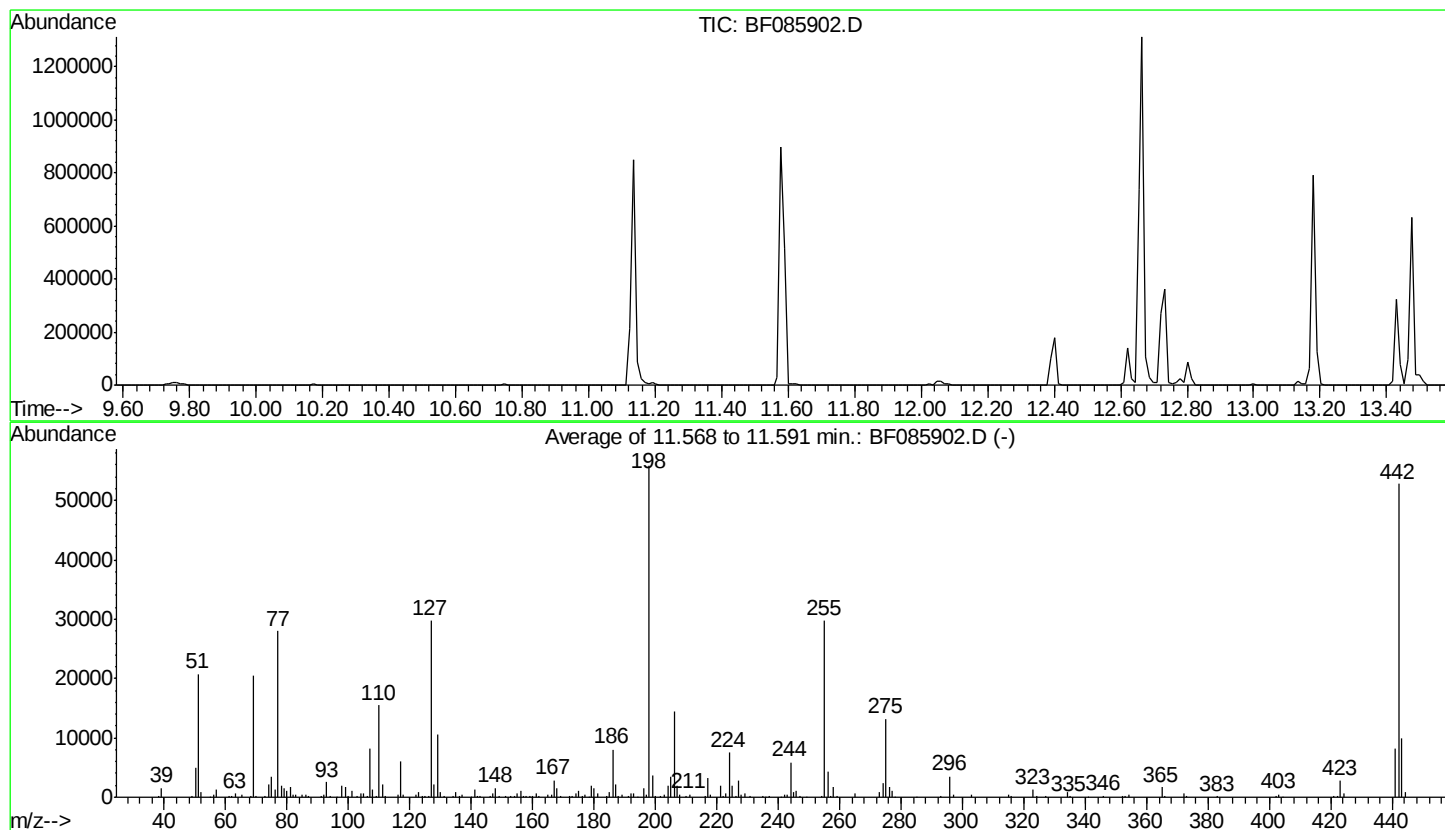

AutoFind: Scans 812, 813, 814; Background Corrected with Scan 809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	20825	PASS
68	69	0.00	2	1.4	294	PASS
69	198	0.00	100	36.8	20588	PASS
70	69	0.00	2	0.6	125	PASS
127	198	10	80	53.1	29681	PASS
197	198	0.00	2	0.8	423	PASS
198	198	100	100	100.0	55893	PASS
199	198	5	9	6.6	3692	PASS
275	198	10	60	23.7	13264	PASS
365	198	1	100	3.0	1684	PASS
441	442	0.01	24	15.4	8135	PASS
442	198	50	100	94.5	52800	PASS
443	442	15	24	18.8	9911	PASS