
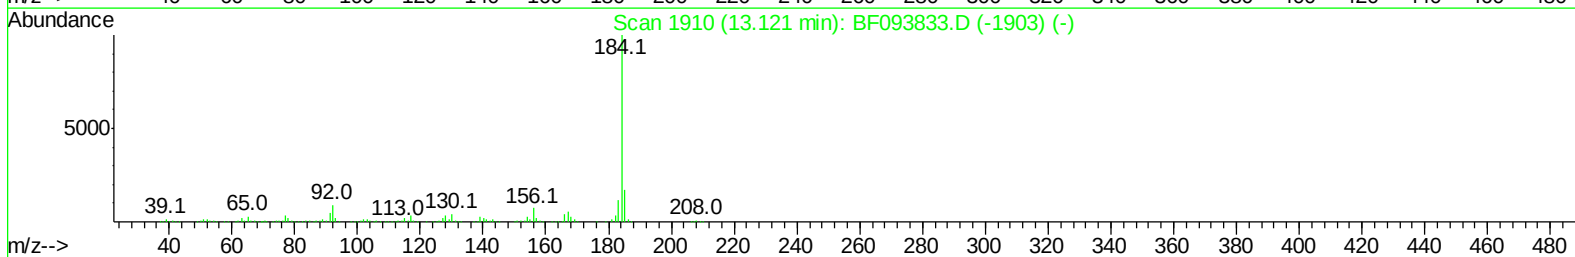
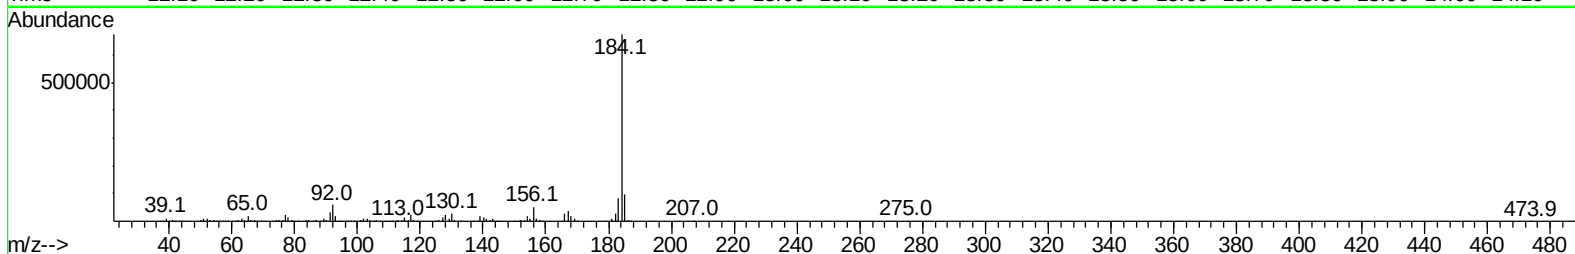


Data Path : Z:\HPCHEM1\BNA F\DATA\BF033017\
Data File : BF094061.D
Acq On : 30 Mar 2017 16:34
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 06:38:57 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 27 16:10:49 2017
Response via : Initial Calibration

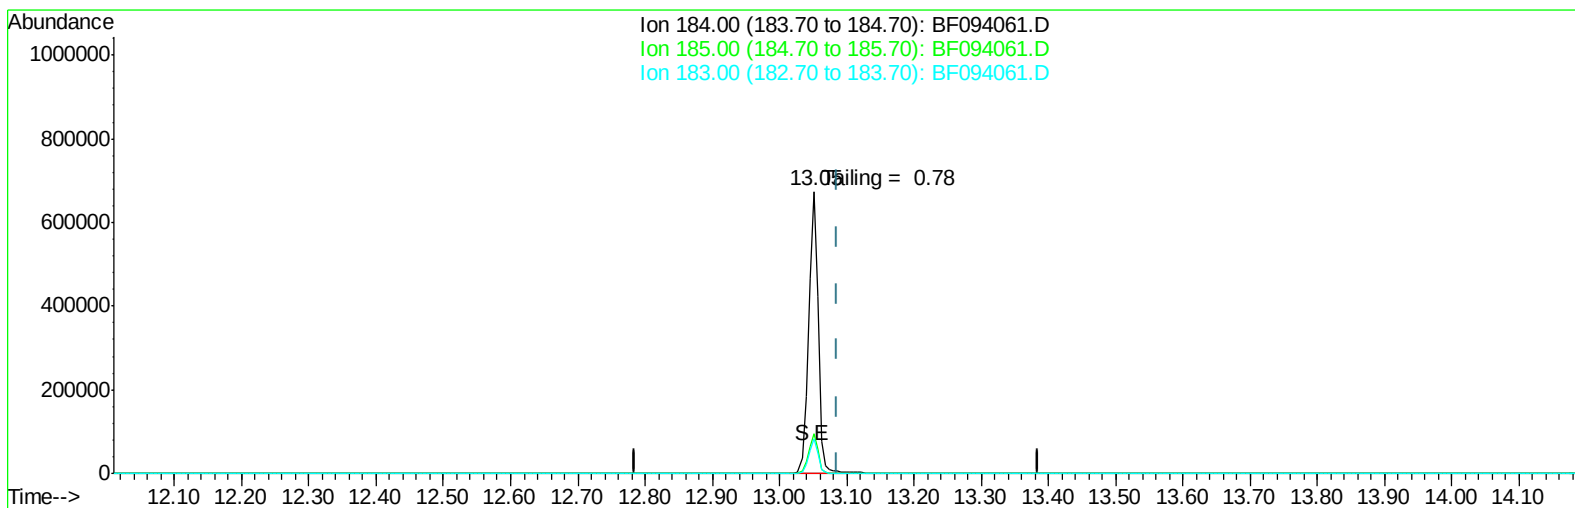

TIC: BF094061.D

(76) Benzidine




13.051min (-0.035) 123823.36ng

response 681199

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.33#
183.00	12.20	12.21
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF033017\
Data File : BF094061.D
Acq On : 30 Mar 2017 16:34
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 06:38:57 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 27 16:10:49 2017
Response via : Initial Calibration

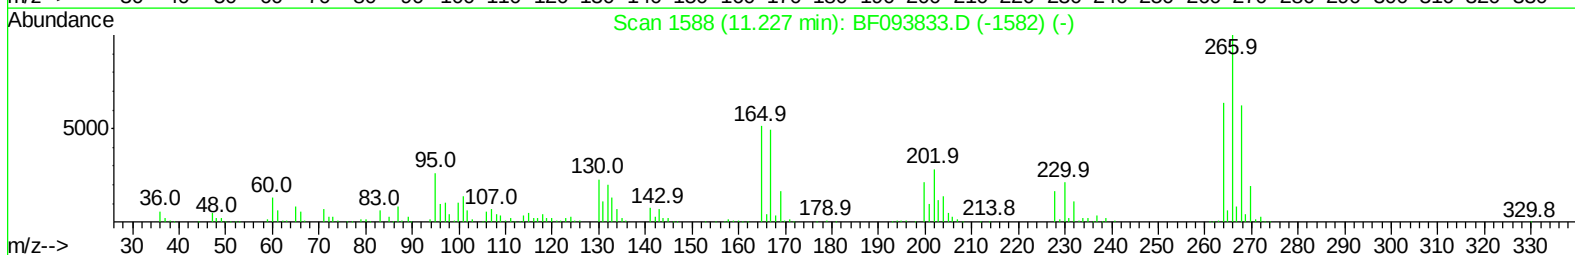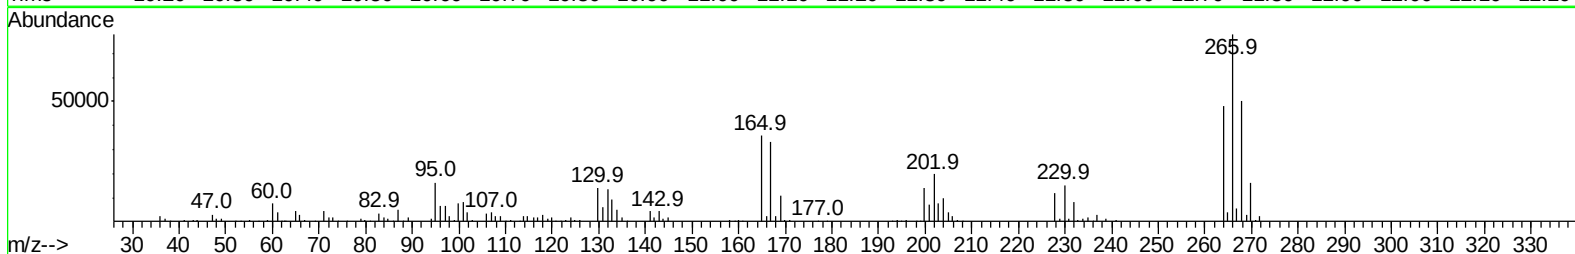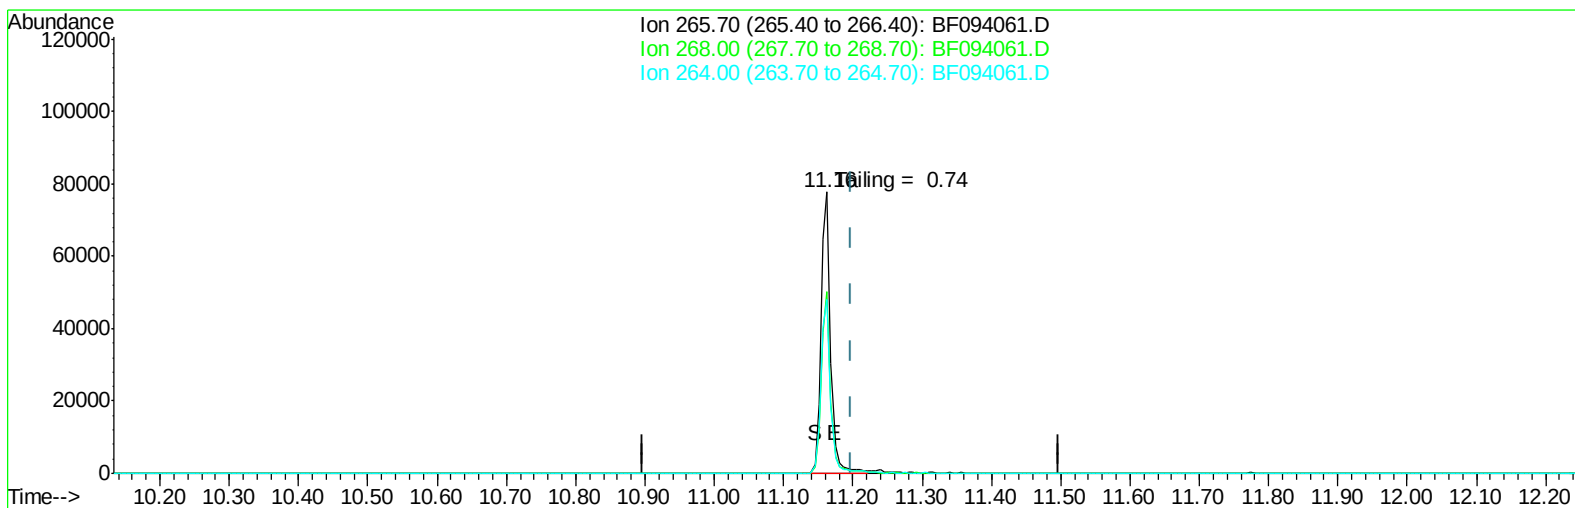

TIC: BF094061.D

(69) Pentachlorophenol (C)

11.163min (-0.035) 0.00ng

response 74940

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.36
264.00	64.60	61.64
0.00	0.00	0.00