


Data Path : Z:\HPCHEM1\BNA_F\Data\BF033017\
 Data File : BF094061.D
 Acq On : 30 Mar 2017 16:34
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 27 16:10:49 2017

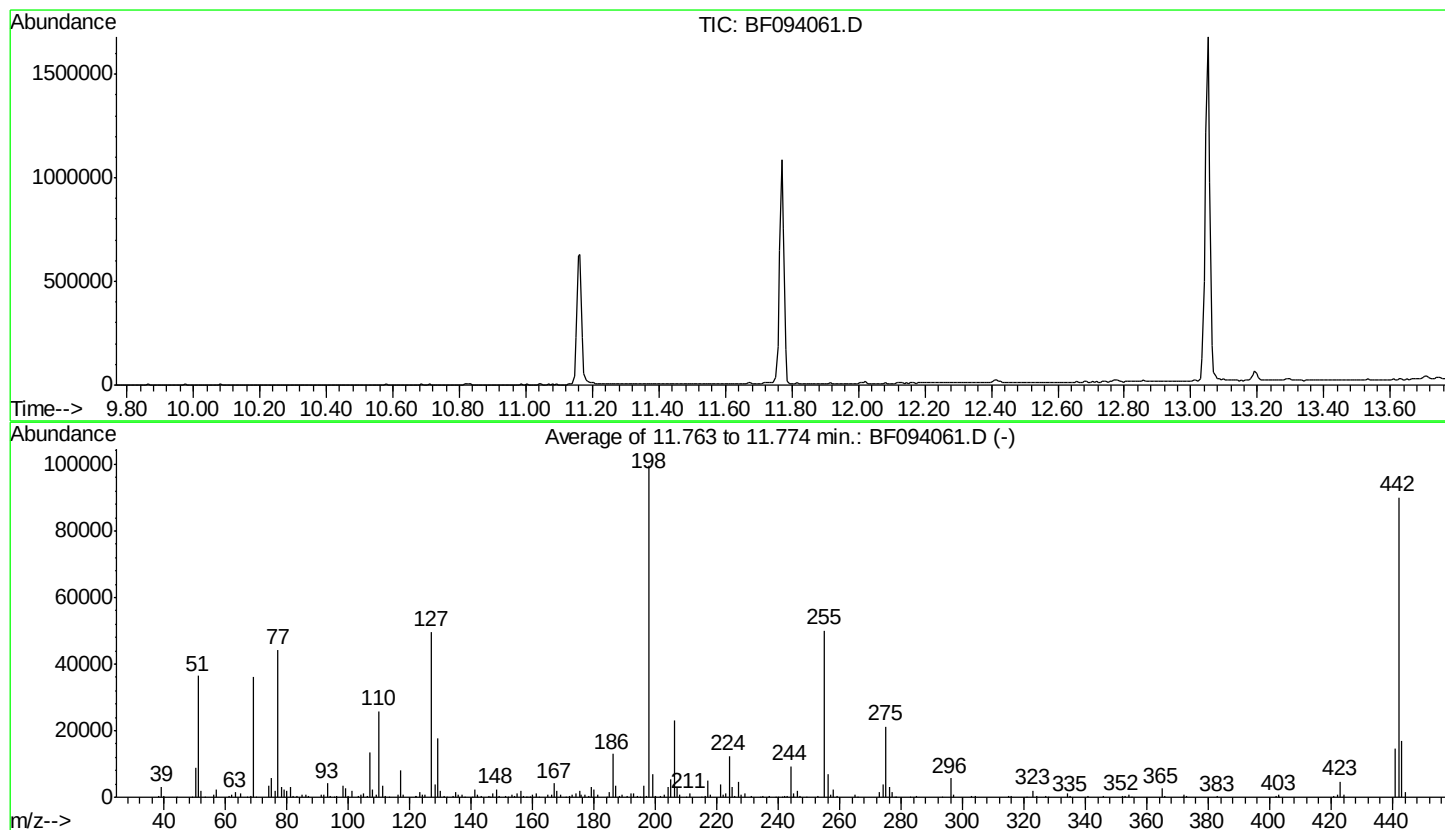

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	36458	PASS
68	69	0.00	2	1.0	364	PASS
69	198	0.00	100	36.4	36260	PASS
70	69	0.00	2	0.3	111	PASS
127	198	10	80	49.9	49674	PASS
197	198	0.00	2	0.4	440	PASS
198	198	100	100	100.0	99578	PASS
199	198	5	9	6.8	6747	PASS
275	198	10	60	21.3	21194	PASS
365	198	1	100	2.5	2514	PASS
441	442	0.01	24	16.2	14575	PASS
442	198	50	100	90.5	90088	PASS
443	442	15	24	18.7	16840	PASS