
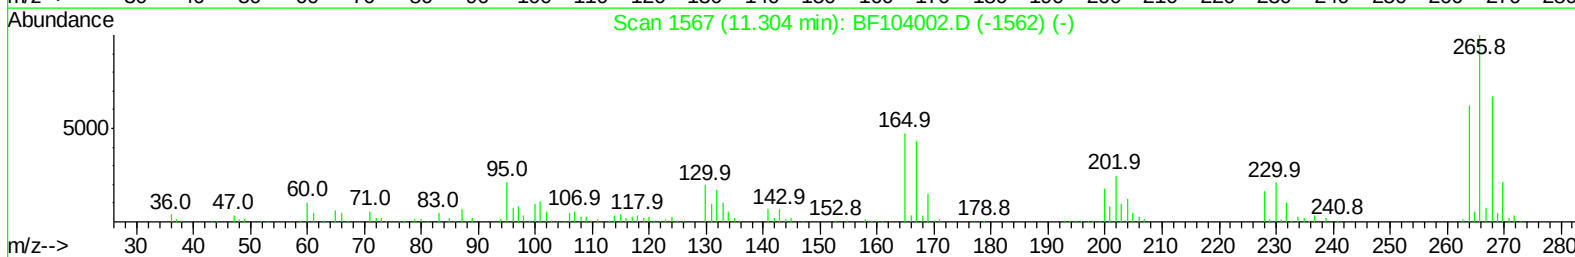
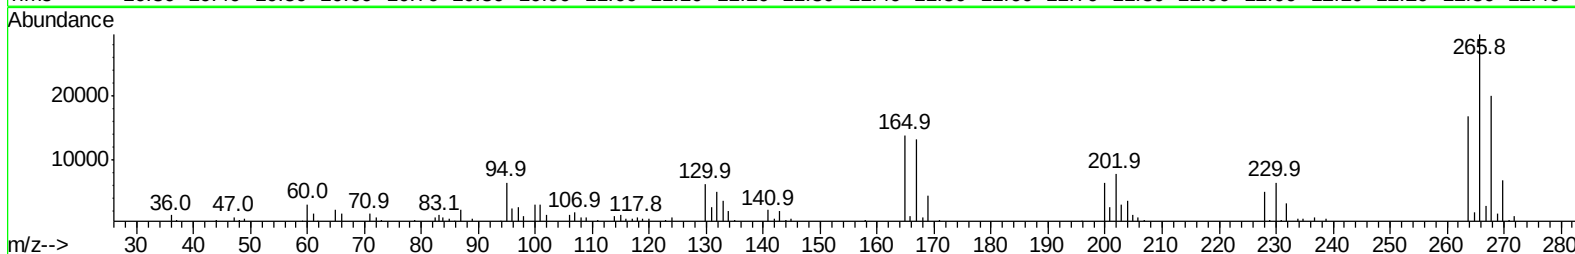


Data Path : U:\HPCHEM1\BNA F\DATA\BF033018\
Data File : BF104092.D
Acq On : 30 Mar 2018 14:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 01:15:23 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 30 17:20:53 2018
Response via : Initial Calibration

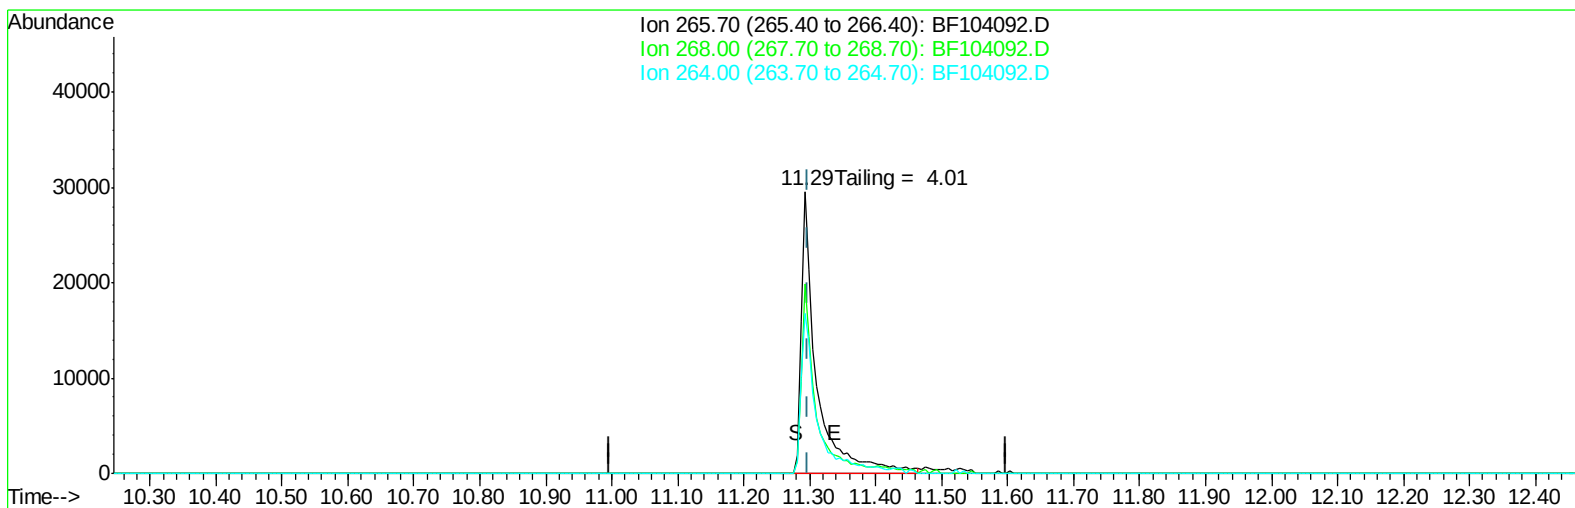

TIC: BF104092.D

(69) Pentachlorophenol (C)




11.292min (-0.006) 25005.37ng

response 48092

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.21
264.00	61.90	56.92
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF033018\
Data File : BF104092.D
Acq On : 30 Mar 2018 14:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 01:15:23 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 30 17:20:53 2018
Response via : Initial Calibration

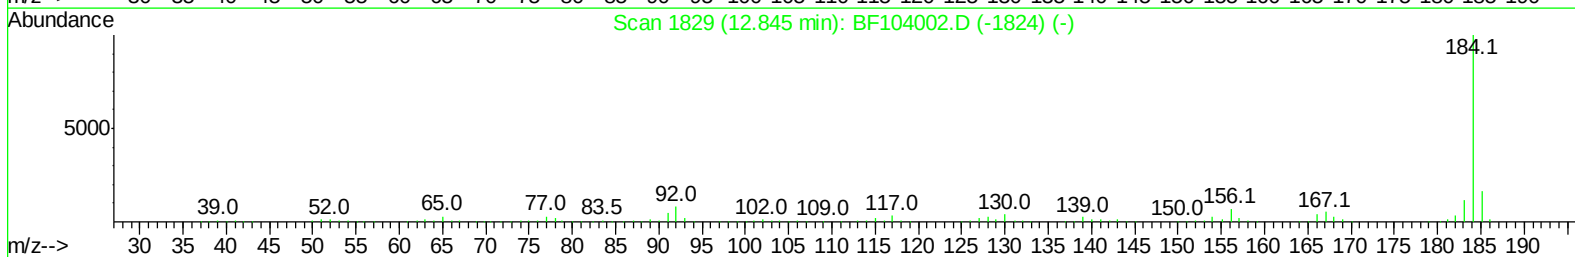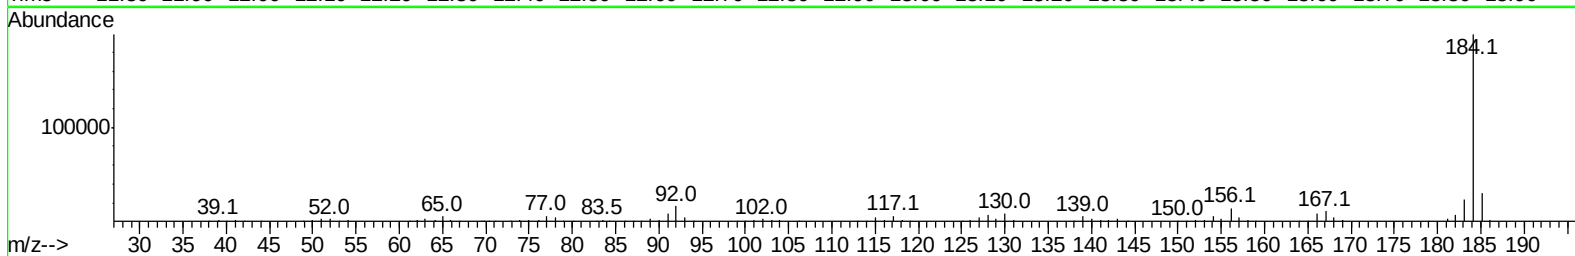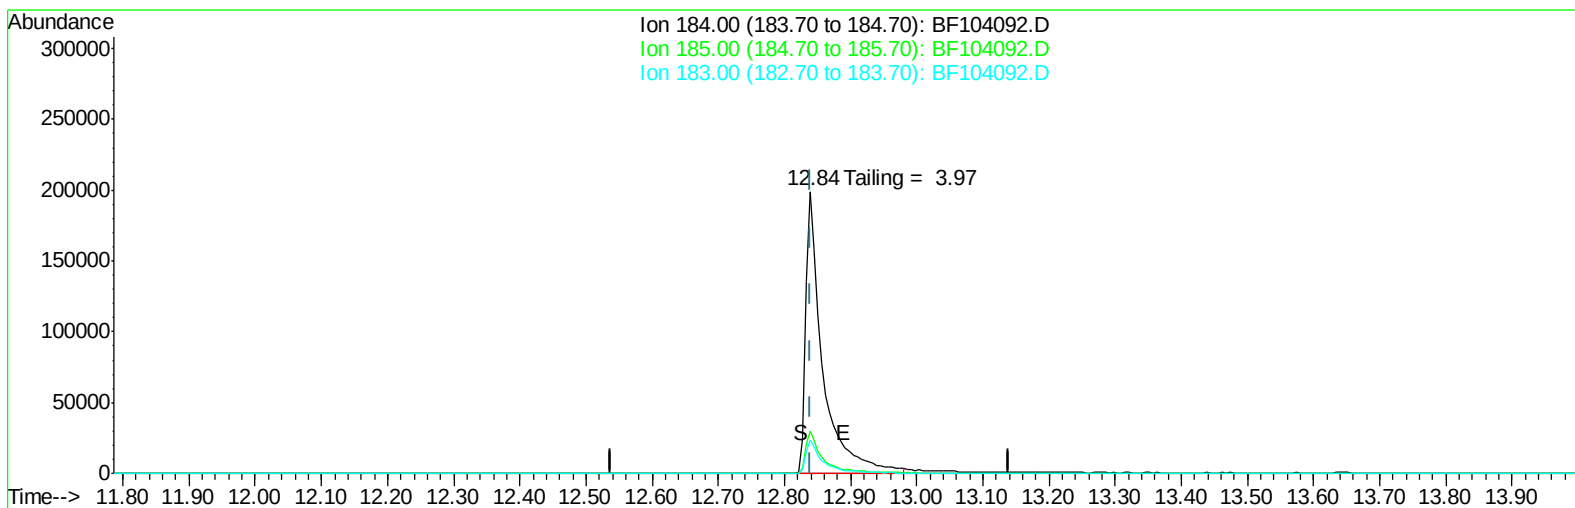

TIC: BF104092.D

(76) Benzidine

12.839min (+0.000) 0.00ng

response 361608

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.12
183.00	11.60	11.95
0.00	0.00	0.00