
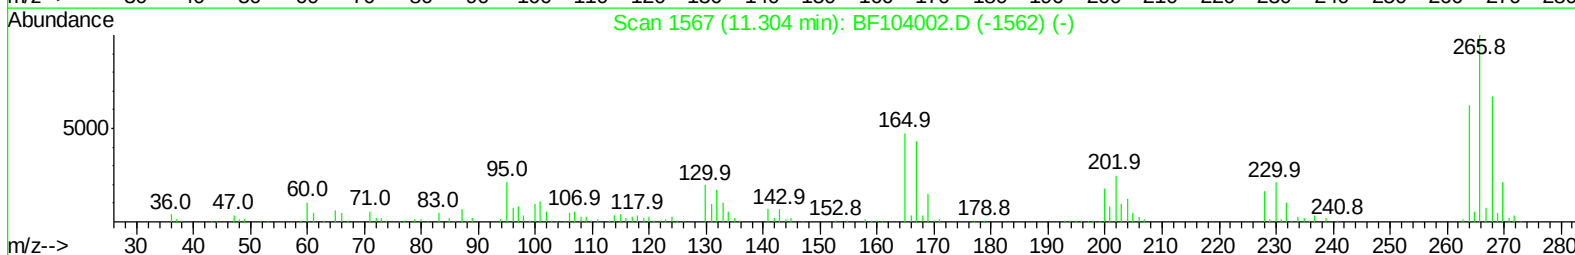
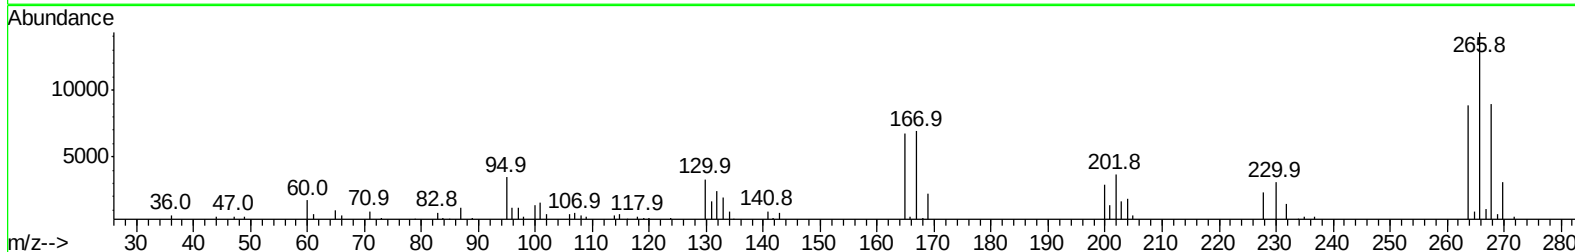


Data Path : U:\HPCHEM1\BNA F\DATA\BF033018\
Data File : BF104118.D
Acq On : 31 Mar 2018 3:03
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 01:16:42 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 30 17:20:53 2018
Response via : Initial Calibration

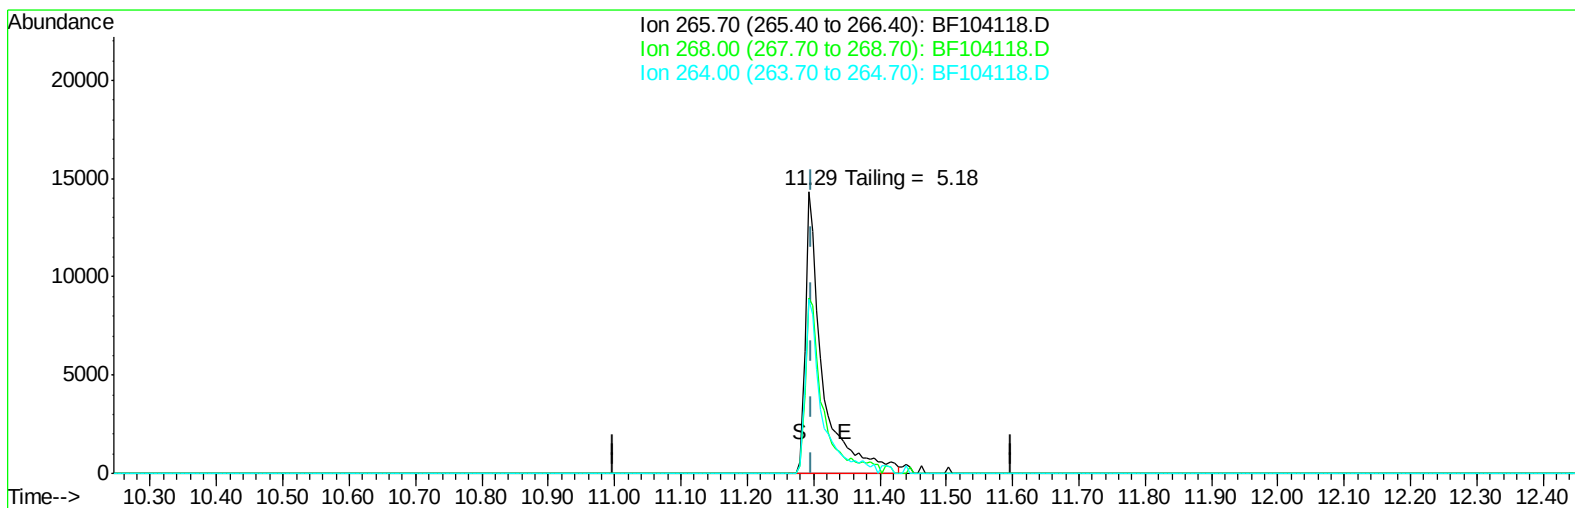

TIC: BF104118.D

(69) Pentachlorophenol (C)




11.292min (-0.006) 14906.77ng

response 26045

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.42
264.00	61.90	61.88
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF033018\
 Data File : BF104118.D
 Acq On : 31 Mar 2018 3:03
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 01:16:42 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 30 17:20:53 2018
 Response via : Initial Calibration

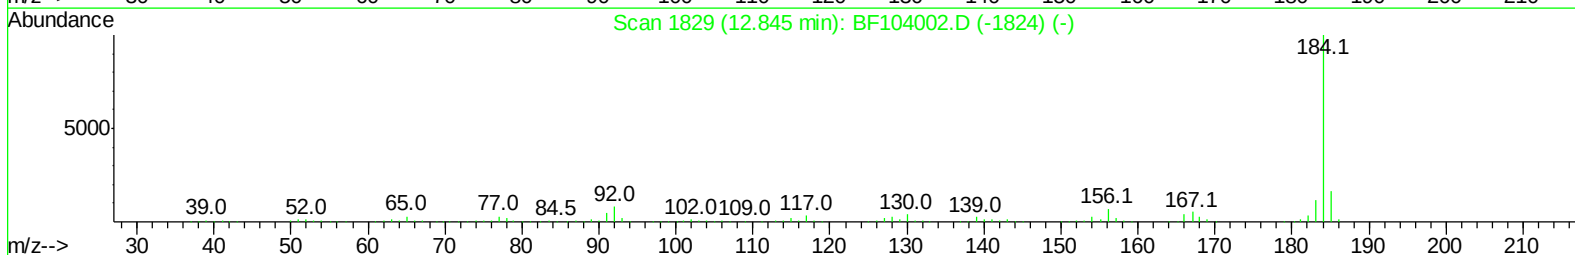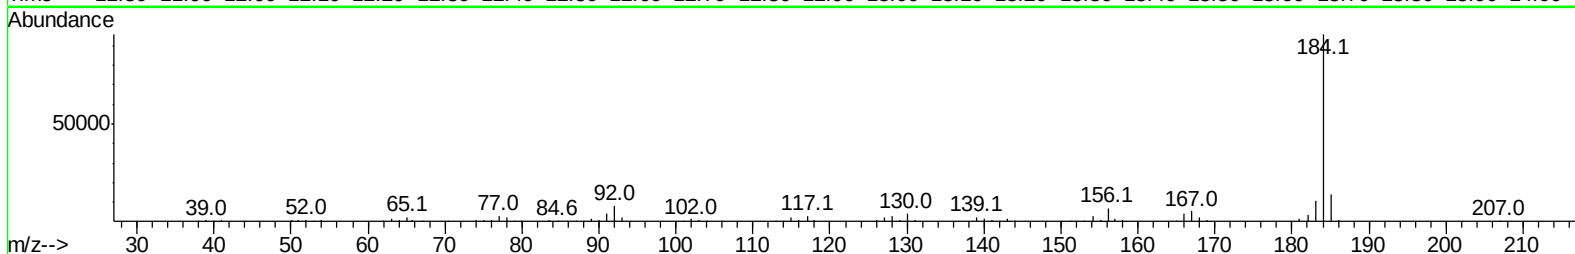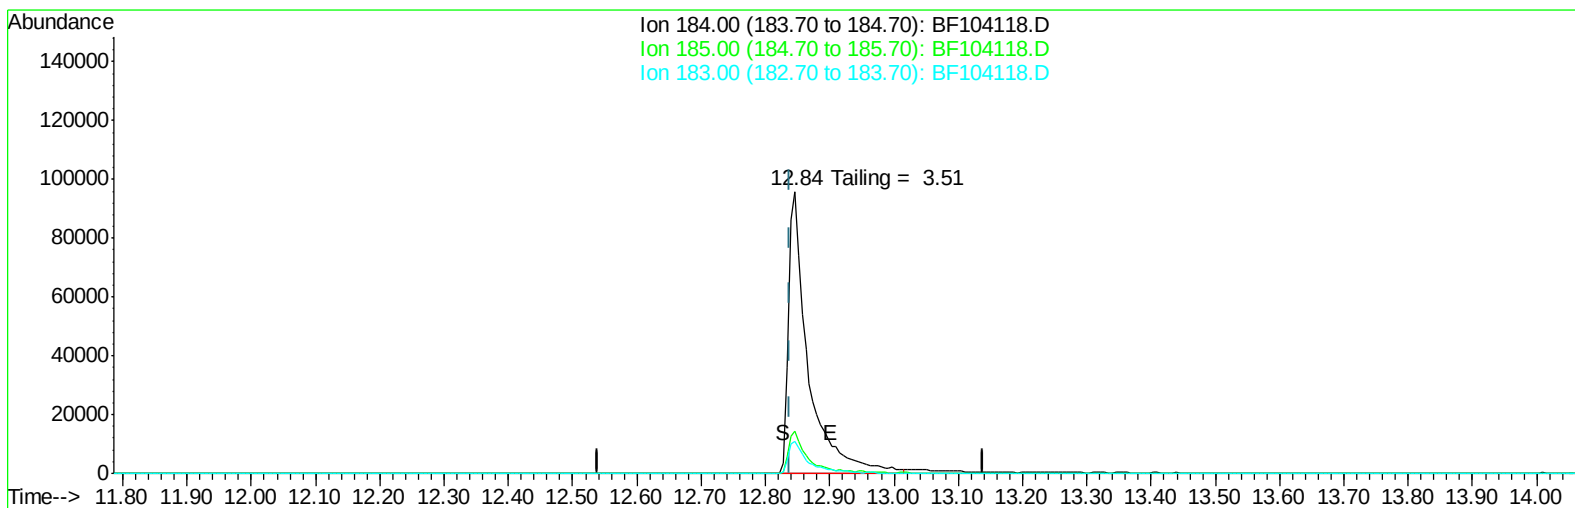

TIC: BF104118.D

(76) Benzidine

12.845min (+0.006) 0.00ng

response 209935

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.87
183.00	11.60	11.28
0.00	0.00	0.00