

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033022\
 Data File : BF127581.D
 Acq On : 30 Mar 2022 11:58
 Operator : CG\JU
 Sample : PB143716BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143716BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127581.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	478	480	495	rBV	21006	41634	1.11%	0.178%
2	5.469	538	541	564	rBV	3110526	3298738	88.22%	14.073%
3	6.481	708	713	741	rBV	2904503	3429880	91.73%	14.633%
4	6.834	769	773	787	rVB	736883	658390	17.61%	2.809%
5	7.404	865	870	873	rBV	2238999	2248406	60.13%	9.592%
6	8.116	987	991	1005	rBV	940574	862873	23.08%	3.681%
7	9.192	1168	1174	1177	rBV	3875700	3739216	100.00%	15.952%
8	9.869	1285	1289	1300	rBV	1125546	989982	26.48%	4.223%
9	10.669	1421	1425	1444	rBV	2229563	2260576	60.46%	9.644%
10	11.363	1539	1543	1553	rBV	1176669	1006556	26.92%	4.294%
11	12.751	1776	1779	1782	rBV	63683	45570	1.22%	0.194%
12	12.951	1808	1813	1816	rBV	3764069	3600537	96.29%	15.361%
13	14.010	1990	1993	2007	rBV	664092	700891	18.74%	2.990%
14	15.492	2242	2245	2260	rVB2	348140	516707	13.82%	2.204%
15	16.392	2392	2398	2406	rBV3	21937	40086	1.07%	0.171%




Sum of corrected areas: 23440042

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033022\
Data File : BF127581.D
Acq On : 30 Mar 2022 11:58
Operator : CG\JU
Sample : PB143716BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143716BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

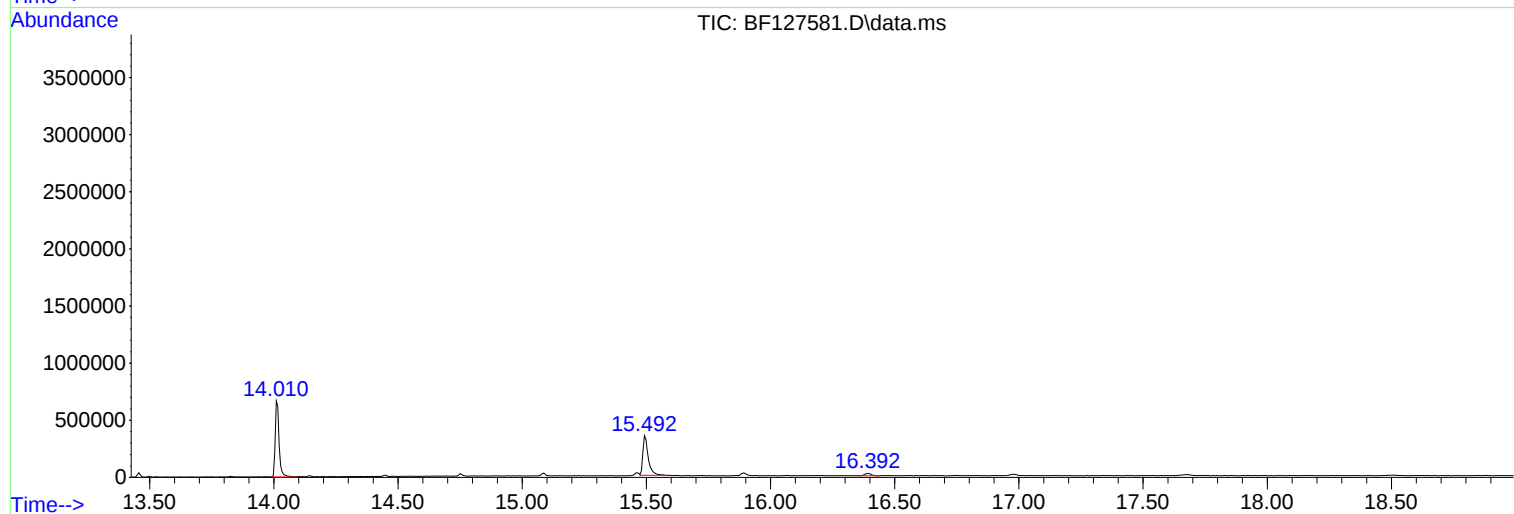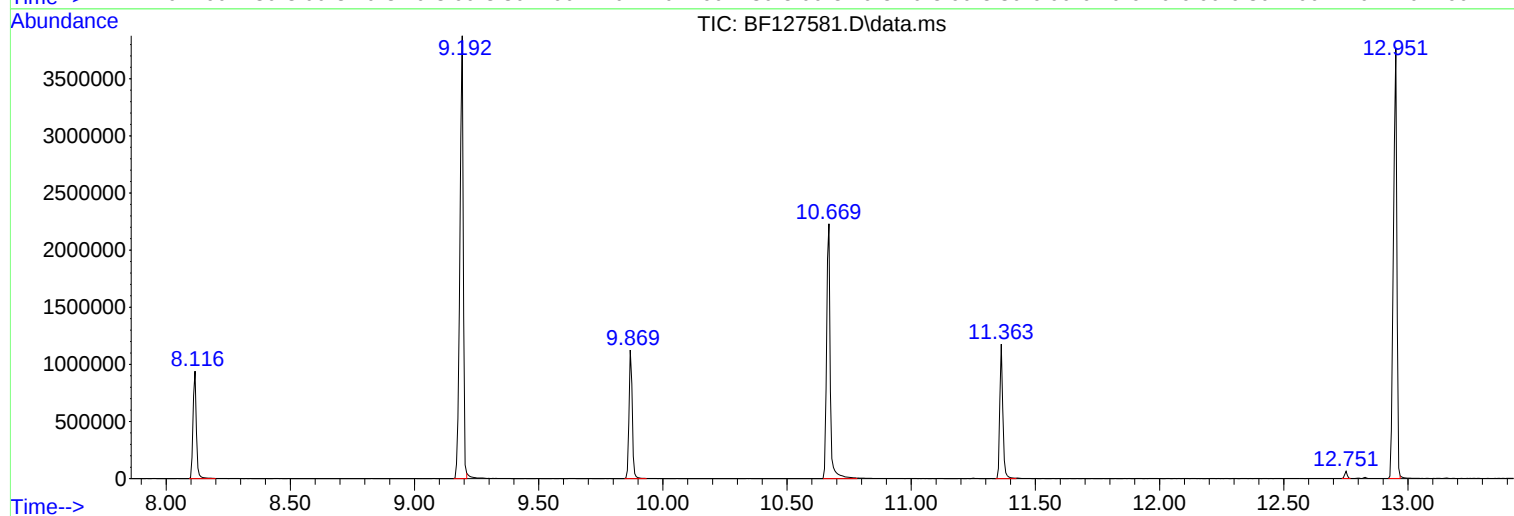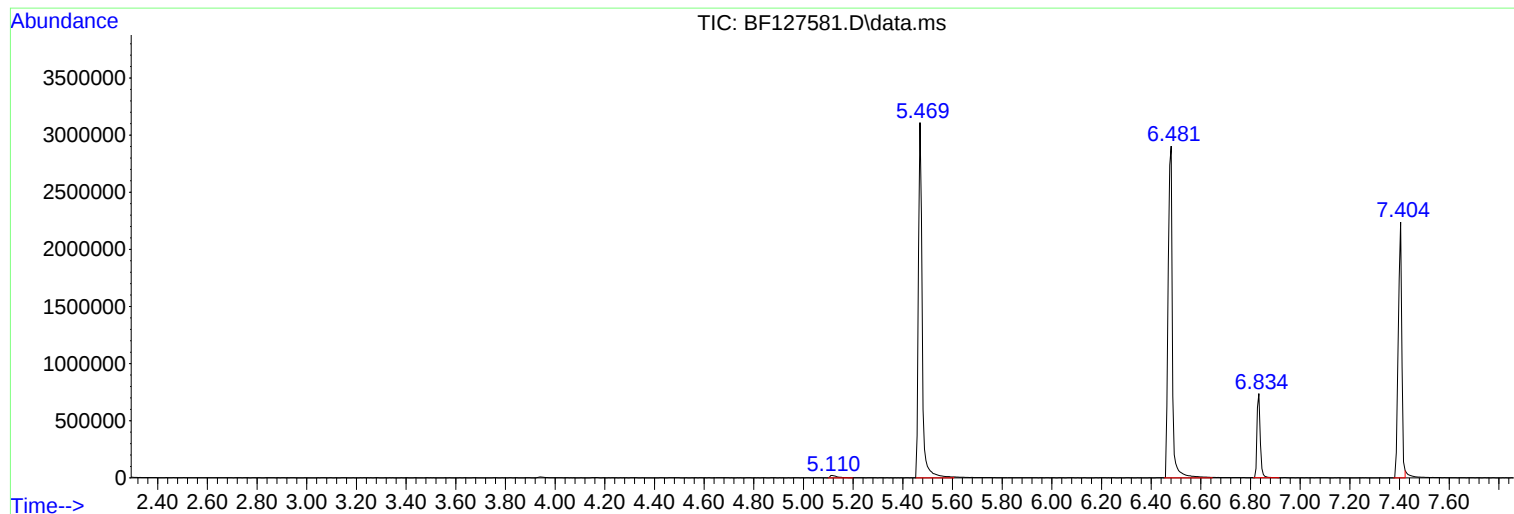

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033022\
Data File : BF127581.D
Acq On : 30 Mar 2022 11:58
Operator : CG\JU
Sample : PB143716BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143716BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033022\
Data File : BF127581.D
Acq On : 30 Mar 2022 11:58
Operator : CG\JU
Sample : PB143716BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143716BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------