

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033022\
 Data File : BF127588.D
 Acq On : 30 Mar 2022 15:16
 Operator : CG\JU
 Sample : PB143741BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143741BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127588.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.116	478	481	496	rBV	21682	42318	1.12%	0.179%
2	5.469	537	541	563	rBV	3124201	3333376	87.98%	14.103%
3	6.481	708	713	736	rBV	2884701	3470396	91.60%	14.683%
4	6.834	769	773	788	rVB	727783	679766	17.94%	2.876%
5	7.404	865	870	873	rBV	2249141	2289755	60.44%	9.687%
6	8.116	987	991	1007	rBV	941351	884470	23.35%	3.742%
7	9.192	1168	1174	1177	rBV	3912284	3788598	100.00%	16.029%
8	9.869	1285	1289	1304	rBV	1150581	1012408	26.72%	4.283%
9	10.669	1421	1425	1445	rBV	2169399	2235216	59.00%	9.457%
10	11.363	1540	1543	1552	rBV	1185444	1013817	26.76%	4.289%
11	12.751	1776	1779	1782	rBV	70049	50229	1.33%	0.213%
12	12.951	1808	1813	1816	rBV	3754493	3617632	95.49%	15.305%
13	14.015	1990	1994	2007	rBV	641474	685347	18.09%	2.900%
14	15.498	2242	2246	2260	rVB	317774	494246	13.05%	2.091%
15	16.392	2393	2398	2404	rBV3	22896	38629	1.02%	0.163%




Sum of corrected areas: 23636203

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033022\
Data File : BF127588.D
Acq On : 30 Mar 2022 15:16
Operator : CG\JU
Sample : PB143741BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143741BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

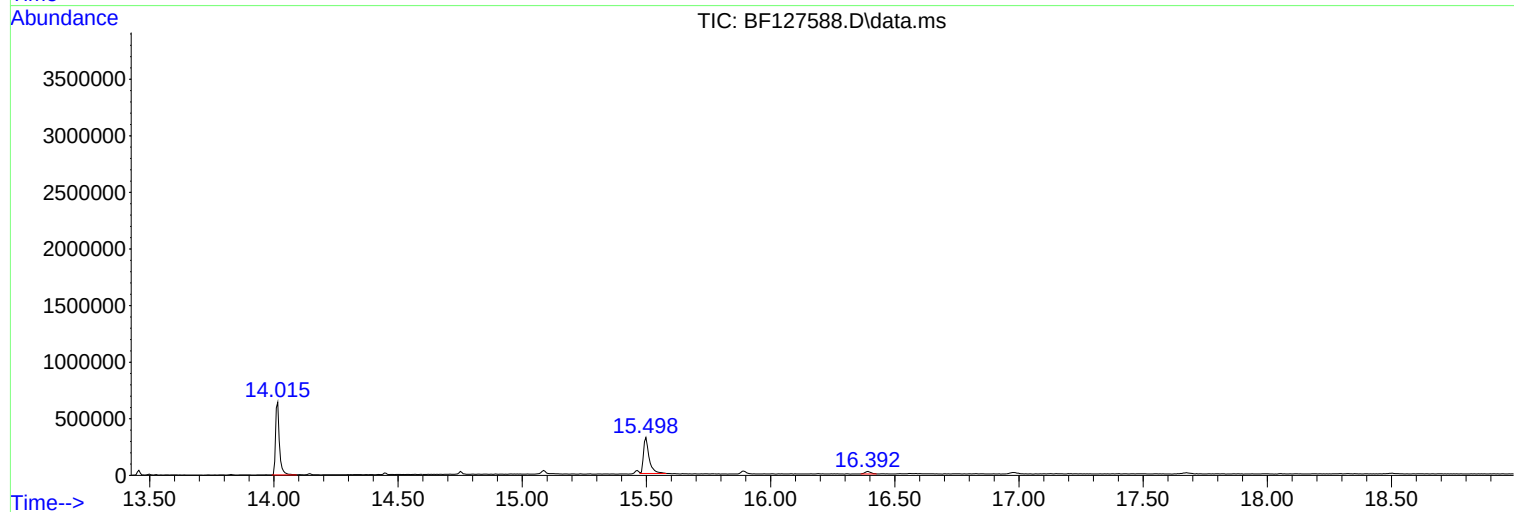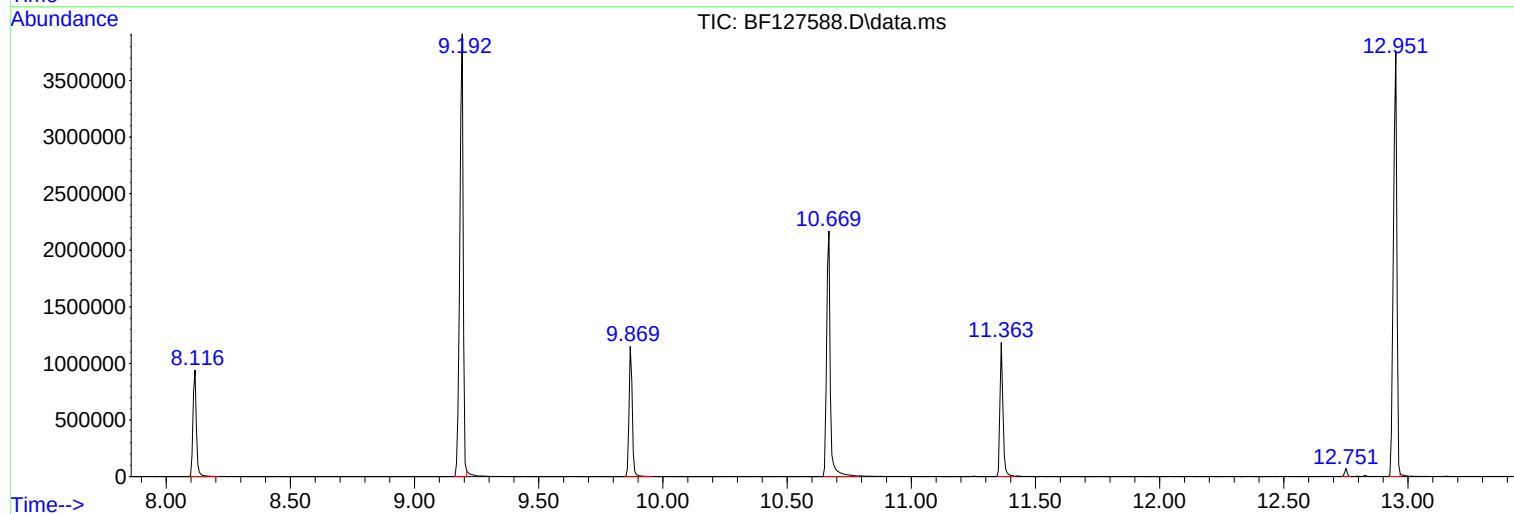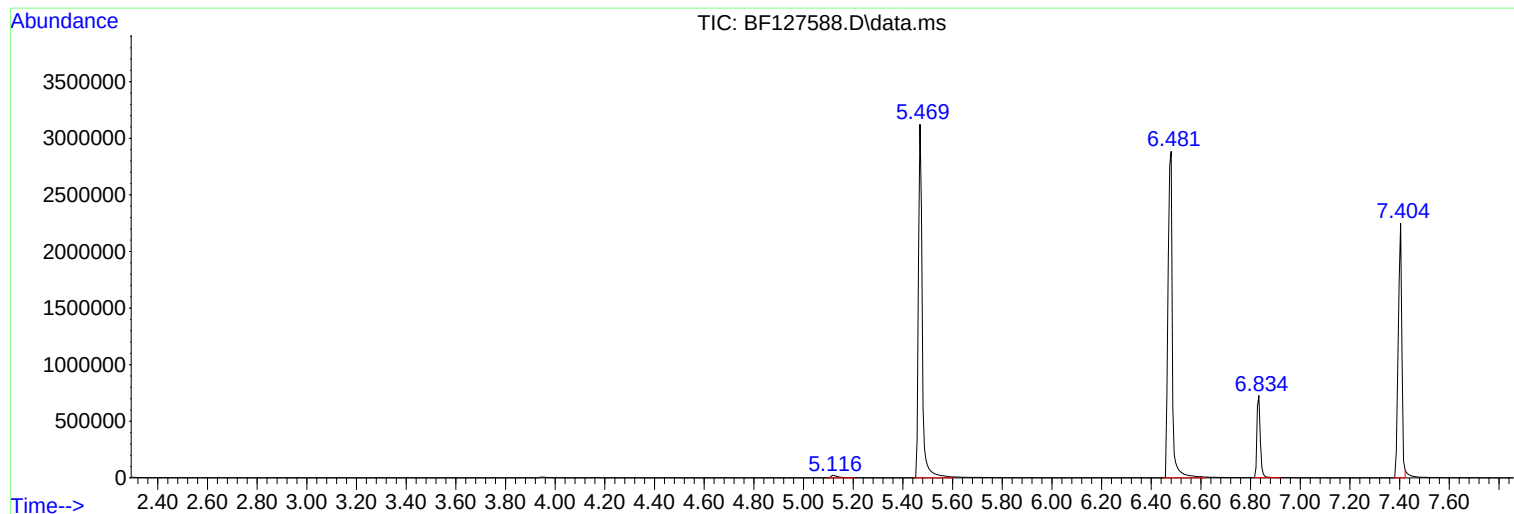

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033022\
Data File : BF127588.D
Acq On : 30 Mar 2022 15:16
Operator : CG\JU
Sample : PB143741BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143741BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033022\
Data File : BF127588.D
Acq On : 30 Mar 2022 15:16
Operator : CG\JU
Sample : PB143741BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143741BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------