


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033022\
 Data File : BF127578.D
 Acq On : 30 Mar 2022 09:59
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 29 07:13:31 2022

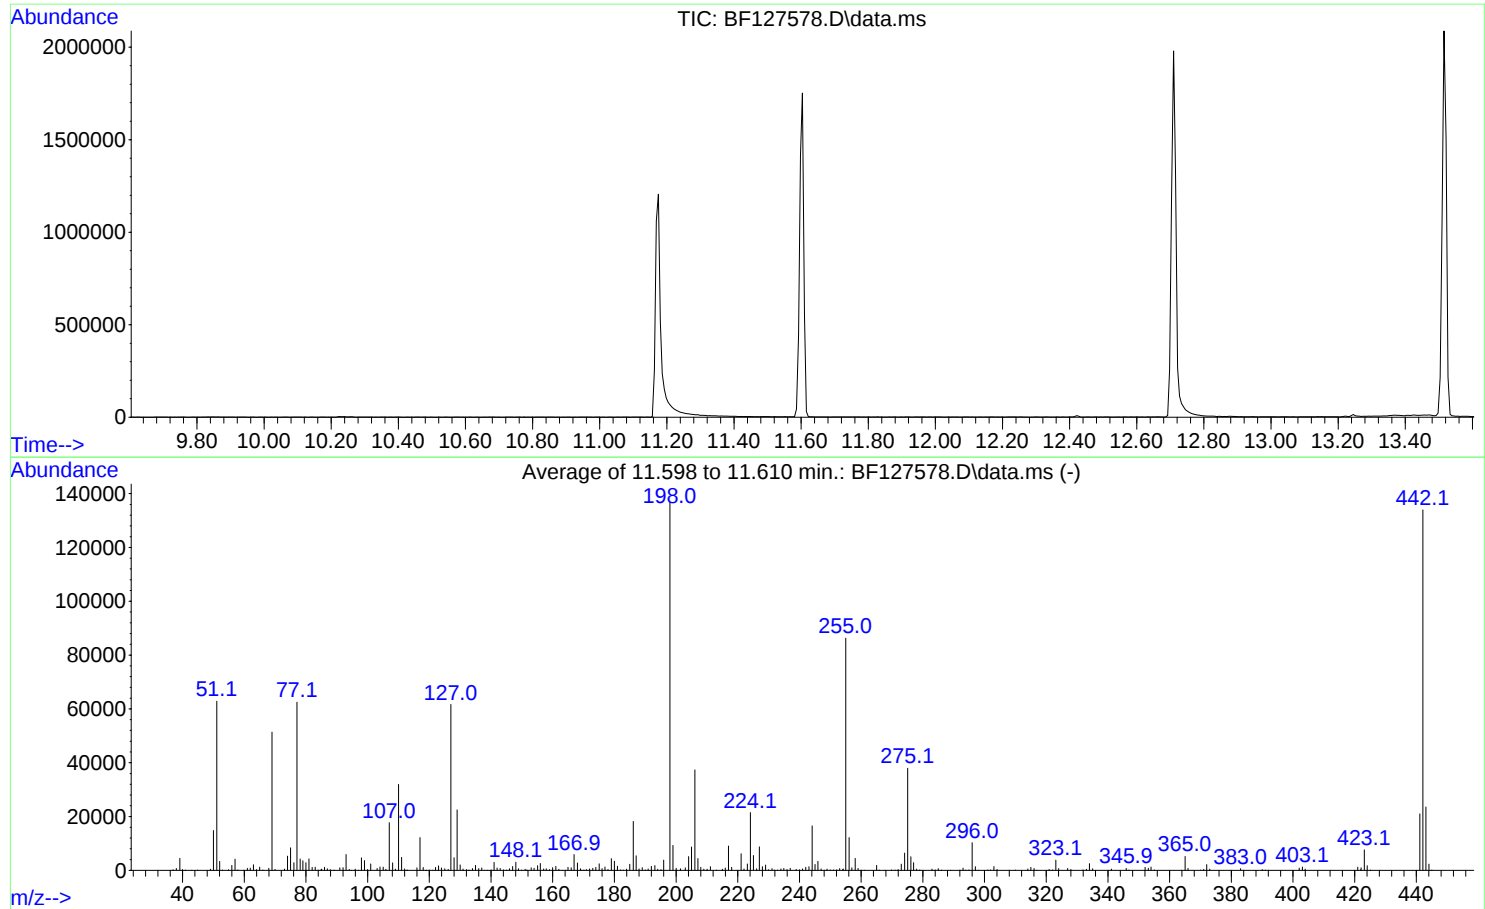




AutoFind: Scans 1583, 1584, 1585; Background Corrected with Scan 1577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	62848	PASS
68	69	0.00	2	1.5	752	PASS
69	198	0.00	100	37.6	51353	PASS
70	69	0.00	2	0.7	341	PASS
127	198	10	80	45.1	61632	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	136704	PASS
199	198	5	9	6.8	9311	PASS
275	198	10	60	27.8	37965	PASS
365	198	1	100	3.8	5195	PASS
441	198	0.01	100	15.3	20981	PASS
442	442	50	100	100.0	133995	PASS
443	442	15	24	17.6	23581	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033022\
 Data File : BF127578.D
 Acq On : 30 Mar 2022 09:59
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 30 16:55:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 29 07:13:31 2022
 Response via : Initial Calibration

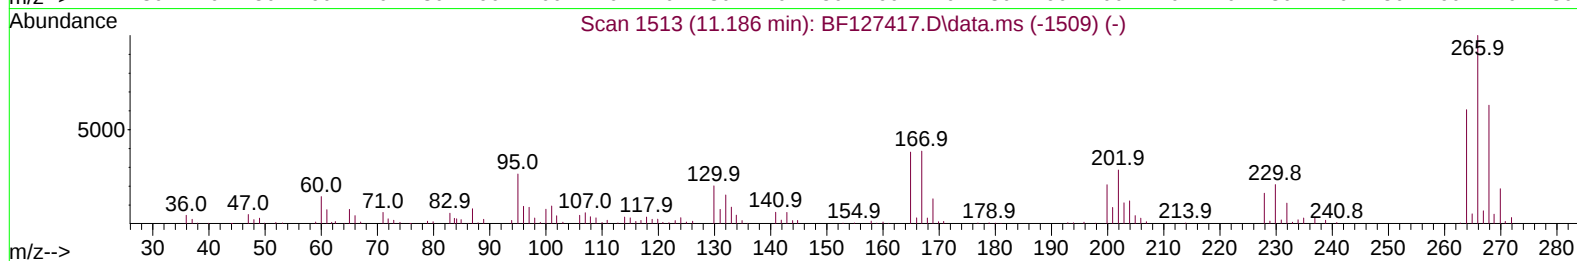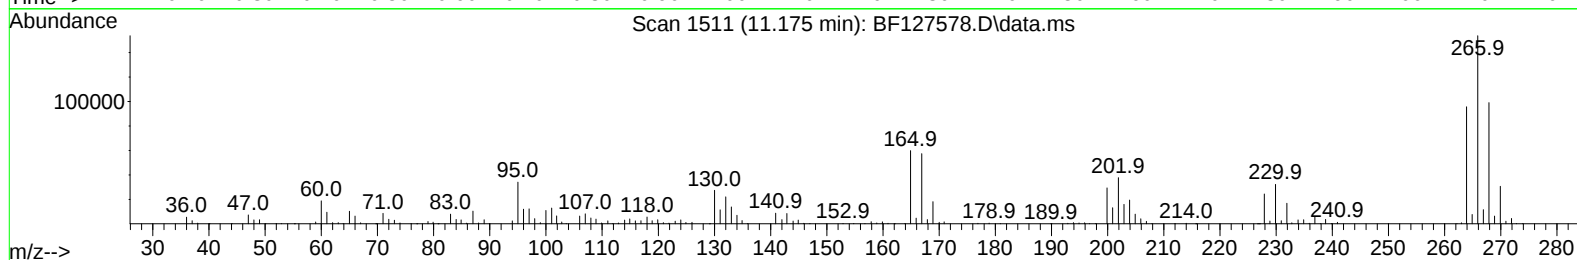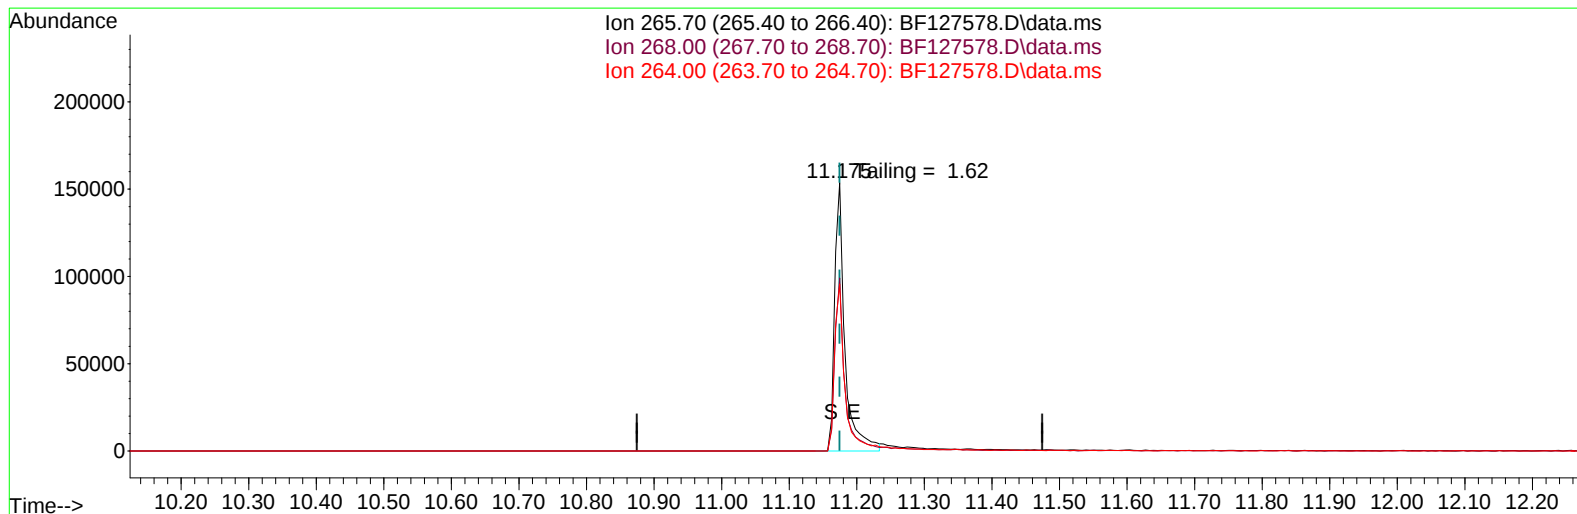

TIC: BF127578.D\data.ms

(70) Pentachlorophenol (C)

11.175min (+ 0.000) 48150.01 ng




response 168664

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.45
264.00	60.60	62.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033022\
Data File : BF127578.D
Acq On : 30 Mar 2022 09:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 30 16:55:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 29 07:13:31 2022
Response via : Initial Calibration

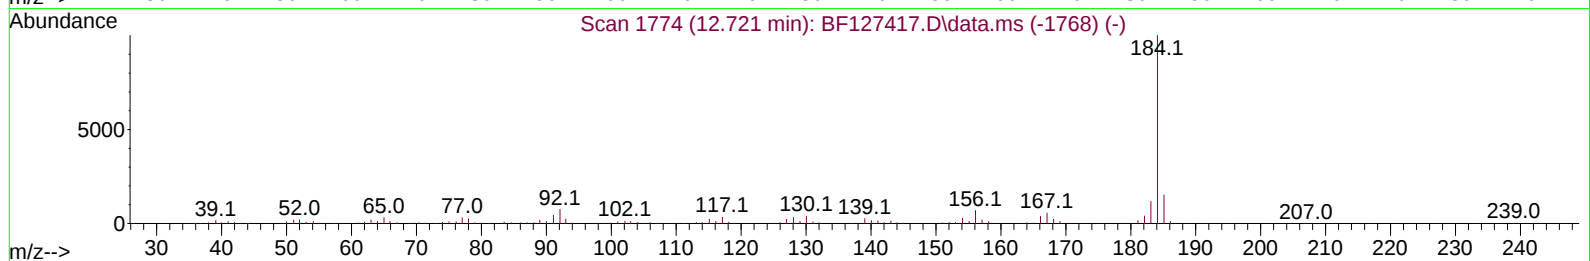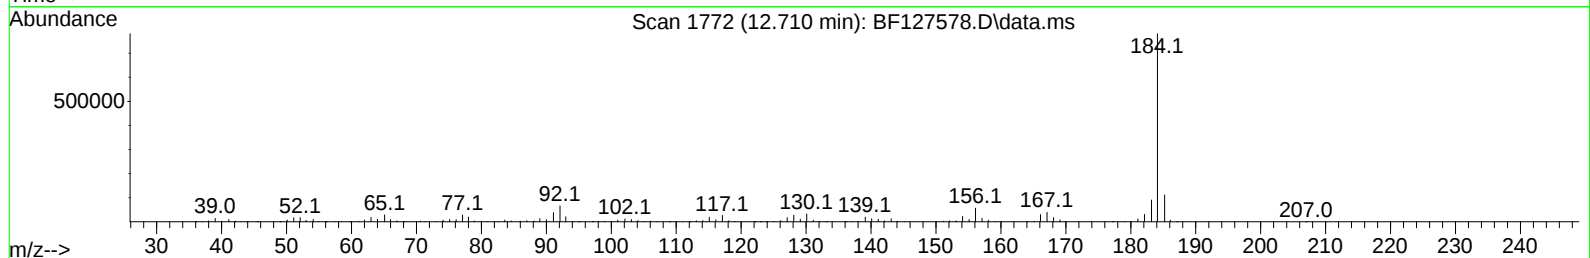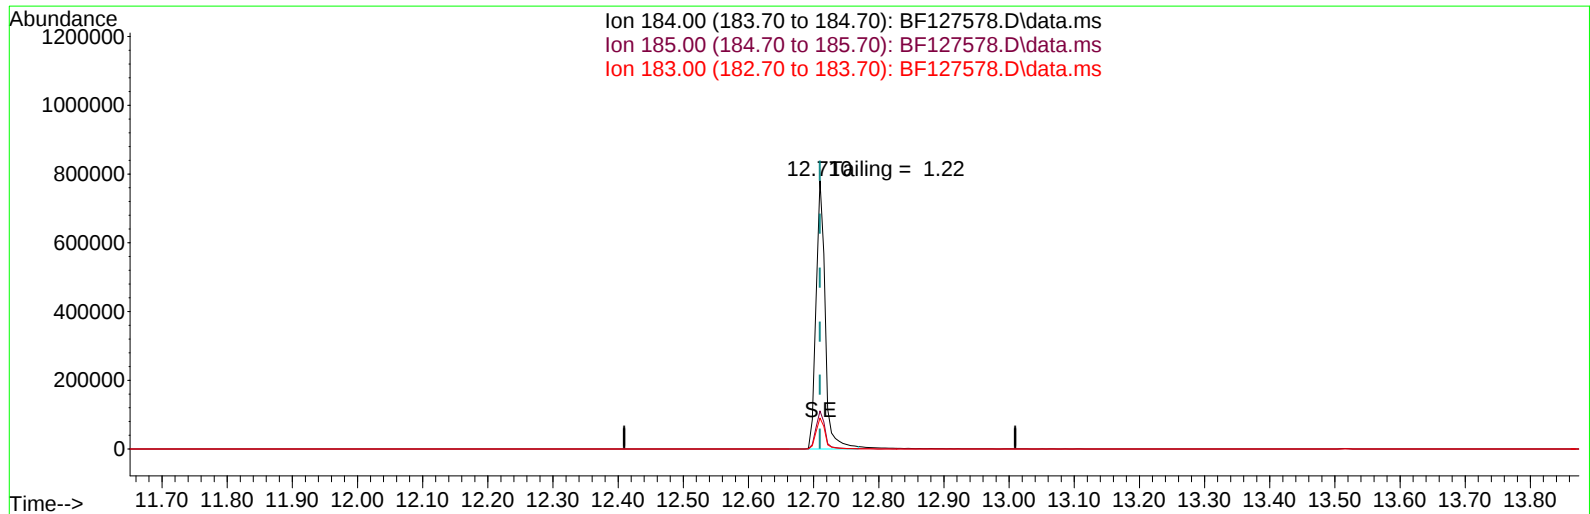

TIC: BF127578.D\data.ms

(77) Benzidine

12.710min (+ 0.000) 0.00 ng

response 776519

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.20
183.00	11.70	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/30/2022	BNA_F	<u>BF127578.D</u>
Compound Name	Response	Retention Time
DDT	364543	13.51
DDD	848	13.22
DDE	494	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1342	365885	0.37

Instrument :
BNA_F
ClientSampleId :
DFTPP