

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033115\
 Data File : BF078115.D
 Acq On : 31 Mar 2015 15:44
 Operator : TP/IZ
 Sample : G1703-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S-5(0-10)

Quant Time: Apr 01 00:20:12 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 01 00:51:03 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.05	152	40020	20.00	ng	0.00
21) Naphthalene-d8	8.62	136	163950	20.00	ng	0.00
38) Acenaphthene-d10	10.78	164	82130	20.00	ng	0.00
63) Phenanthrene-d10	12.63	188	162364	20.00	ng	0.00
75) Chrysene-d12	15.91	240	167443	20.00	ng	0.01
86) Perylene-d12	17.65	264	155976	20.00	ng	0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	154809	67.52	ng	0.00
7) Phenol-d6	6.64	99	204294	72.12	ng	0.00
23) Nitrobenzene-d5	7.74	82	110619	44.23	ng	0.00
41) 2,4,6-Tribromophenol	11.77	330	46435	59.09	ng	0.00
44) 2-Fluorobiphenyl	9.97	172	226712	40.57	ng	0.00
78) Terphenyl-d14	14.61	244	248837	36.30	ng	0.00
Target Compounds						
76) Benzidine	14.32	184	1628	Below Cal	Qvalue #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033115\
Data File : BF078115.D
Acq On : 31 Mar 2015 15:44
Operator : TP/IZ
Sample : G1703-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S-5(0-10)

Quant Time: Apr 01 00:20:12 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 01 00:51:03 2015
Response via : Initial Calibration

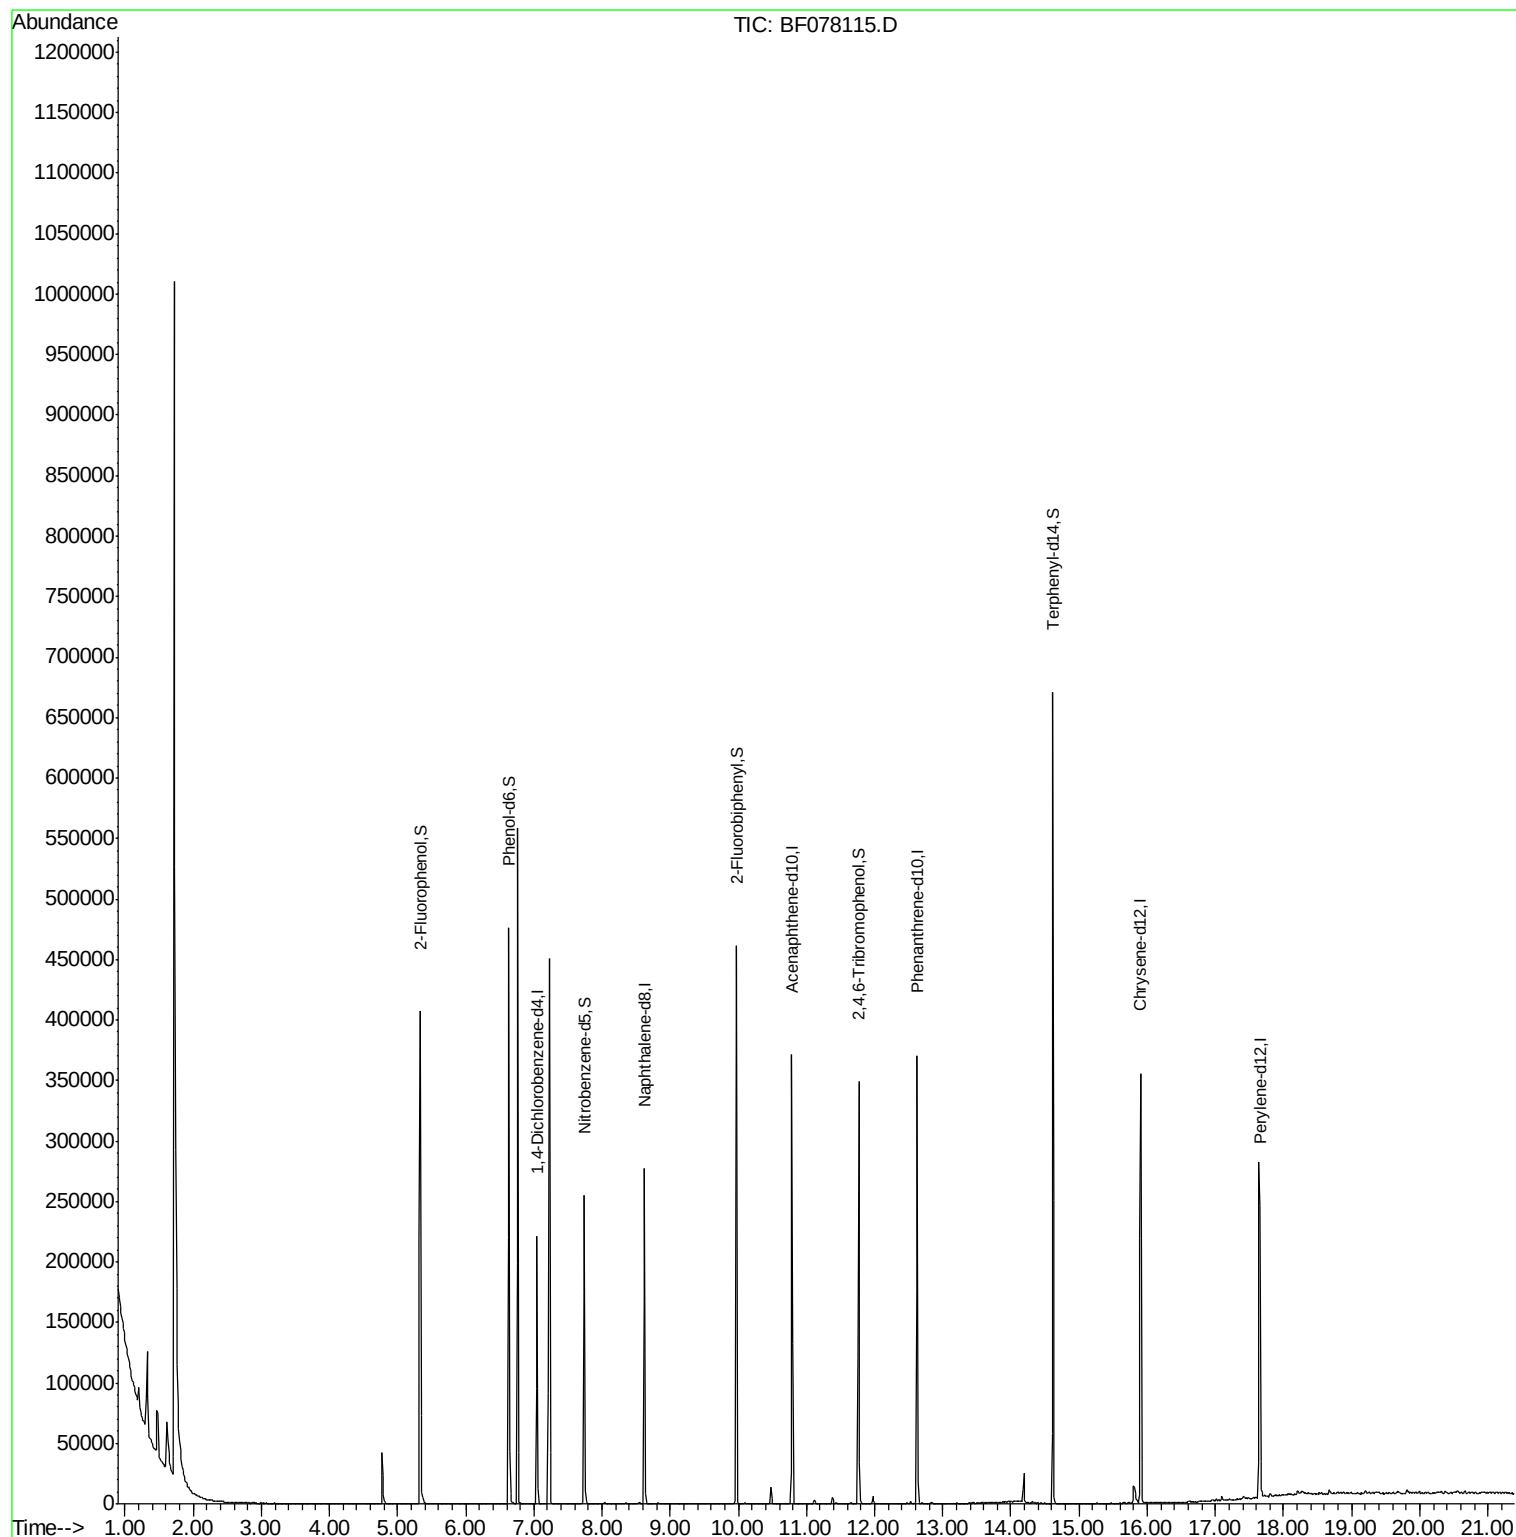

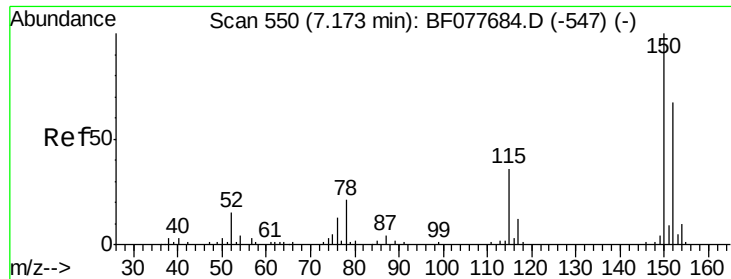


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.05 min Scan# 539
Delta R.T. 0.00 min
Lab File: BF078115.D
Acq: 31 Mar 2015 15:44

Instrument :
BNA_F
ClientSampleId :
S-5(0-10)

Tgt Ion:152 Resp: 40020
Ion Ratio Lower Upper
152 100
150 153.9 119.5 179.3
115 57.8 43.0 64.4

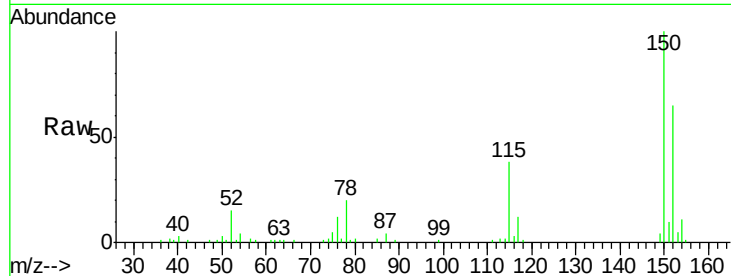


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

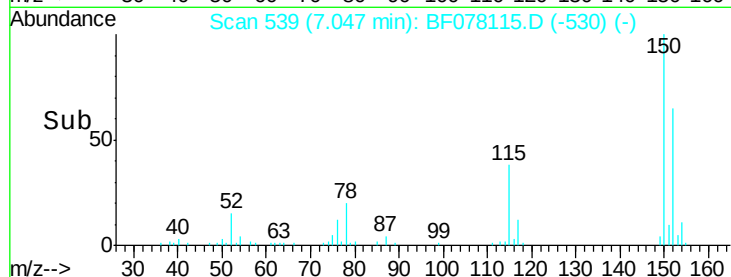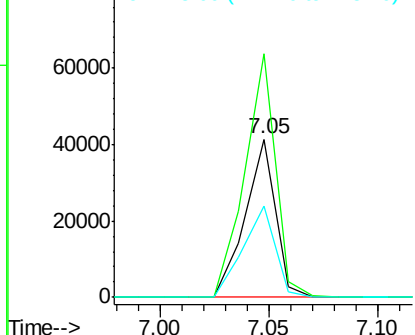



#5


2-Fluorophenol
Concen: 67.52 ng
RT: 5.33 min Scan# 389
Delta R.T. 0.00 min
Lab File: BF078115.D
Acq: 31 Mar 2015 15:44

Tgt Ion:112 Resp: 154809
Ion Ratio Lower Upper
112 100
64 50.4 38.6 57.8
63 24.9 19.3 28.9



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

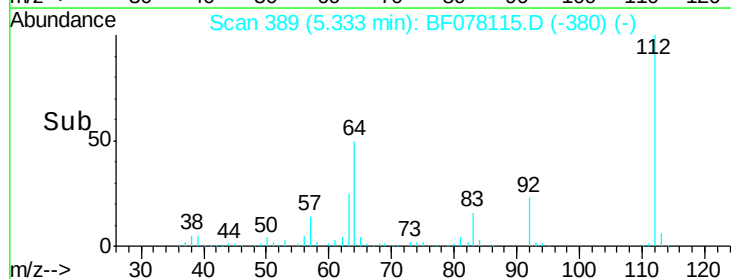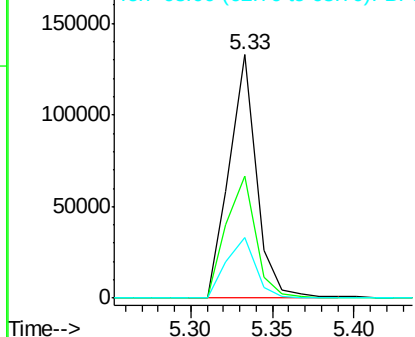

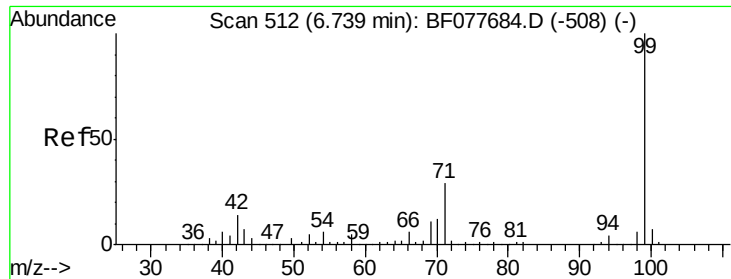

#7

Phenol-d6

Concen: 72.12 ng

RT: 6.64 min Scan# 503

Delta R.T. 0.00 min

Lab File: BF078115.D

Acq: 31 Mar 2015 15:44

Instrument :

BNA_F

ClientSampleId :

S-5(0-10)


Tgt Ion: 99 Resp: 204294

Ion Ratio Lower Upper

99 100

42 14.1 11.0 16.4

71 28.3 23.4 35.2



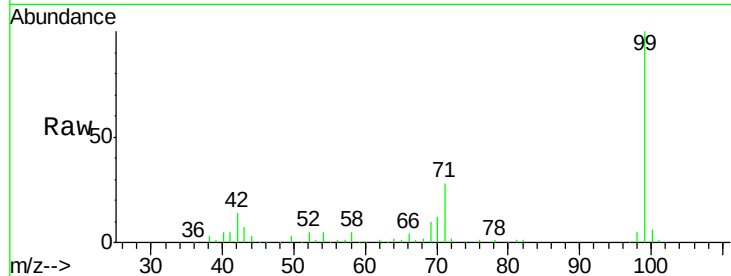


Abundance Ion 99.00 (98.70 to 99.70): BF077684.D (-508) (-)

Ion 42.00 (41.70 to 42.70): BF077684.D (-508) (-)

Ion 71.00 (70.70 to 71.70): BF077684.D (-508) (-)

Time-->

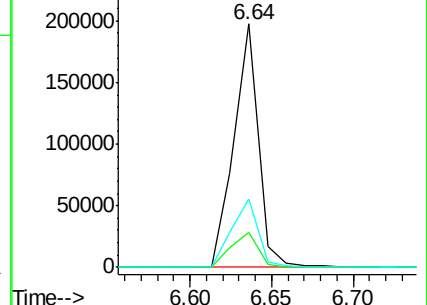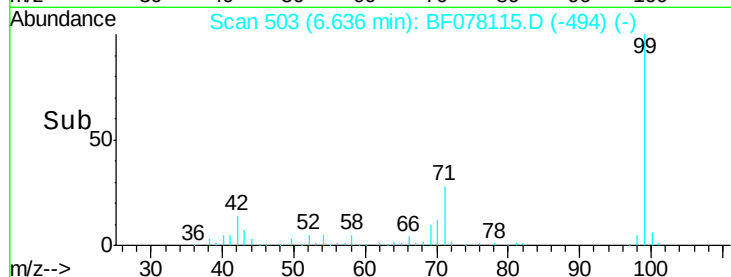

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.62 min Scan# 677

Delta R.T. 0.00 min

Lab File: BF078115.D

Acq: 31 Mar 2015 15:44

Tgt Ion: 136 Resp: 163950


Ion Ratio Lower Upper

136 100

137 10.4 8.7 13.1

54 5.3 4.6 6.8

68 4.6 3.7 5.5





Abundance Ion 136.00 (135.70 to 136.70): BF077684.D (-684) (-)


Ion 137.00 (136.70 to 137.70): BF077684.D (-684) (-)

Ion 54.00 (53.70 to 54.70): BF077684.D (-684) (-)

Ion 68.00 (67.70 to 68.70): BF077684.D (-684) (-)

Time-->

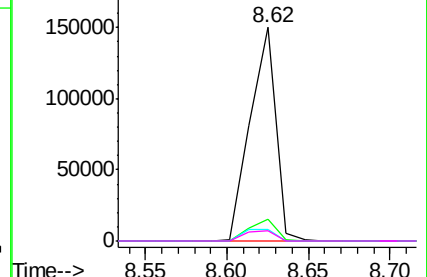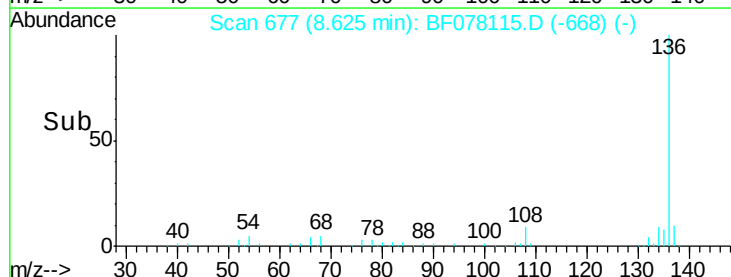


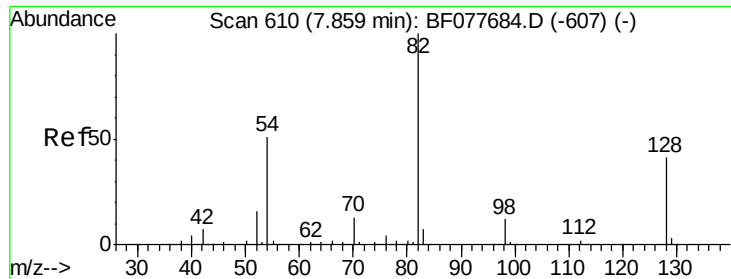




#23
 Nitrobenzene-d5
 Concen: 44.23 ng
 RT: 7.74 min Scan# 600
 Delta R.T. 0.00 min
 Lab File: BF078115.D
 Acq: 31 Mar 2015 15:44

Instrument :
 BNA_F
 ClientSampleId :
 S-5(0-10)

Tgt Ion: 82 Resp: 110619
 Ion Ratio Lower Upper
 82 100
 128 52.1 32.8 49.2#
 54 41.7 40.6 60.8




Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

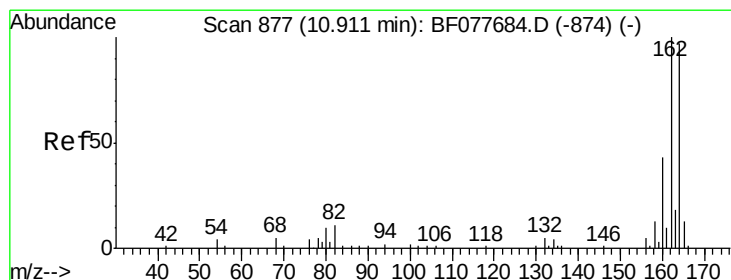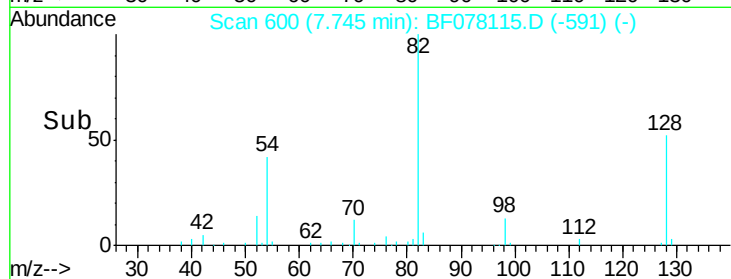
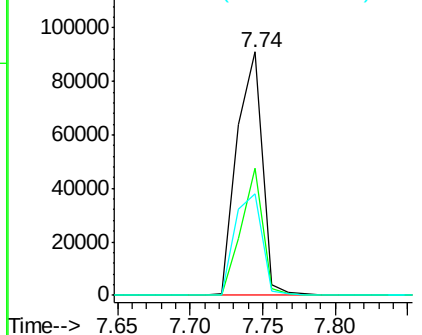



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.78 min Scan# 866
 Delta R.T. 0.00 min
 Lab File: BF078115.D
 Acq: 31 Mar 2015 15:44

Tgt Ion: 164 Resp: 82130
 Ion Ratio Lower Upper
 164 100
 162 100.1 82.4 123.6
 160 44.2 35.8 53.6

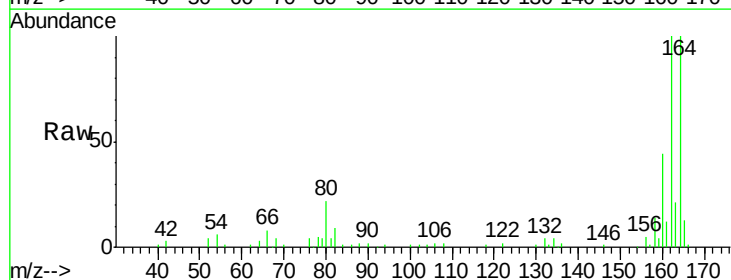

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

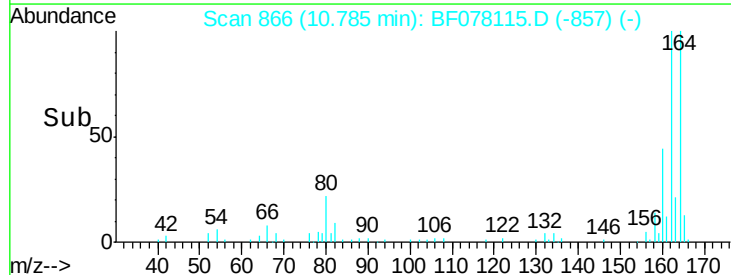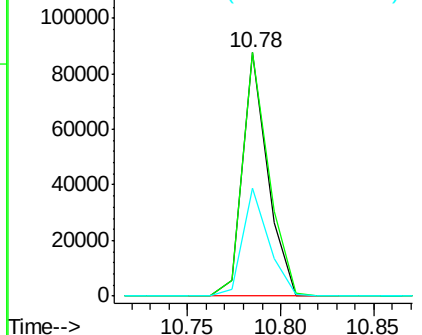


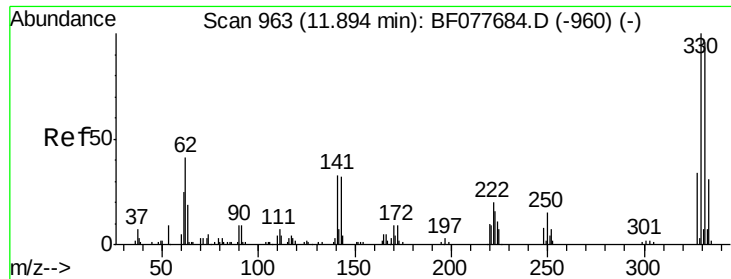




#41
2,4,6-Tribromophenol
Concen: 59.09 ng
RT: 11.77 min Scan# 952
Delta R.T. 0.00 min
Lab File: BF078115.D
Acq: 31 Mar 2015 15:44

Instrument :
BNA_F
ClientSampleId :
S-5(0-10)

Tgt Ion:330 Resp: 46435
Ion Ratio Lower Upper
330 100
332 91.4 0.0 0.0#
141 35.1 0.0 0.0#

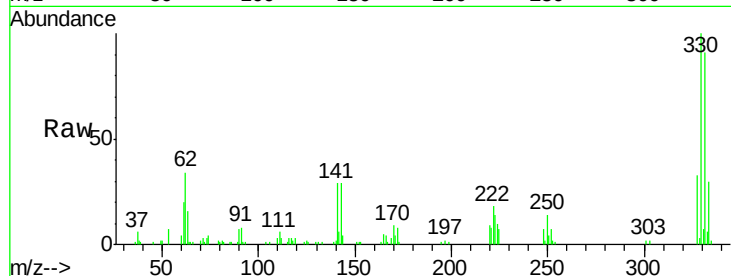


Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

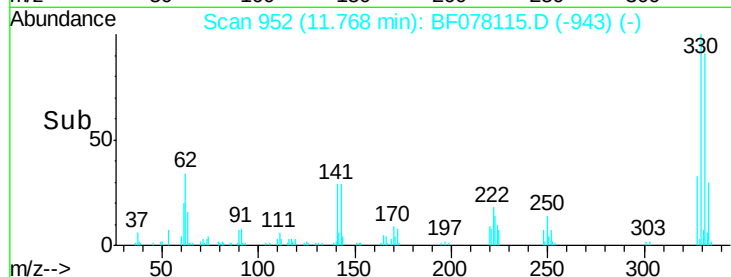
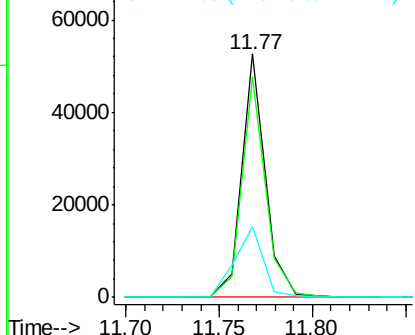



#44
2-Fluorobiphenyl
Concen: 40.57 ng
RT: 9.97 min Scan# 795
Delta R.T. 0.00 min
Lab File: BF078115.D
Acq: 31 Mar 2015 15:44

Tgt Ion:172 Resp: 226712
Ion Ratio Lower Upper
172 100
171 34.2 28.5 42.7
170 22.3 18.8 28.2



Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

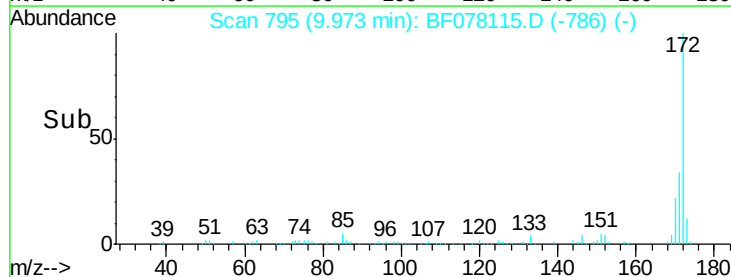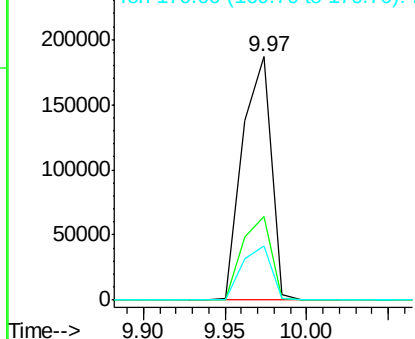


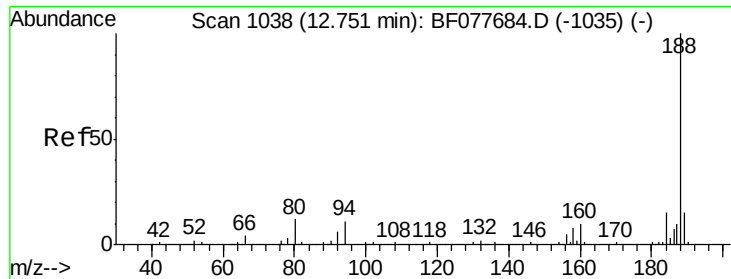




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.63 min Scan# 1027
Delta R.T. 0.00 min
Lab File: BF078115.D
Acq: 31 Mar 2015 15:44

Instrument :
BNA_F
ClientSampleId :
S-5(0-10)

Tgt Ion:188 Resp: 162364
Ion Ratio Lower Upper
188 100
94 8.4 8.7 13.1#
80 8.4 9.3 13.9#




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

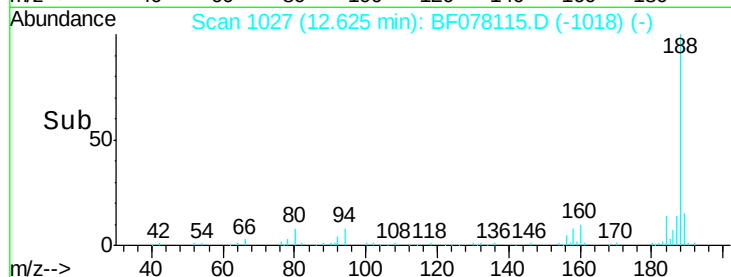
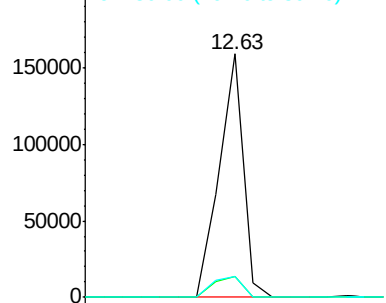



#75
Chrysene-d12
Concen: 20.00 ng
RT: 15.91 min Scan# 1314
Delta R.T. 0.01 min
Lab File: BF078115.D
Acq: 31 Mar 2015 15:44

Tgt Ion:240 Resp: 167443
Ion Ratio Lower Upper
240 100
120 9.1 8.2 12.2
236 24.4 20.0 30.0



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



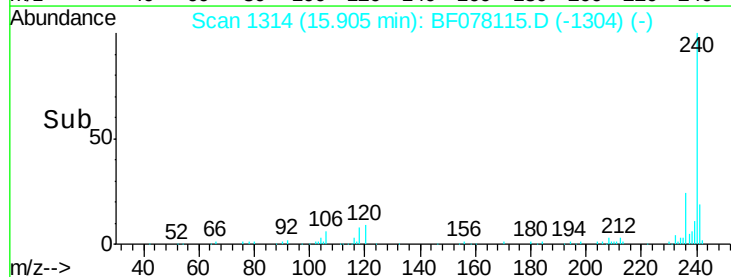
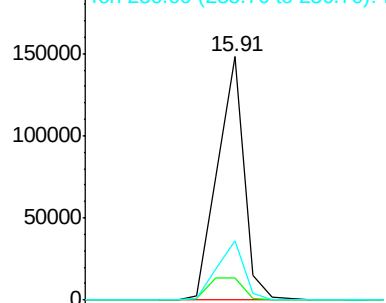


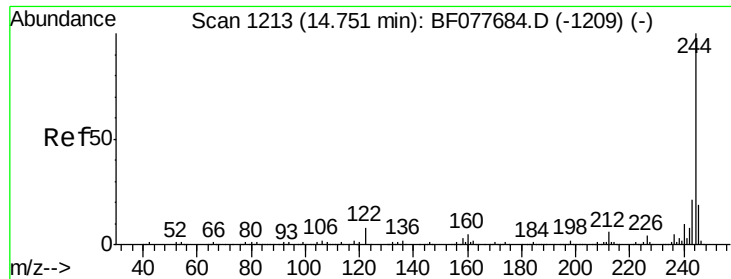

#78
 Terphenyl-d14
 Concen: 36.30 ng
 RT: 14.61 min Scan# 1201
 Delta R.T. 0.00 min
 Lab File: BF078115.D
 Acq: 31 Mar 2015 15:44

Instrument :
 BNA_F
 ClientSampleId :
 S-5(0-10)

Tgt Ion	Ratio	Lower	Upper
244	100		
212	6.7	4.9	7.3
122	13.6	6.2	9.4

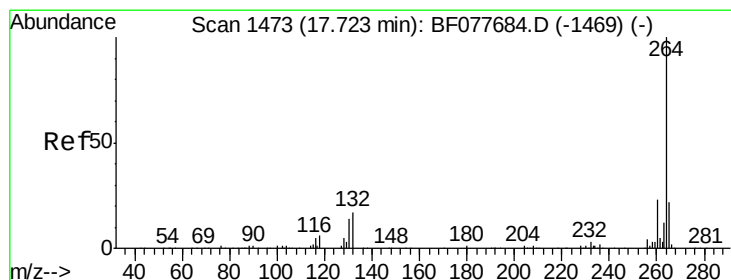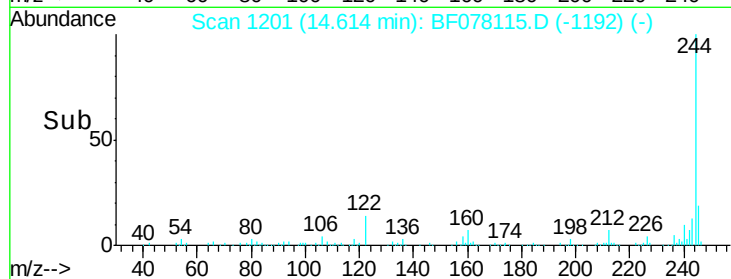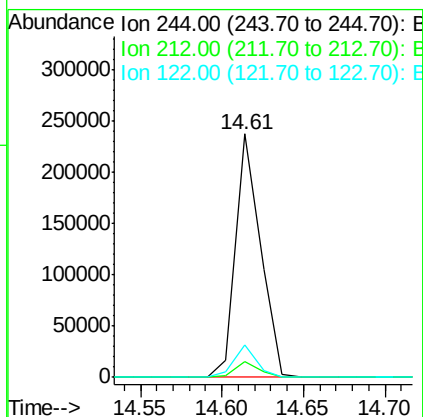

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 17.65 min Scan# 1467
 Delta R.T. 0.05 min
 Lab File: BF078115.D
 Acq: 31 Mar 2015 15:44

Tgt Ion	Ratio	Lower	Upper
264	100		
260	22.2	18.6	27.8
265	21.3	17.3	25.9

