

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031115\
 Data File : BF078140.D
 Acq On : 1 Apr 2015 5:30
 Operator : TP/IZ
 Sample : G1703-19
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S-10(0-10)

Quant Time: Apr 01 05:46:47 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 01 00:51:03 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.05	152	40656	20.00	ng	0.00
21) Naphthalene-d8	8.62	136	169057	20.00	ng	0.00
38) Acenaphthene-d10	10.79	164	84882	20.00	ng	0.00
63) Phenanthrene-d10	12.63	188	171435	20.00	ng	0.00
75) Chrysene-d12	15.91	240	169491	20.00	ng	0.01
86) Perylene-d12	17.67	264	158161	20.00	ng	0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	346762	148.88	ng	0.00
7) Phenol-d6	6.64	99	462910	160.86	ng	0.00
23) Nitrobenzene-d5	7.74	82	257377	99.80	ng	0.00
41) 2,4,6-Tribromophenol	11.77	330	103419	127.34	ng	0.00
44) 2-Fluorobiphenyl	9.97	172	499236	86.44	ng	0.00
78) Terphenyl-d14	14.61	244	576247	83.05	ng	0.00
Target Compounds						
49) Dimethylphthalate	10.48	163	13009	2.07	ng	96
76) Benzidine	14.32	184	1900	Below Cal	#	68
79) Butylbenzylphthalate	15.24	149	9777	2.33	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033115\
Data File : BF078140.D
Acq On : 1 Apr 2015 5:30
Operator : TP/IZ
Sample : G1703-19
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S-10(0-10)

Quant Time: Apr 01 05:46:47 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 01 00:51:03 2015
Response via : Initial Calibration

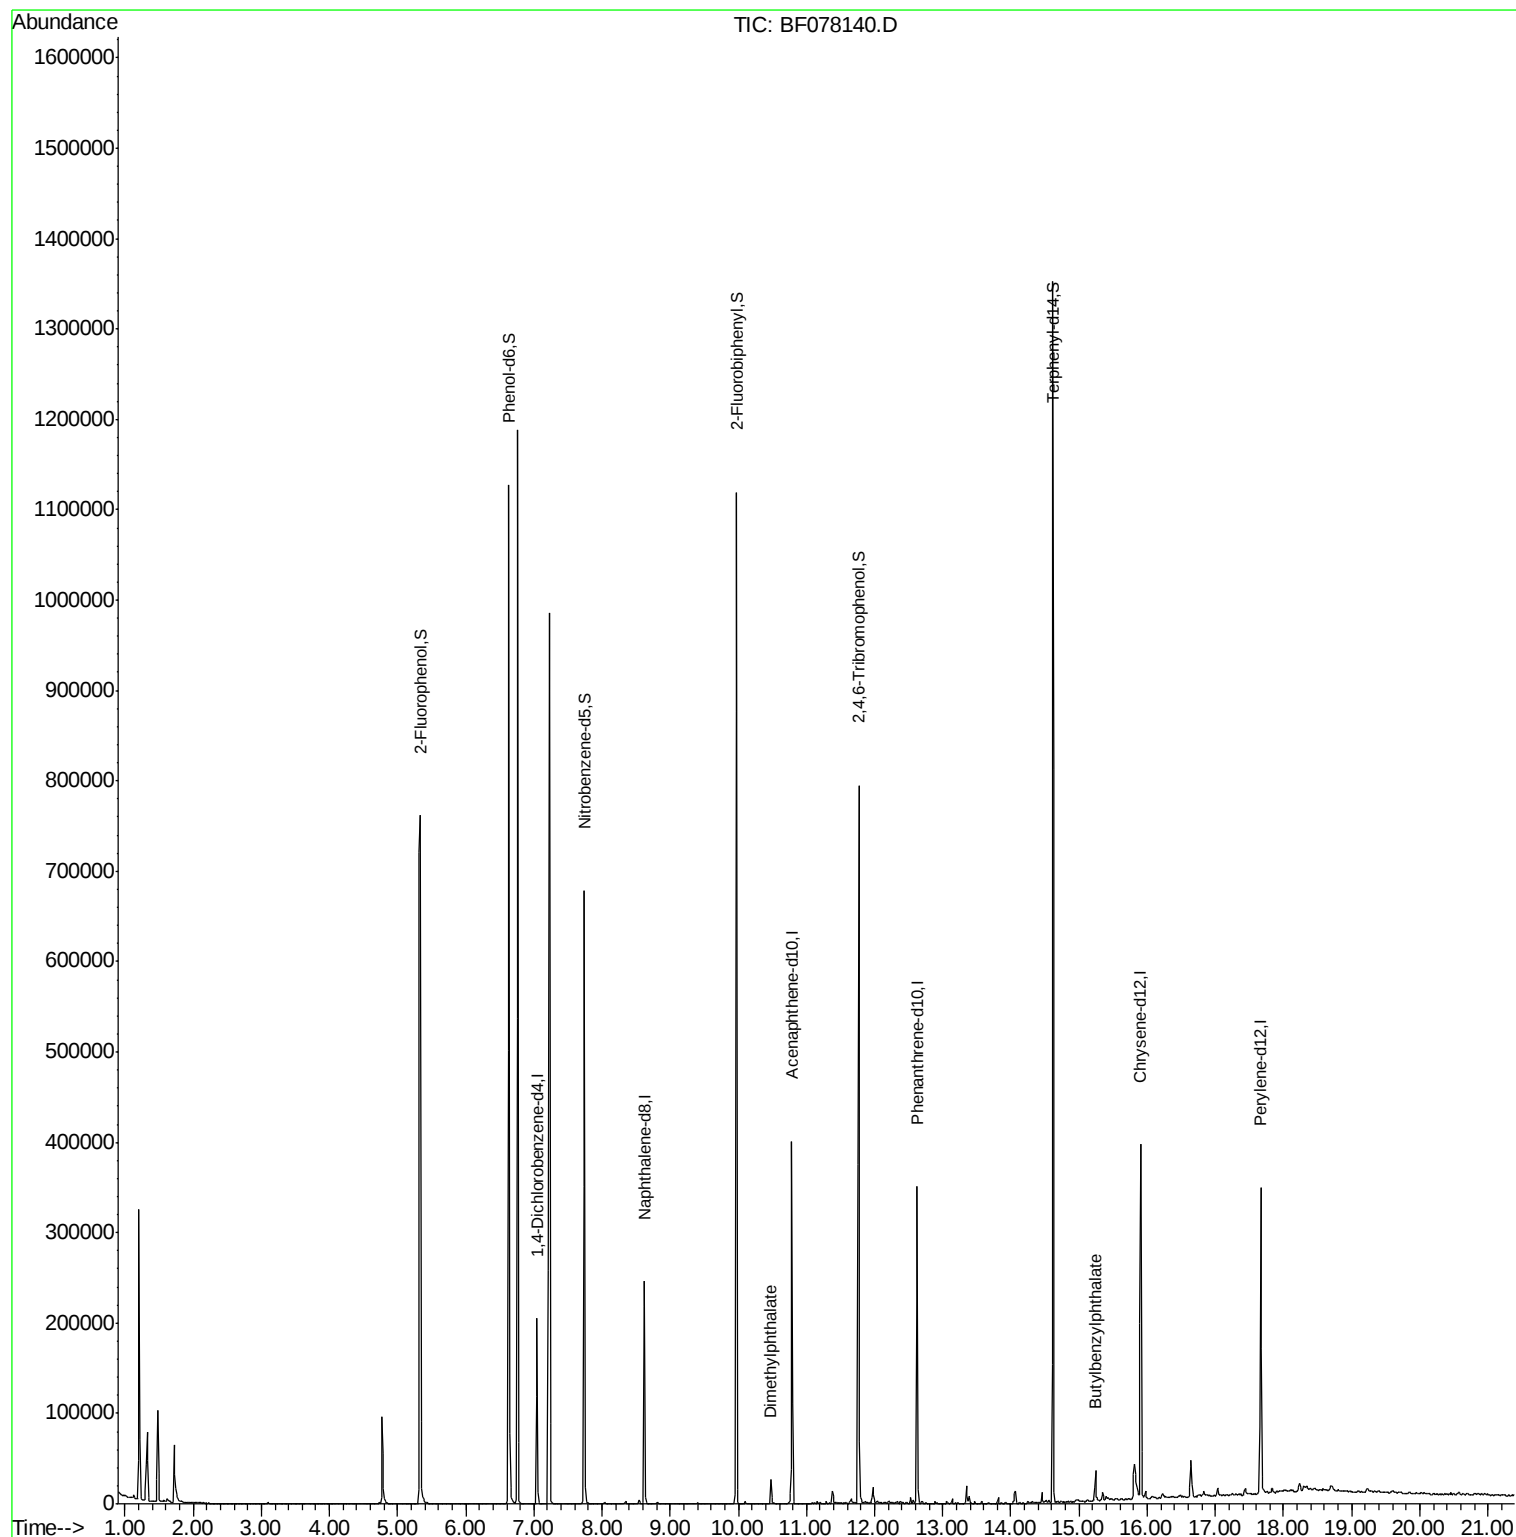

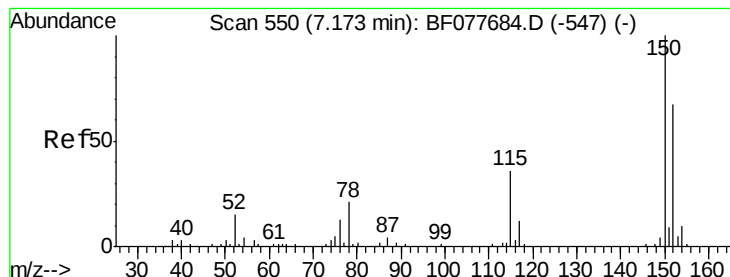

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.05 min Scan# 539

Delta R.T. 0.00 min

Lab File: BF078140.D

Acq: 1 Apr 2015 5:30

Instrument :

BNA_F

ClientSampleId :

S-10(0-10)


Tgt Ion:152 Resp: 40656

Ion Ratio Lower Upper

152 100

150 157.8 119.5 179.3




115 56.2 43.0 64.4

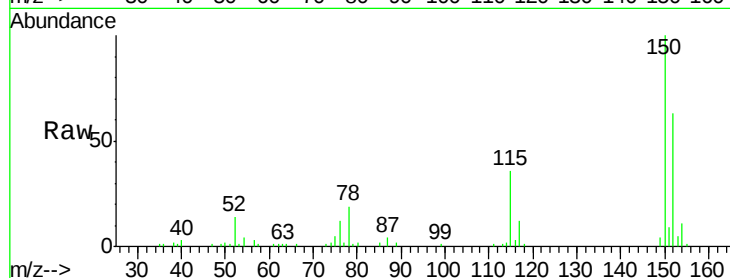

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

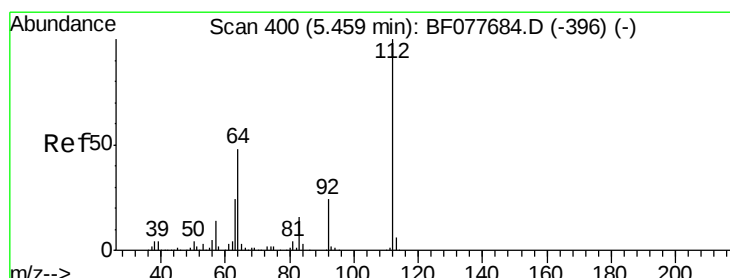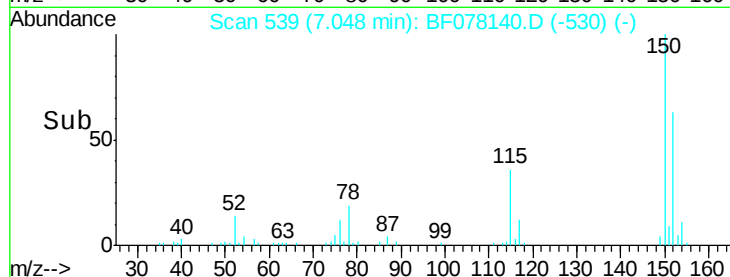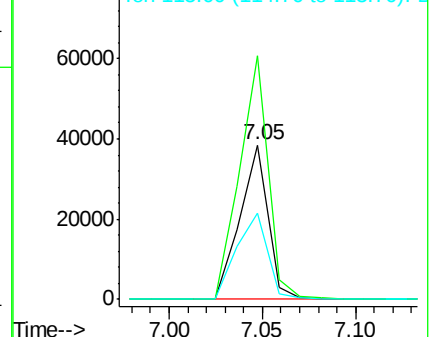

#5

2-Fluorophenol

Concen: 148.88 ng

RT: 5.33 min Scan# 389

Delta R.T. 0.00 min

Lab File: BF078140.D

Acq: 1 Apr 2015 5:30


Tgt Ion:112 Resp: 346762

Ion Ratio Lower Upper

112 100

64 47.7 38.6 57.8



63 24.5 19.3 28.9

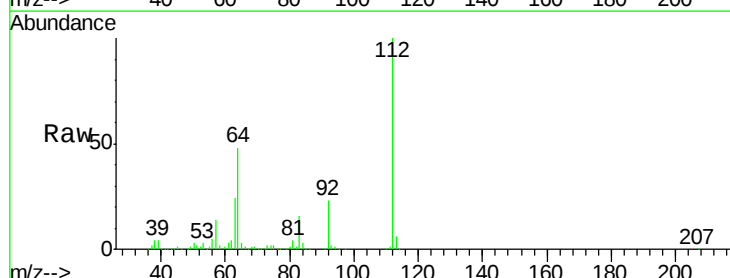

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

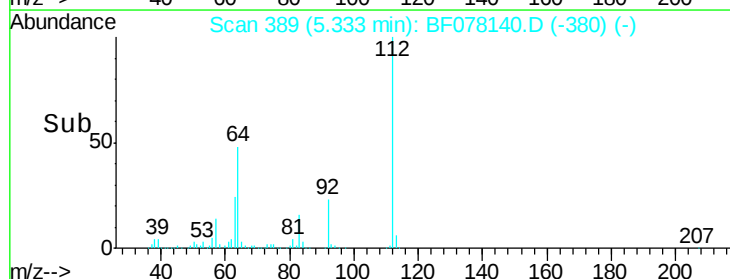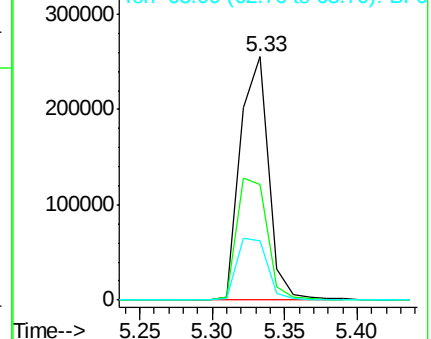



#7

Phenol-d6

Concen: 160.86 ng

RT: 6.64 min Scan# 503

Delta R.T. 0.00 min

Lab File: BF078140.D

Acq: 1 Apr 2015 5:30

Instrument :

BNA_F

ClientSampleId :

S-10(0-10)


Tgt Ion: 99 Resp: 462910

Ion Ratio Lower Upper

99 100

42 14.4 11.0 16.4



71 30.4 23.4 35.2

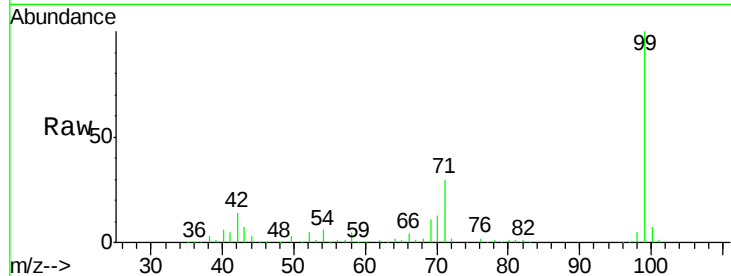

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

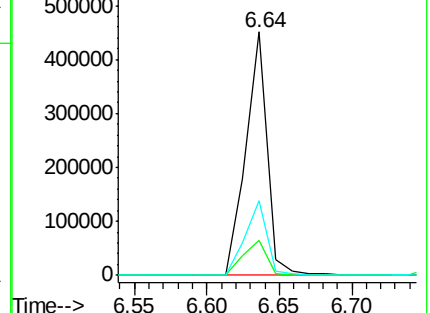

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.62 min Scan# 677

Delta R.T. 0.00 min

Lab File: BF078140.D

Acq: 1 Apr 2015 5:30

Tgt Ion: 136 Resp: 169057


Ion Ratio Lower Upper

136 100

137 10.6 8.7 13.1

54 5.0 4.6 6.8

68 4.7 3.7 5.5


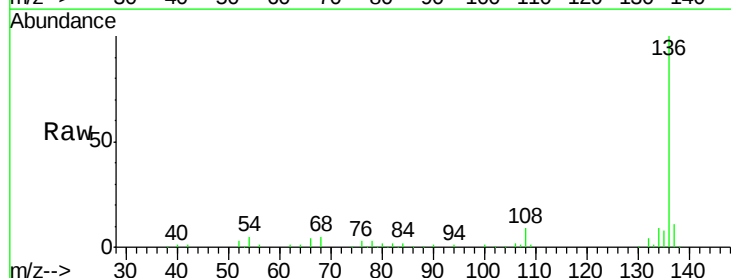



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

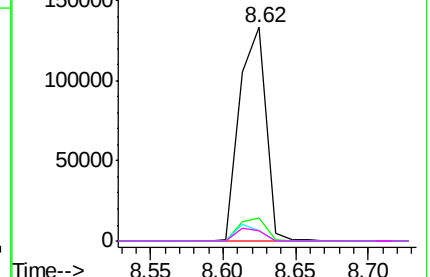







#23
 Nitrobenzene-d5
 Concen: 99.80 ng
 RT: 7.74 min Scan# 600
 Delta R.T. 0.00 min
 Lab File: BF078140.D
 Acq: 1 Apr 2015 5:30

Instrument :
 BNA_F
 ClientSampleId :
 S-10(0-10)

Tgt Ion: 82 Resp: 257377
 Ion Ratio Lower Upper
 82 100
 128 52.9 32.8 49.2#
 54 42.9 40.6 60.8

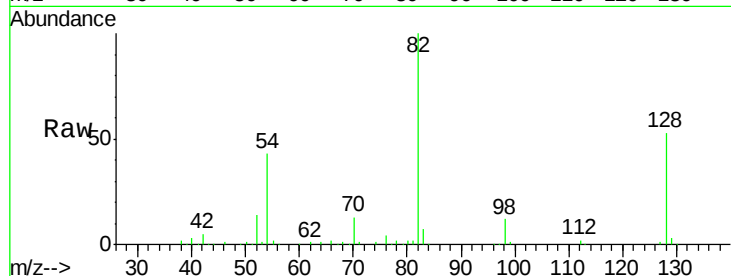


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

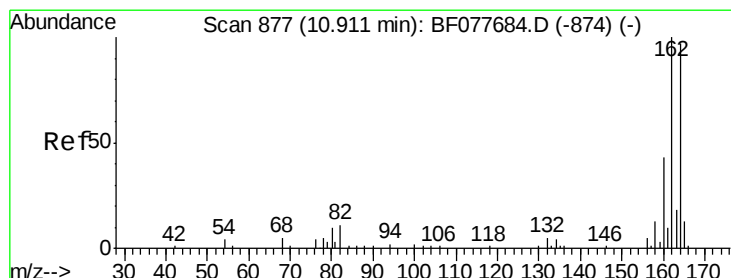
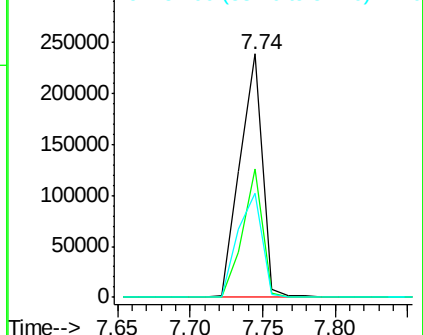


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.79 min Scan# 866
 Delta R.T. 0.00 min
 Lab File: BF078140.D
 Acq: 1 Apr 2015 5:30

Tgt Ion: 164 Resp: 84882
 Ion Ratio Lower Upper
 164 100
 162 102.3 82.4 123.6
 160 44.8 35.8 53.6

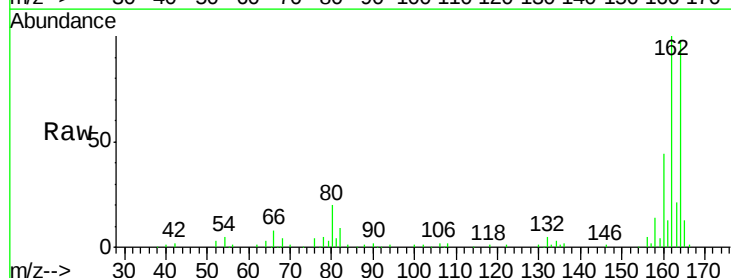

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

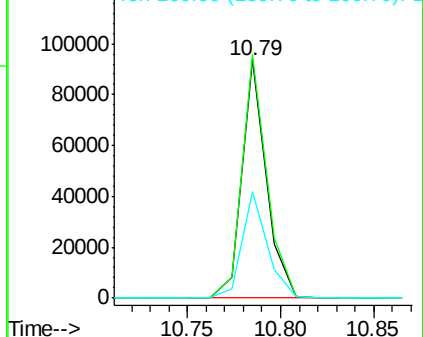




#41
 2,4,6-Tribromophenol
 Concen: 127.34 ng
 RT: 11.77 min Scan# 952
 Delta R.T. 0.00 min
 Lab File: BF078140.D
 Acq: 1 Apr 2015 5:30



Instrument :
 BNA_F
 ClientSampleId :
 S-10(0-10)

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.8	0.0	0.0#
141	37.7	0.0	0.0#

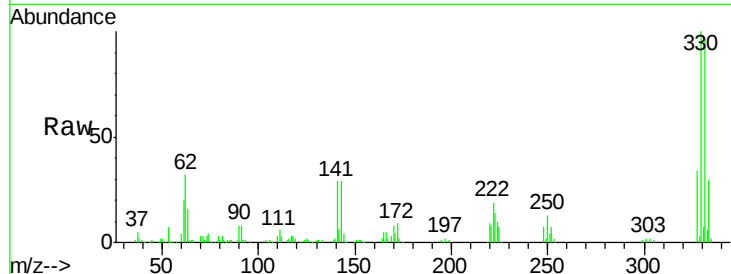


Abundance

Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

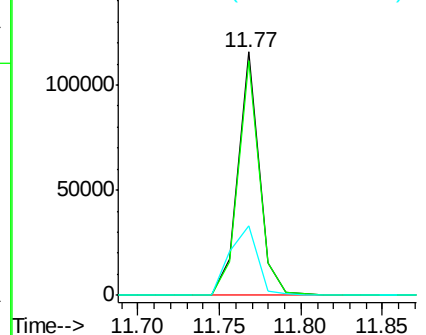



#44
 2-Fluorobiphenyl
 Concen: 86.44 ng
 RT: 9.97 min Scan# 795
 Delta R.T. 0.00 min
 Lab File: BF078140.D
 Acq: 1 Apr 2015 5:30


Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.8	28.5	42.7
170	23.1	18.8	28.2

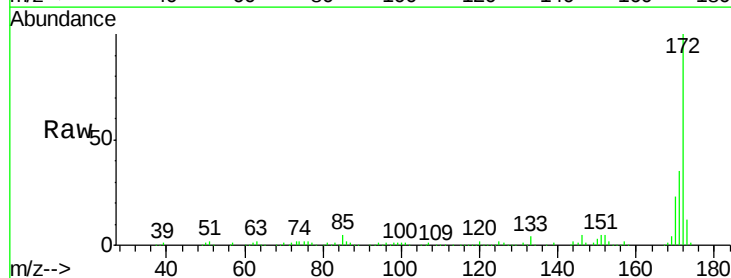

Abundance

Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

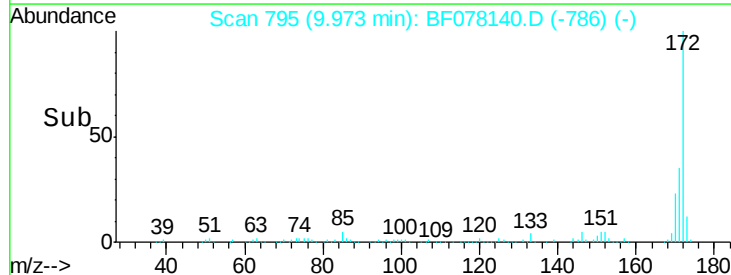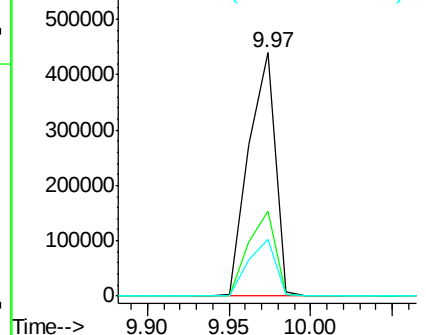

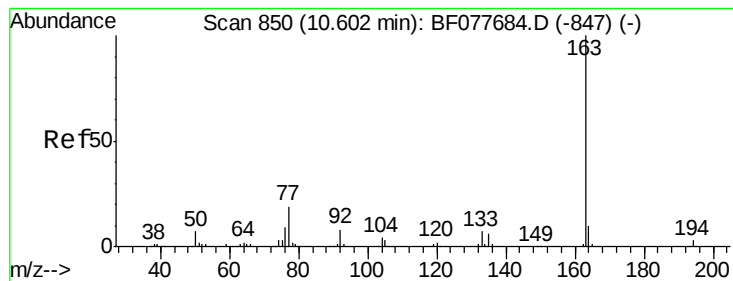

#49

Dimethylphthalate

Concen: 2.07 ng

RT: 10.48 min Scan# 839

Delta R.T. -0.01 min

Lab File: BF078140.D

Acq: 1 Apr 2015 5:30

Instrument :

BNA_F

ClientSampleId :

S-10(0-10)


Tgt Ion:163 Resp: 13009

Ion Ratio Lower Upper

163 100

194 3.9 2.7 4.1




164 11.8 8.2 12.2

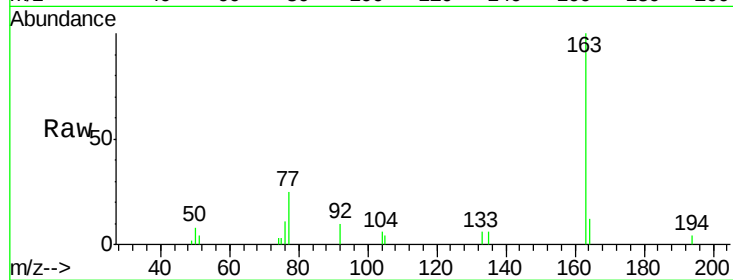

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

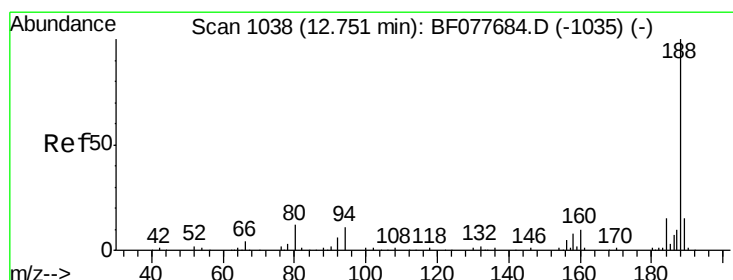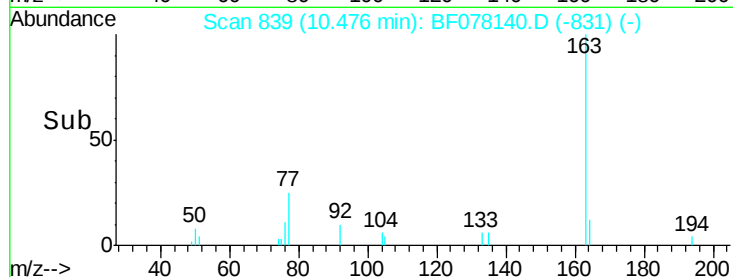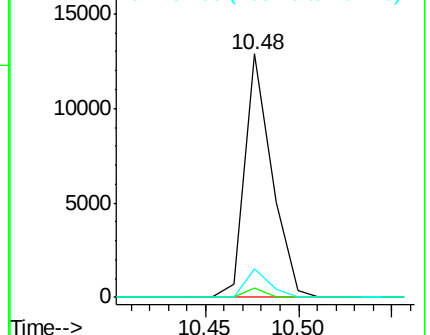

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 12.63 min Scan# 1027

Delta R.T. 0.00 min

Lab File: BF078140.D

Acq: 1 Apr 2015 5:30


Tgt Ion:188 Resp: 171435

Ion Ratio Lower Upper

188 100

94 7.6 8.7 13.1#



80 7.6 9.3 13.9#

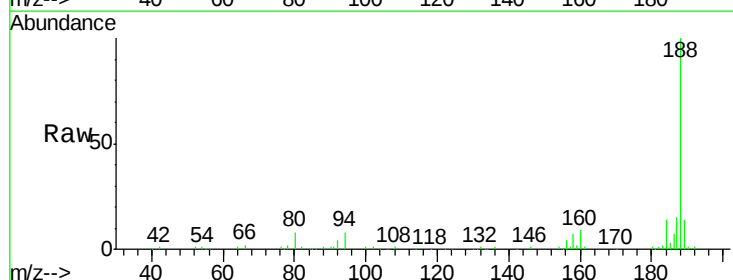


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

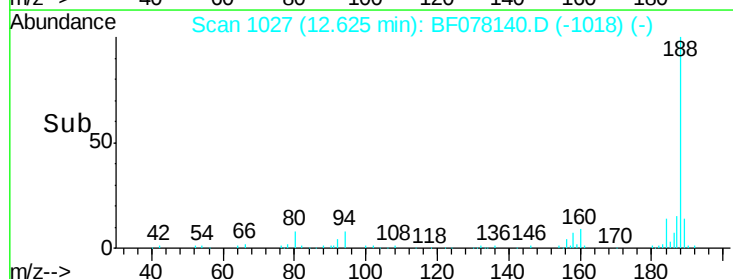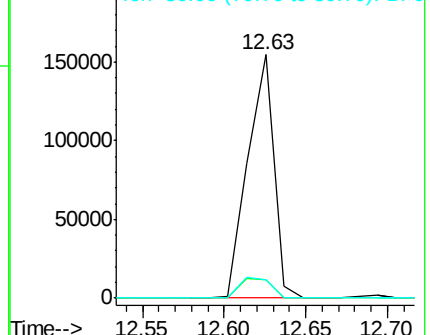

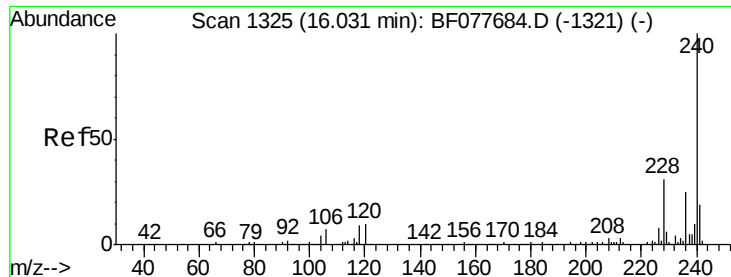

#75

Chrysene-d12

Concen: 20.00 ng

RT: 15.91 min Scan# 1314

Delta R.T. 0.01 min

Lab File: BF078140.D

Acq: 1 Apr 2015 5:30

Instrument :

BNA_F

ClientSampleId :

S-10(0-10)


Tgt Ion:240 Resp: 169491

Ion Ratio Lower Upper

240 100

120 10.1 8.2 12.2




236 24.8 20.0 30.0

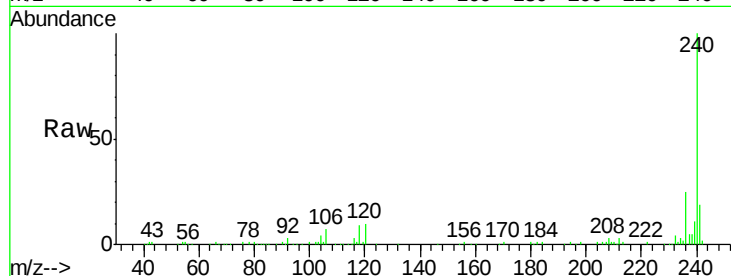

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

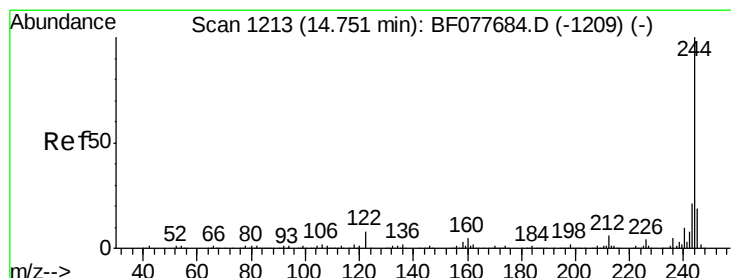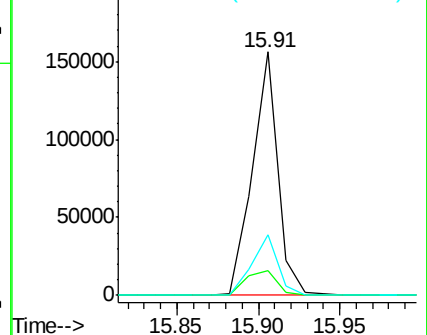

#78

Terphenyl-d14

Concen: 83.05 ng

RT: 14.61 min Scan# 1201

Delta R.T. 0.00 min

Lab File: BF078140.D

Acq: 1 Apr 2015 5:30


Tgt Ion:244 Resp: 576247

Ion Ratio Lower Upper

244 100

212 7.1 4.9 7.3



122 14.9 6.2 9.4#

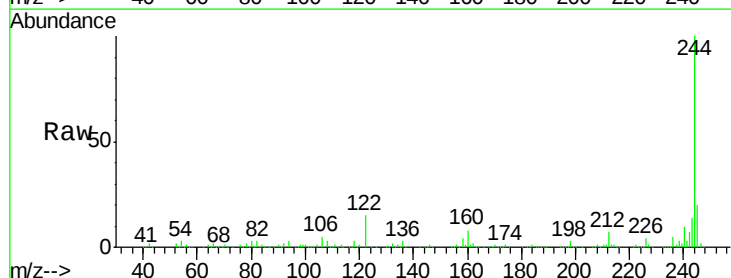


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

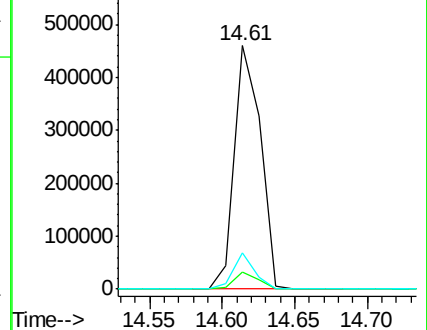



#79

Butylbenzylphthalate

Concen: 2.33 ng

RT: 15.24 min Scan# 1256

Delta R.T. 0.00 min

Lab File: BF078140.D

Acq: 1 Apr 2015 5:30

Instrument :

BNA_F

ClientSampleId :

S-10(0-10)


Tgt Ion:149 Resp: 9777

Ion Ratio Lower Upper

149 100

91 58.6 50.1 75.1




206 20.9 16.2 24.2

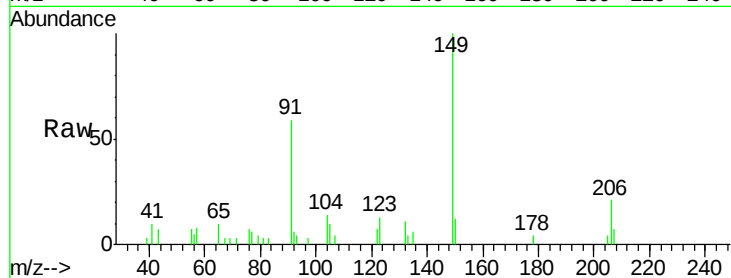

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 91.00 (90.70 to 91.70): BF0

Ion 206.00 (205.70 to 206.70): E

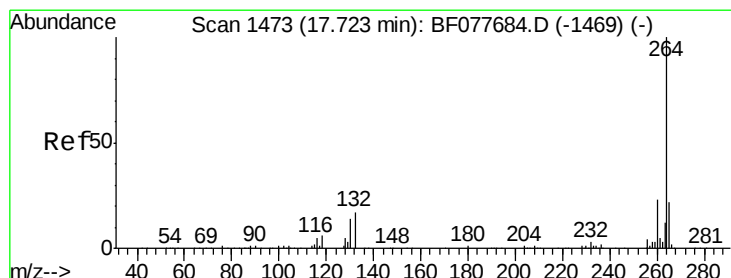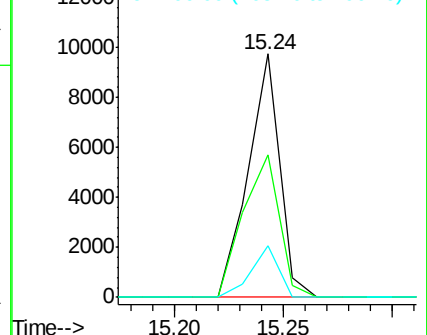

#86

Perylene-d12

Concen: 20.00 ng

RT: 17.67 min Scan# 1468

Delta R.T. 0.06 min

Lab File: BF078140.D

Acq: 1 Apr 2015 5:30


Tgt Ion:264 Resp: 158161

Ion Ratio Lower Upper

264 100

260 23.3 18.6 27.8

265 20.9 17.3 25.9

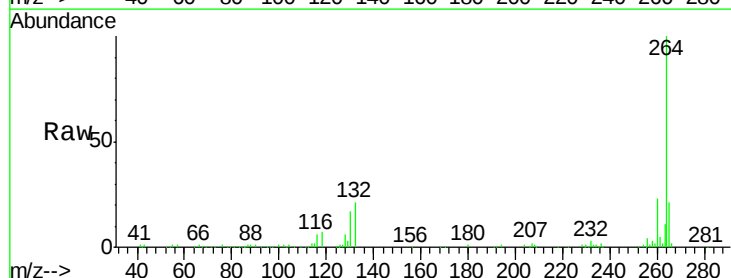

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

