


Data Path : Z:\HPCHEM1\BNA_F\Data\BF033115\
 Data File : BF078108.D
 Acq On : 31 Mar 2015 11:20
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 31 14:58:34 2015

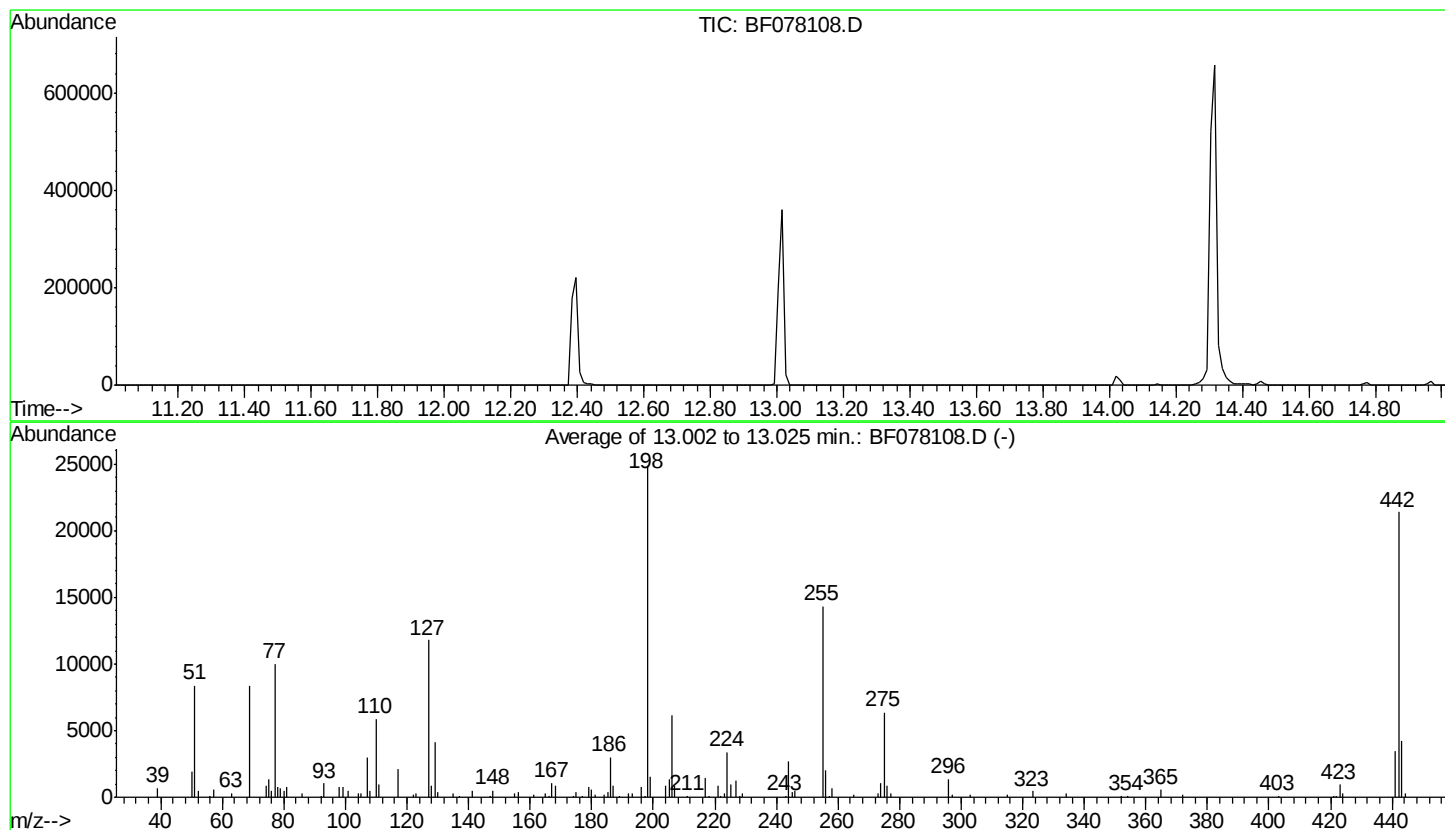

AutoFind: Scans 1060, 1061, 1062; Background Corrected with Scan 1056

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	8363	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.5	8341	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.4	11783	PASS
197	198	0.00	2	0.6	138	PASS
198	198	100	100	100.0	24880	PASS
199	198	5	9	6.1	1522	PASS
275	198	10	60	25.6	6364	PASS
365	198	1	100	2.3	565	PASS
441	442	0.01	24	16.0	3413	PASS
442	198	50	100	86.0	21385	PASS
443	442	15	24	19.6	4202	PASS