
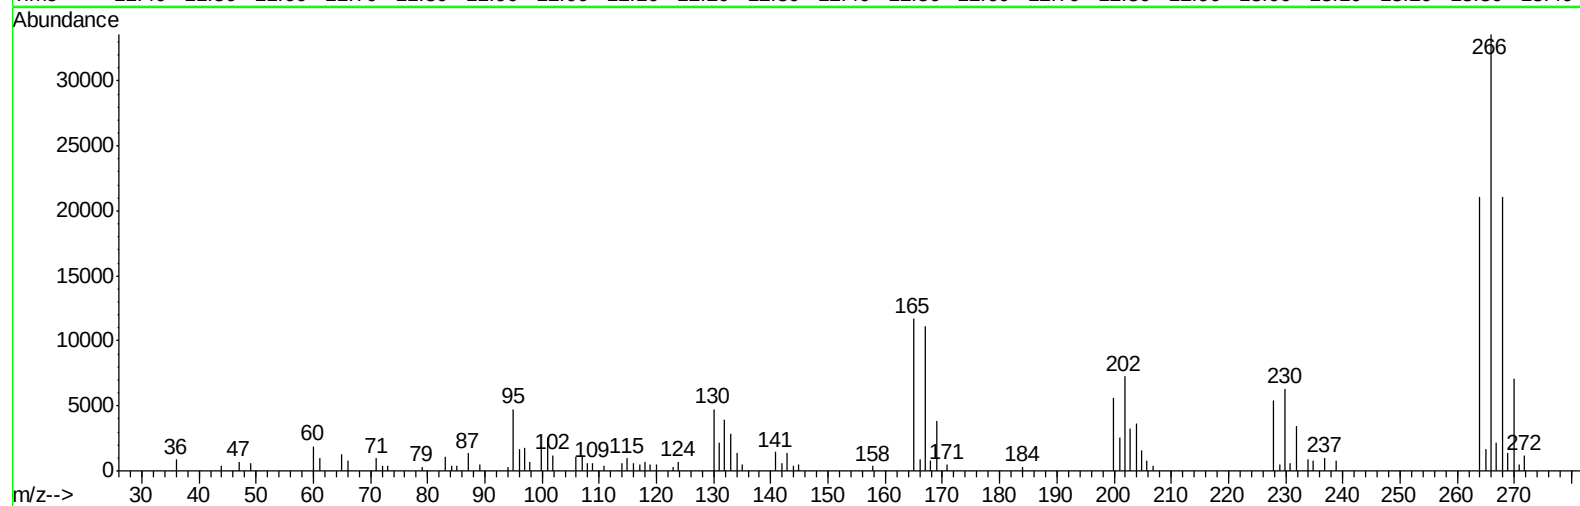


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033115\
Data File : BF078108.D
Acq On : 31 Mar 2015 11:20
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 07:15:14 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 01 00:51:03 2015
Response via : Initial Calibration

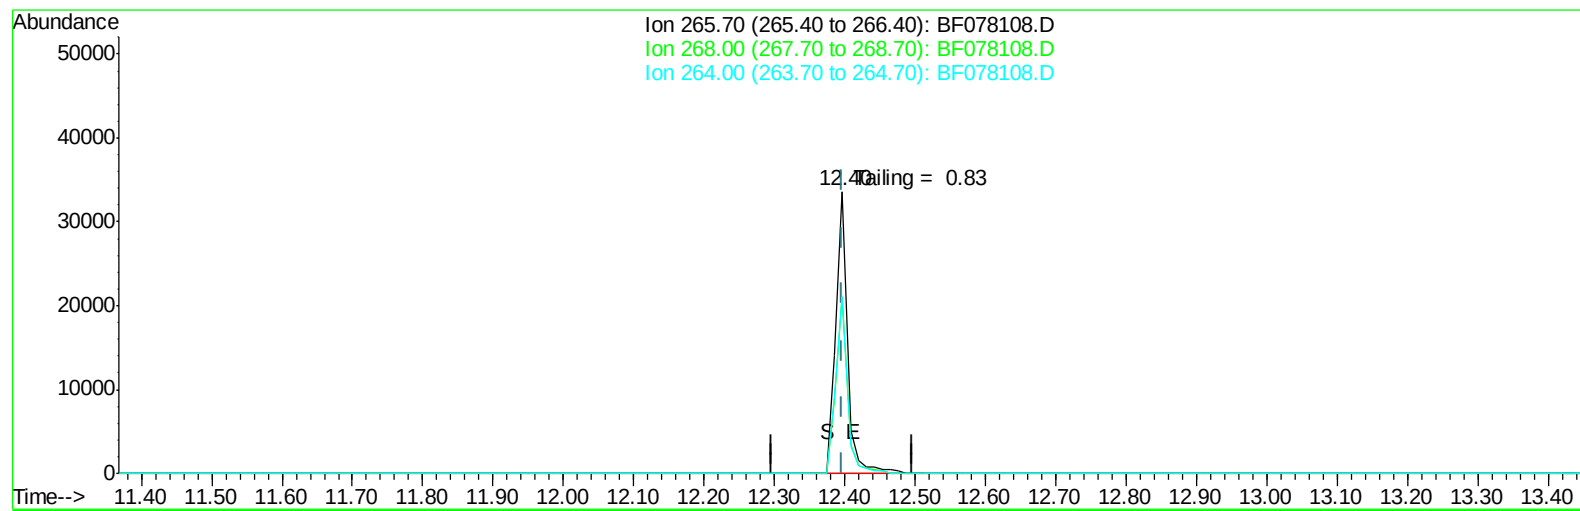

TIC: BF078108.D

(69) Pentachlorophenol (C)



12.397min (+0.000) 0.00ng

response 38455

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.81
264.00	61.20	62.76
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF033115\
Data File : BF078108.D
Acq On : 31 Mar 2015 11:20
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 07:15:14 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 01 00:51:03 2015
Response via : Initial Calibration

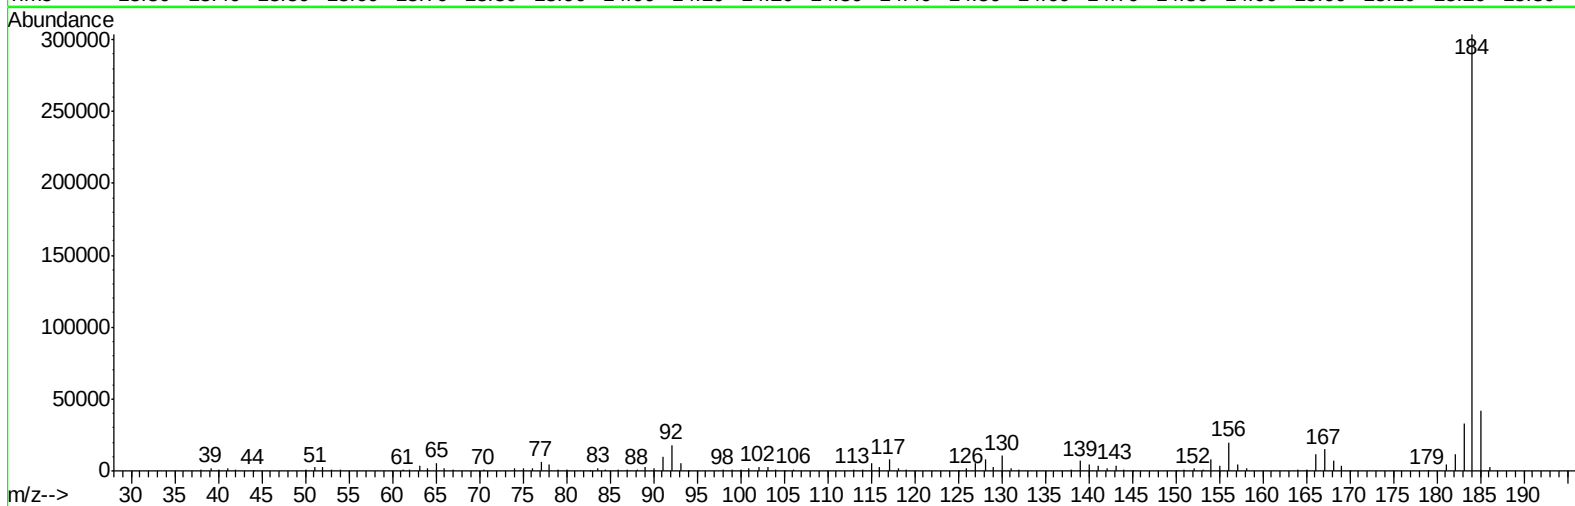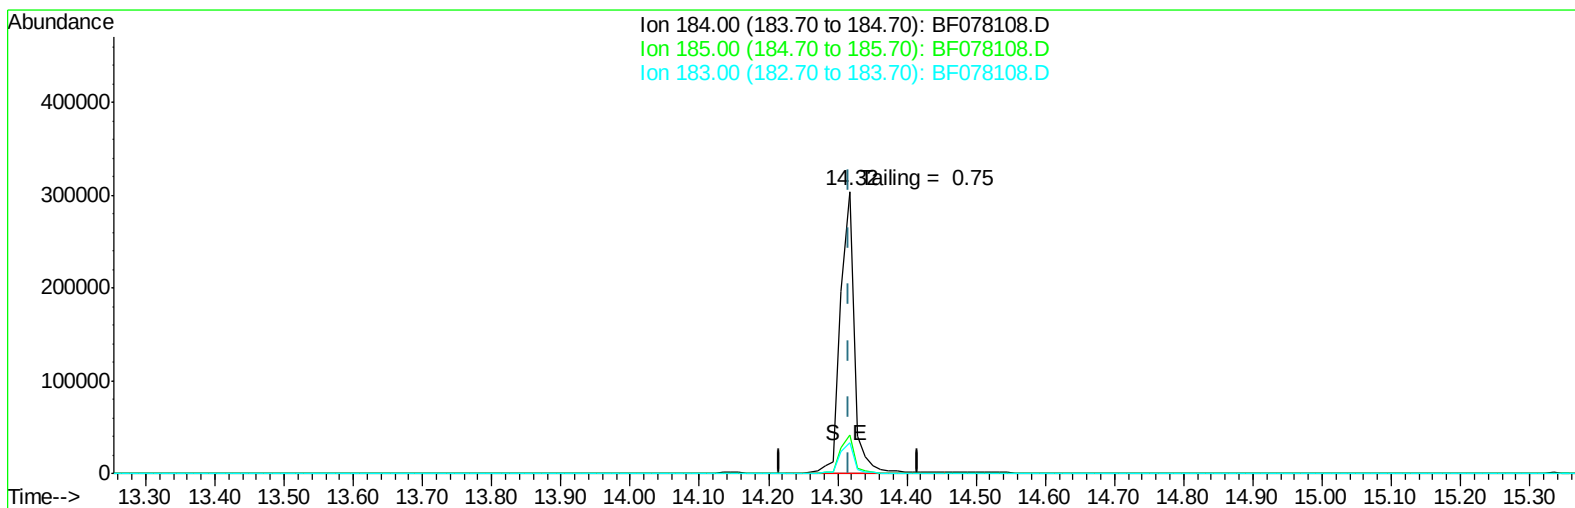

TIC: BF078108.D

(76) Benzidine

14.317min (+0.000) 0.00ng

response 405610

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.87
183.00	11.10	11.00
0.00	0.00	0.00